


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082316\
 Data File : BF089820.D
 Acq On : 23 Aug 2016 8:35
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 19 14:02:57 2016

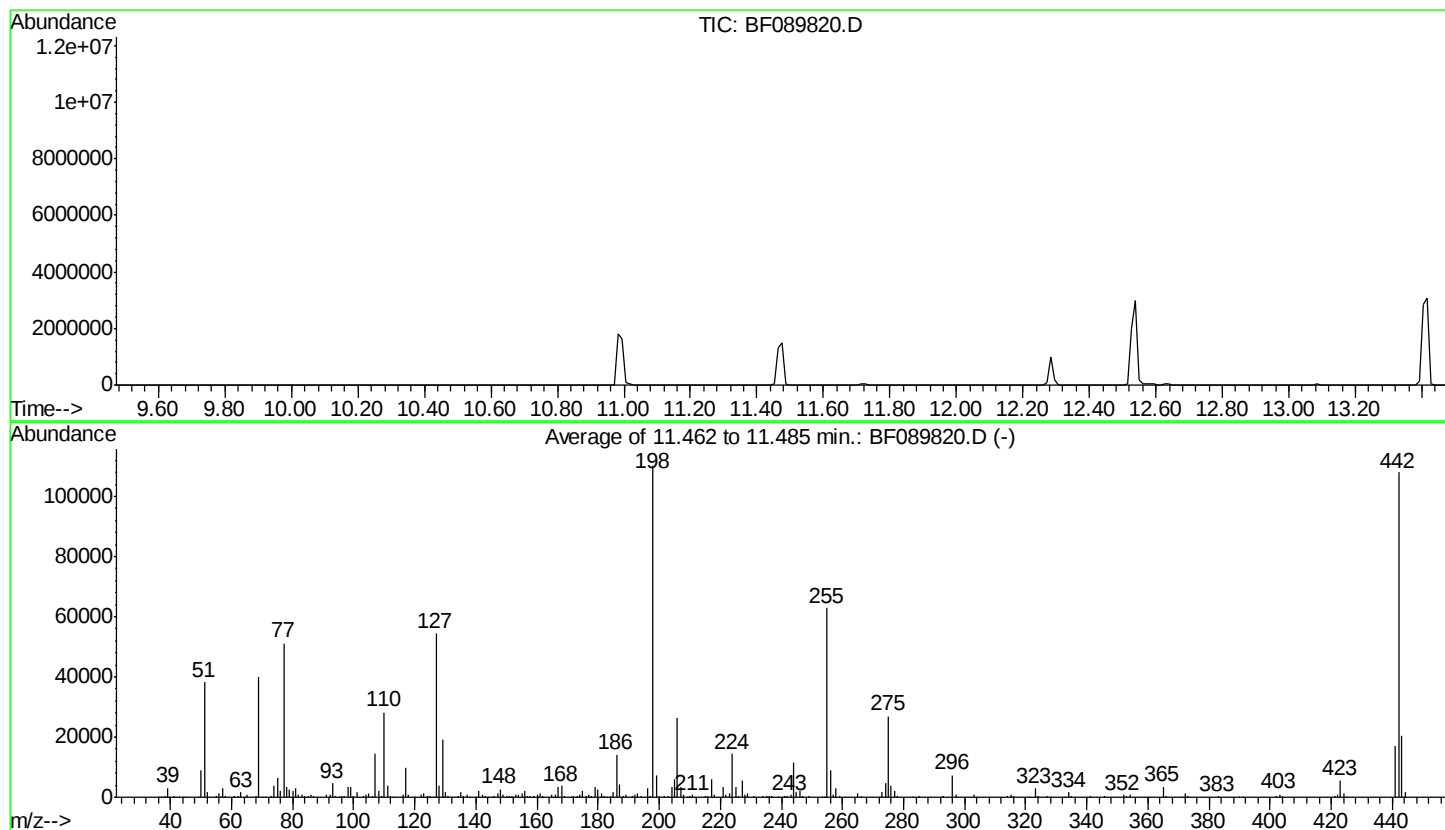

AutoFind: Scans 864, 865, 866; Background Corrected with Scan 860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	38195	PASS
68	69	0.00	2	1.6	637	PASS
69	198	0.00	100	36.5	40220	PASS
70	69	0.00	2	0.5	204	PASS
127	198	10	80	49.4	54434	PASS
197	198	0.00	2	0.4	448	PASS
198	198	100	100	100.0	110250	PASS
199	198	5	9	6.5	7208	PASS
275	198	10	60	24.5	27029	PASS
365	198	1	100	3.2	3502	PASS
441	442	0.01	24	16.0	17247	PASS
442	198	50	100	98.0	108050	PASS
443	442	15	24	19.1	20646	PASS