


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082316\
 Data File : BF089847.D
 Acq On : 23 Aug 2016 22:56
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 19 14:02:57 2016

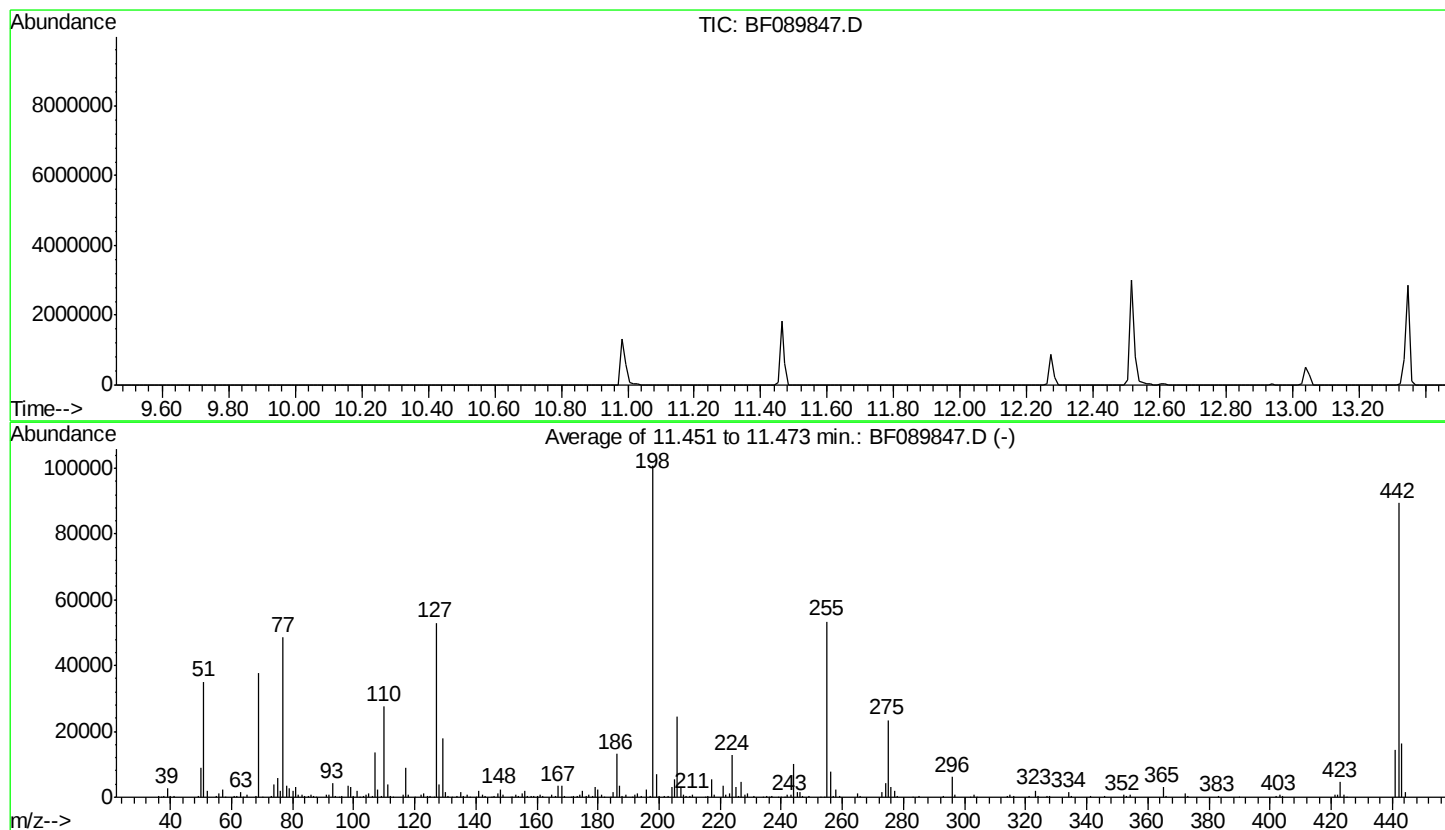

AutoFind: Scans 863, 864, 865; Background Corrected with Scan 860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	35201	PASS
68	69	0.00	2	1.3	497	PASS
69	198	0.00	100	37.4	37656	PASS
70	69	0.00	2	0.5	194	PASS
127	198	10	80	52.7	53100	PASS
197	198	0.00	2	0.4	400	PASS
198	198	100	100	100.0	100759	PASS
199	198	5	9	7.0	7061	PASS
275	198	10	60	23.3	23521	PASS
365	198	1	100	2.9	2946	PASS
441	442	0.01	24	16.0	14311	PASS
442	198	50	100	88.7	89397	PASS
443	442	15	24	18.3	16392	PASS