

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082317\
 Data File : BF097992.D
 Acq On : 23 Aug 2017 12:29
 Operator : SJ/JU
 Sample : I4914-04
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 165-COMP

Quant Time: Aug 23 17:54:07 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 21 15:59:04 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	134133	20.00	ng	-0.01
21) Naphthalene-d8	8.02	136	526703	20.00	ng	-0.01
38) Acenaphthene-d10	9.77	164	232610	20.00	ng	-0.01
63) Phenanthrene-d10	11.25	188	445215	20.00	ng	-0.01
75) Chrysene-d12	13.89	240	292045	20.00	ng	-0.01
86) Perylene-d12	15.30	264	238690	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.35	112	650118	73.72	ng	0.00
7) Phenol-d6	6.37	99	977887	81.62	ng	-0.01
23) Nitrobenzene-d5	7.30	82	625251	64.49	ng	-0.02
41) 2,4,6-Tribromophenol	10.56	330	180820	89.59	ng	-0.01
44) 2-Fluorobiphenyl	9.10	172	1082707	68.39	ng	-0.01
78) Terphenyl-d14	12.84	244	1055566	75.37	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.49	163	70842	4.166	ng	100
83) Bis(2-ethylhexyl)phthalate	13.87	149	214362	21.124	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082317\
Data File : BF097992.D
Acq On : 23 Aug 2017 12:29
Operator : SJ/JU
Sample : I4914-04
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
165-COMP

Quant Time: Aug 23 17:54:07 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

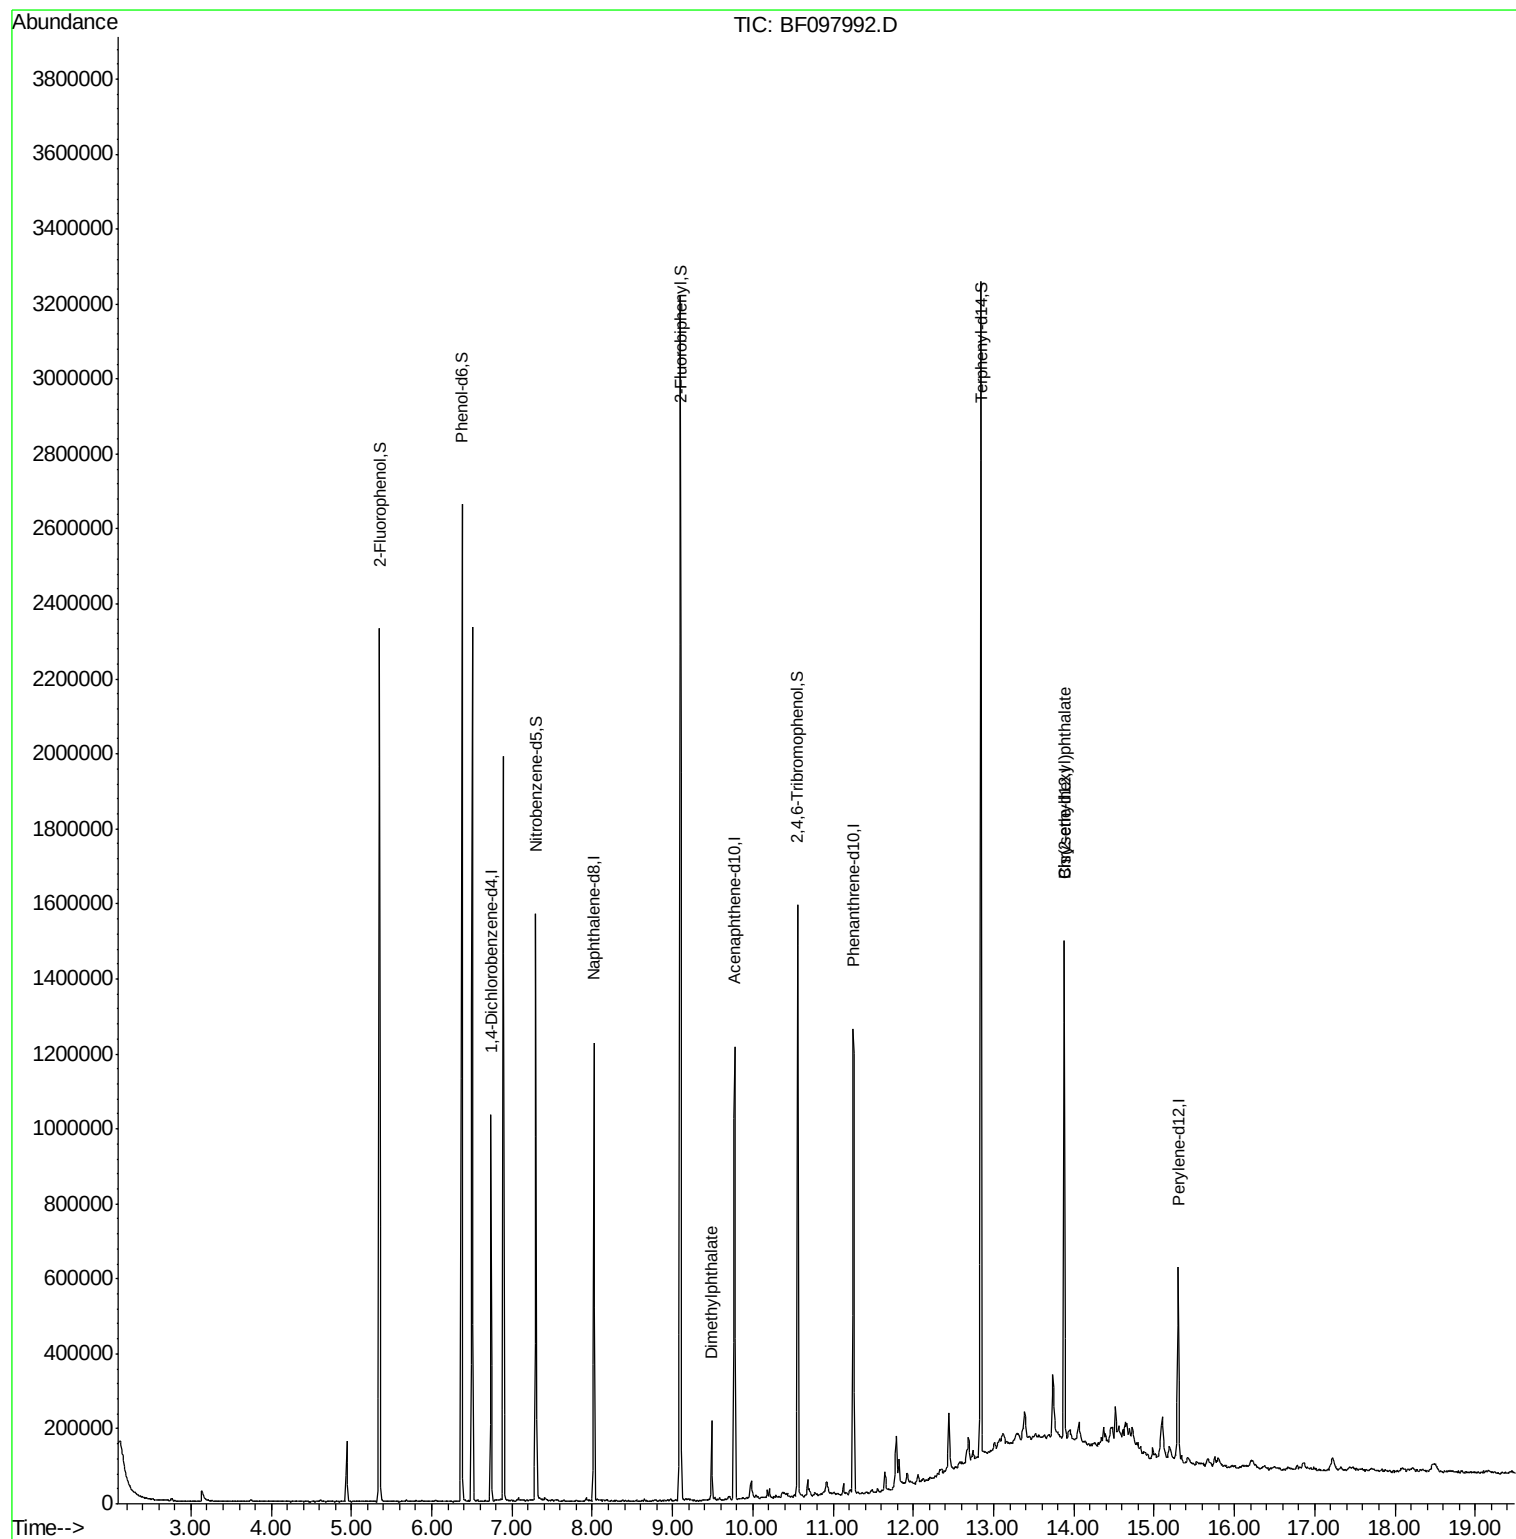




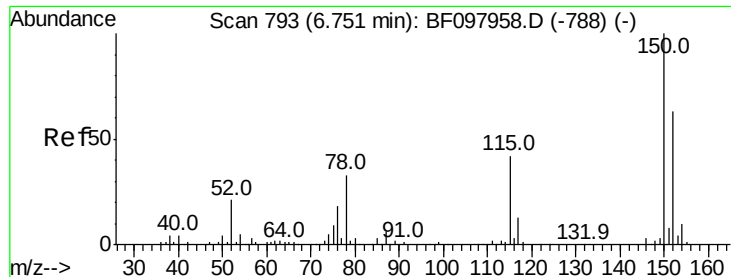


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.74 min Scan# 791
Delta R.T. -0.01 min
Lab File: BF097992.D
Acq: 23 Aug 2017 12:29

Instrument :
BNA_F
ClientSampleId :
165-COMP




Tot Ion	Ratio	Lower	Upper
152	100		
150	158.3	126.2	189.2
115	66.0	52.2	78.2

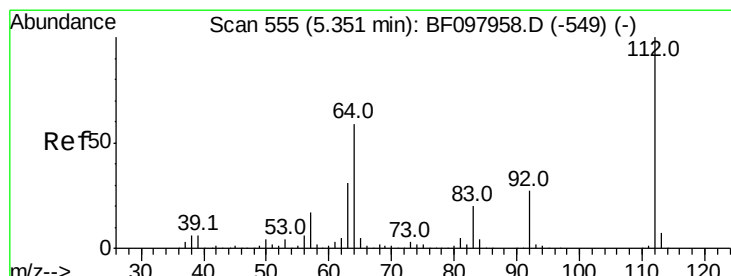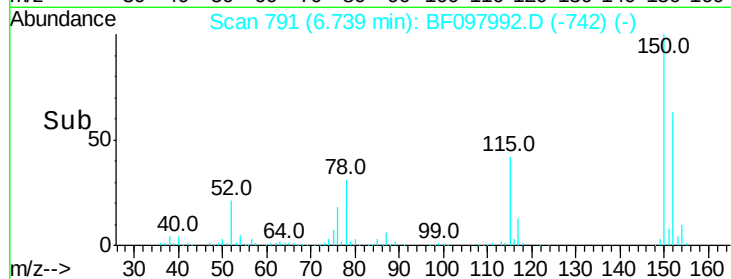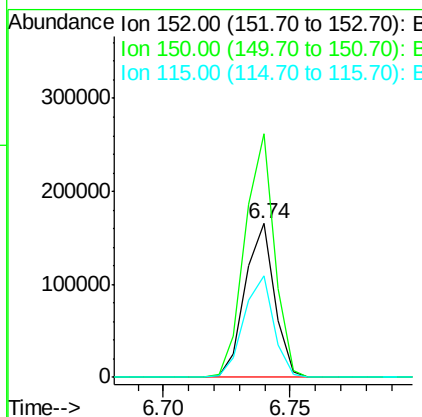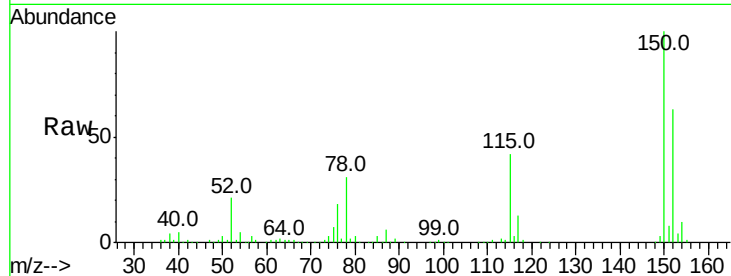


#5

2-Fluorophenol
Concen: 73.724 ng
RT: 5.35 min Scan# 555
Delta R.T. 0.00 min
Lab File: BF097992.D
Acq: 23 Aug 2017 12:29

Tgt Ion	Ratio	Lower	Upper
112	100		
64	57.5	46.0	69.0
63	29.8	23.4	35.0

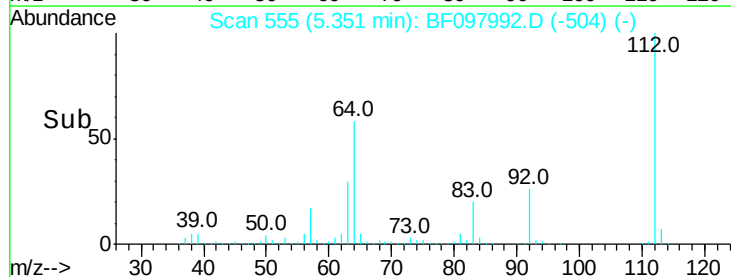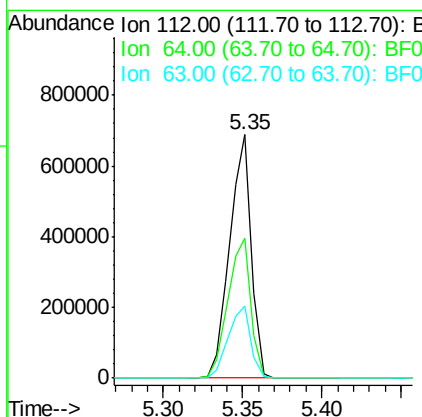

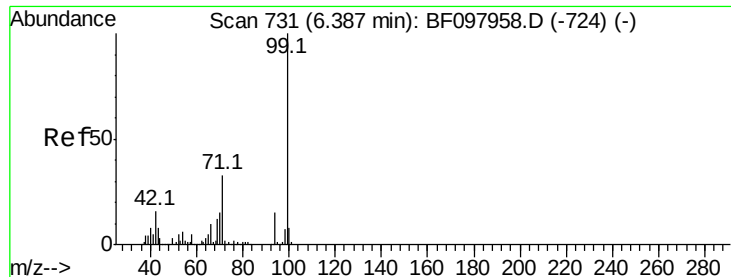

#7

Phenol-d6

Concen: 81.616 ng

RT: 6.37 min Scan# 729

Delta R.T. -0.01 min

Lab File: BF097992.D

Acq: 23 Aug 2017 12:29

Instrument :

BNA_F

ClientSampled :

165-COMP


Tot Ion: 99 Resp: 977887

Ion Ratio Lower Upper

99 100

42 15.7 13.5 20.3




71 32.8 24.5 36.7

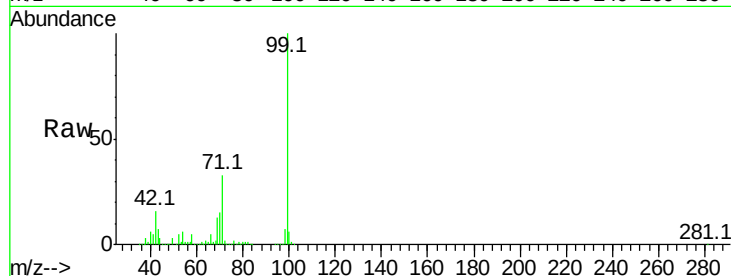

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

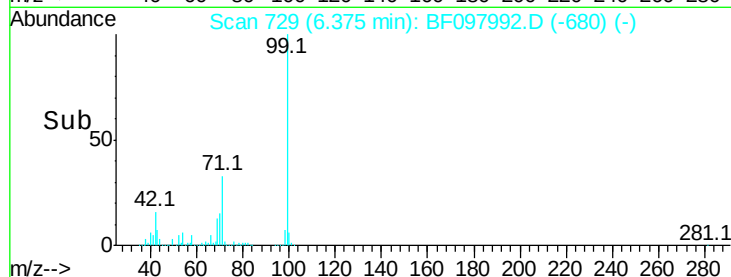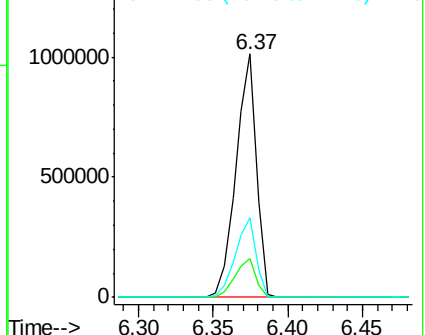

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.02 min Scan# 1009

Delta R.T. -0.01 min

Lab File: BF097992.D

Acq: 23 Aug 2017 12:29

Tgt Ion: 136 Resp: 526703


Ion Ratio Lower Upper

136 100

137 11.1 8.5 12.7

54 7.5 4.9 7.3#

68 6.8 4.1 6.1#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



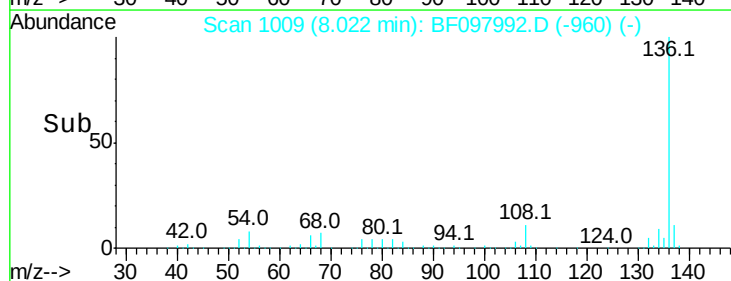
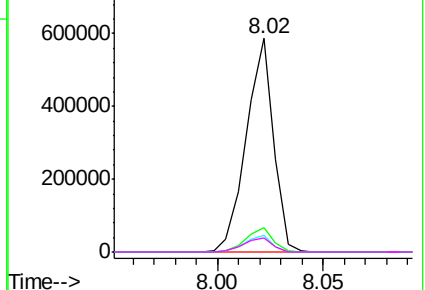


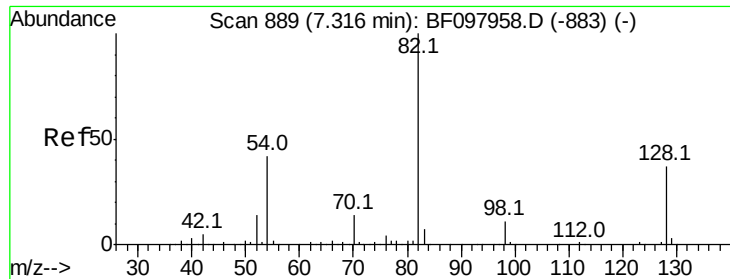

#23
 Nitrobenzene-d5
 Concen: 64.489 ng
 RT: 7.30 min Scan# 886
 Delta R.T. -0.02 min
 Lab File: BF097992.D
 Acq: 23 Aug 2017 12:29




Instrument :
 BNA_F
 ClientSampleId :
 165-COMP


Tot Ion	82	Resp	625251
Ion Ratio	Lower	Upper	
82	100		
128	37.0	34.0	51.0
54	42.8	42.2	63.2

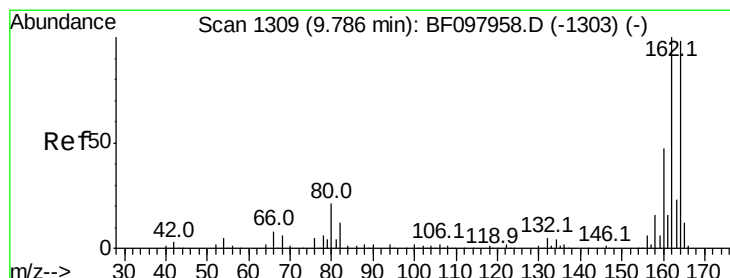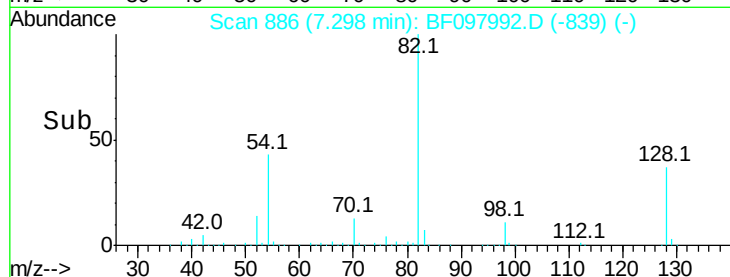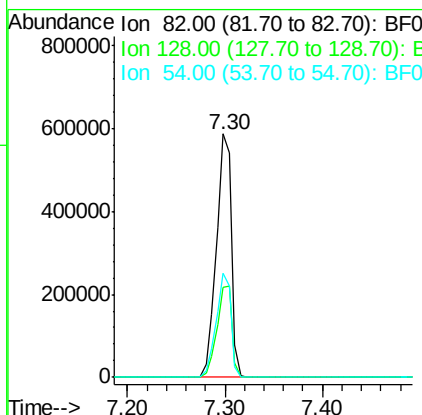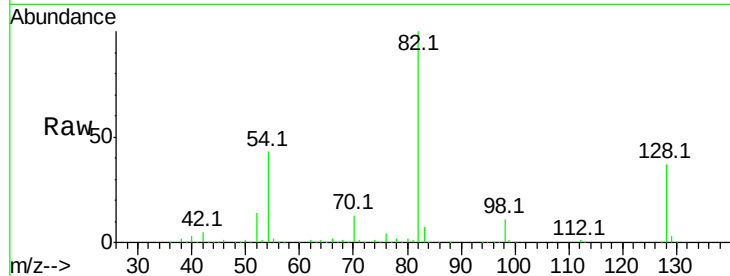

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.77 min Scan# 1307
 Delta R.T. -0.01 min
 Lab File: BF097992.D
 Acq: 23 Aug 2017 12:29

Tgt Ion	164	Resp	232610
Ion Ratio	Lower	Upper	
164	100		
162	103.7	82.6	123.8
160	49.2	36.2	54.2

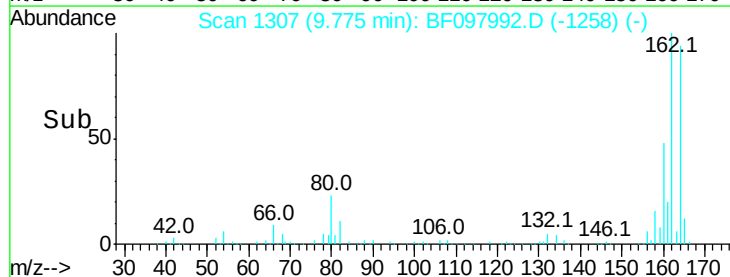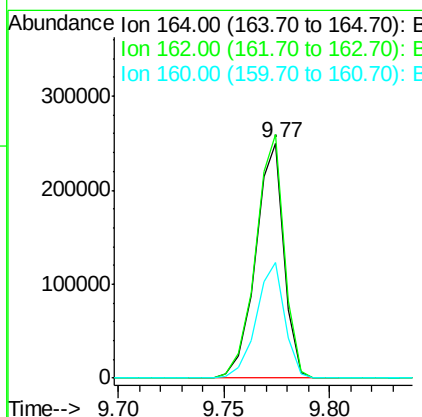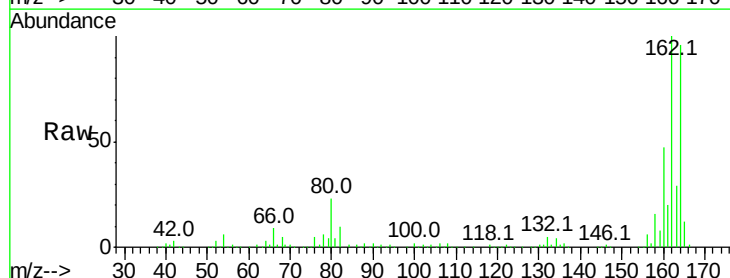


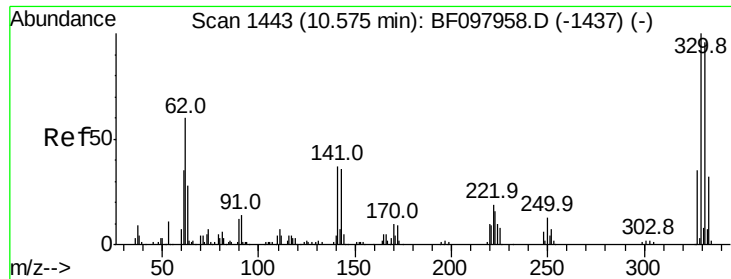




#41
 2,4,6-Tribromophenol
 Concen: 89.592 ng
 RT: 10.56 min Scan# 1441
 Delta R.T. -0.01 min
 Lab File: BF097992.D
 Acq: 23 Aug 2017 12:29

Instrument :
 BNA_F
 ClientSampleId :
 165-COMP

Tot Ion	Ratio	Lower	Upper
330	100		
332	93.5	76.6	115.0
141	39.0	31.4	47.2




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

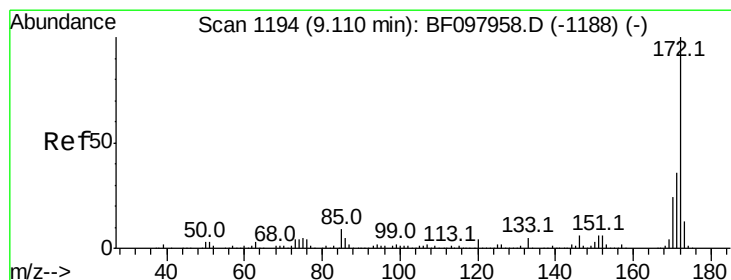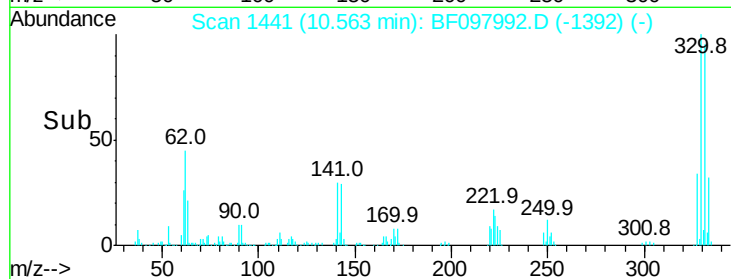
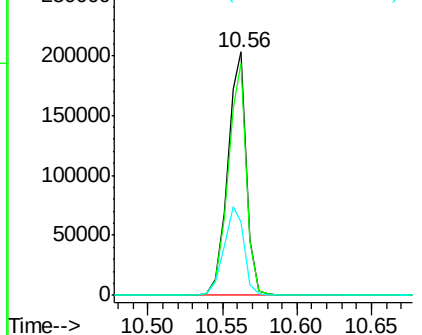



#44
 2-Fluorobiphenyl
 Concen: 68.386 ng
 RT: 9.10 min Scan# 1192
 Delta R.T. -0.01 min
 Lab File: BF097992.D
 Acq: 23 Aug 2017 12:29

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.3	29.6	44.4
170	24.9	19.8	29.8

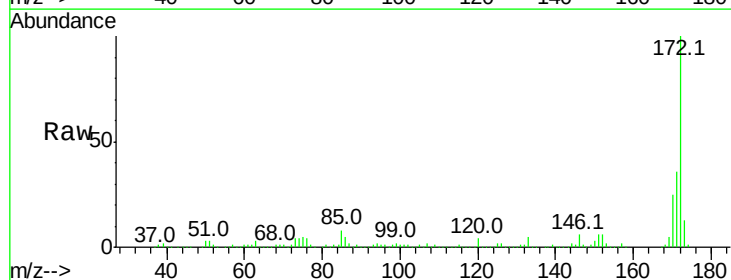

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

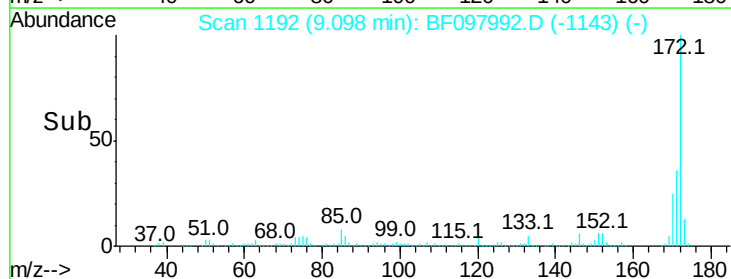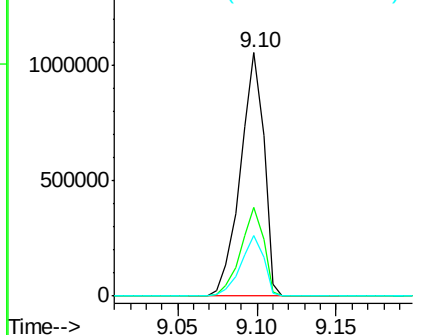

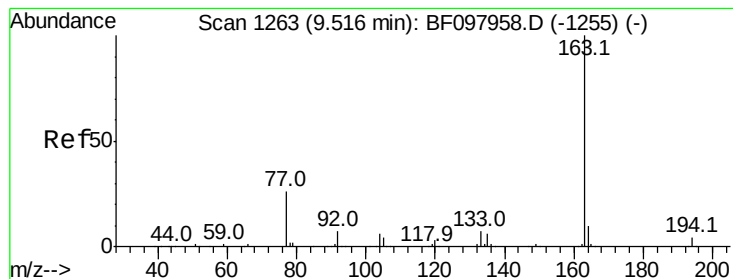

#49

Dimethylphthalate

Concen: 4.166 ng

RT: 9.49 min Scan# 1259

Delta R.T. -0.02 min

Lab File: BF097992.D

Acq: 23 Aug 2017 12:29

Instrument :

BNA_F

ClientSampleId :

165-COMP


Tot Ion:163 Resp: 70842

Ion Ratio Lower Upper

163 100

194 3.6 2.6 4.0




164 10.5 8.4 12.6

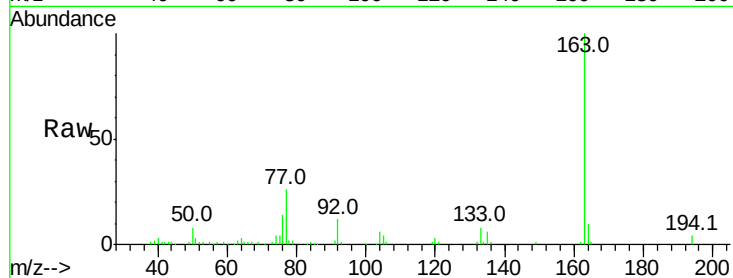

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

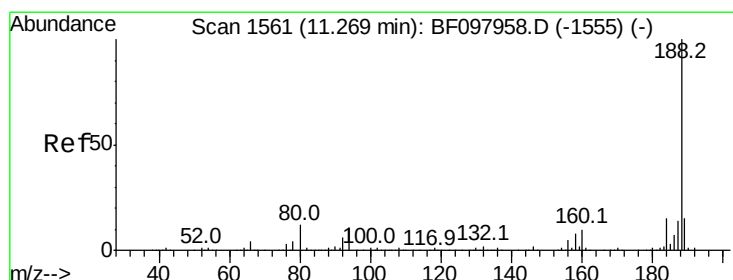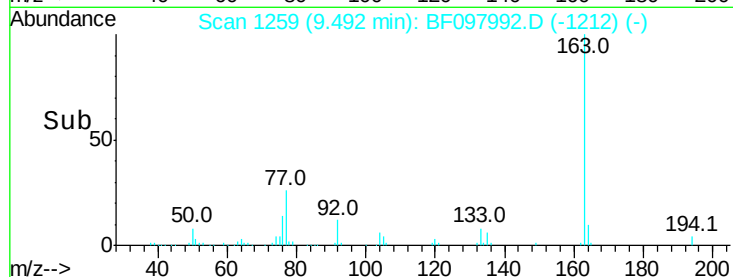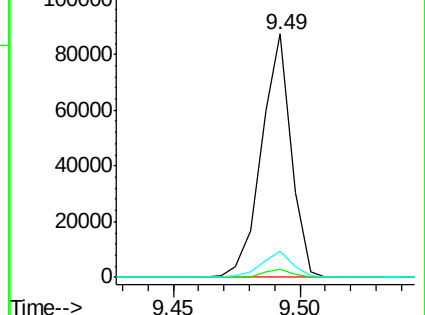

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.25 min Scan# 1558

Delta R.T. -0.01 min

Lab File: BF097992.D

Acq: 23 Aug 2017 12:29


Tgt Ion:188 Resp: 445215

Ion Ratio Lower Upper

188 100

94 12.2 9.4 14.2



80 13.5 10.2 15.2

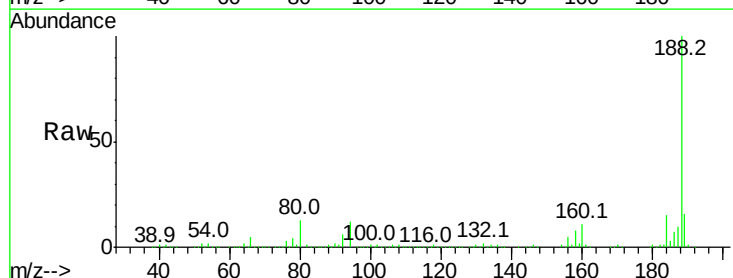


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

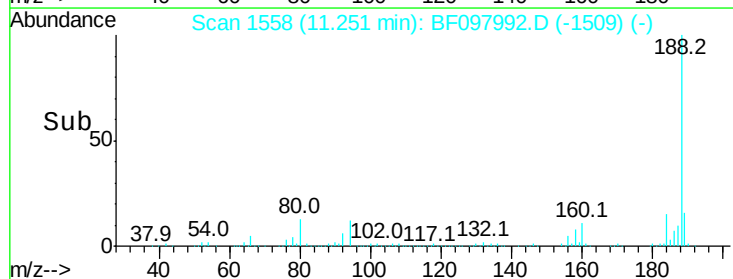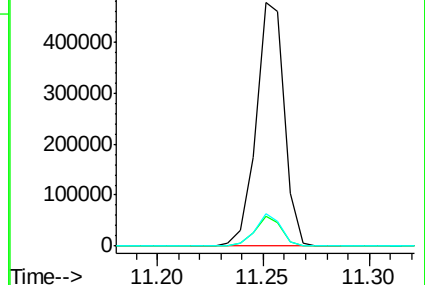

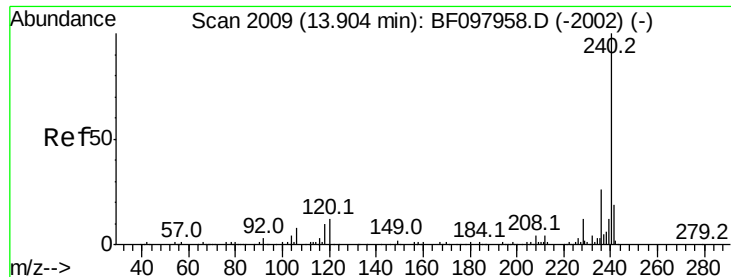

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.89 min Scan# 2006

Delta R.T. -0.01 min

Lab File: BF097992.D

Acq: 23 Aug 2017 12:29

Instrument :

BNA_F

ClientSampleId :

165-COMP


Tot Ion:240 Resp: 292045

Ion Ratio Lower Upper

240 100

120 11.1 5.8 8.8#




236 26.1 20.5 30.7



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

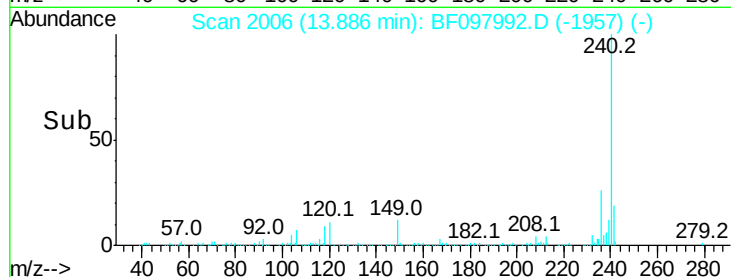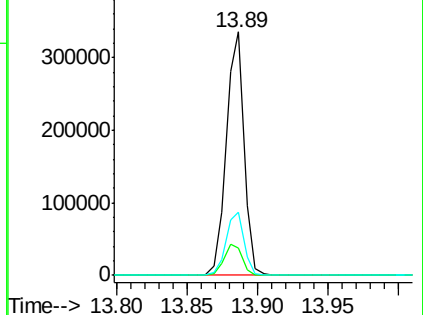

#78

Terphenyl-d14

Concen: 75.372 ng

RT: 12.84 min Scan# 1829

Delta R.T. -0.01 min

Lab File: BF097992.D

Acq: 23 Aug 2017 12:29


Tgt Ion:244 Resp: 1055566

Ion Ratio Lower Upper

244 100

212 7.3 6.0 9.0



122 12.3 10.3 15.5




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

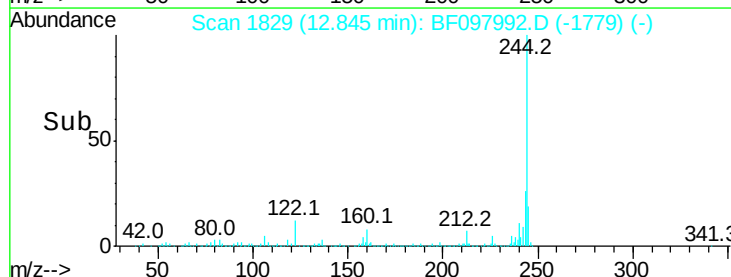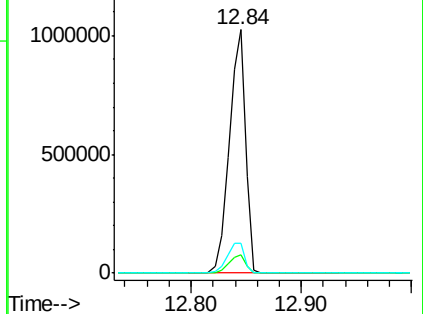

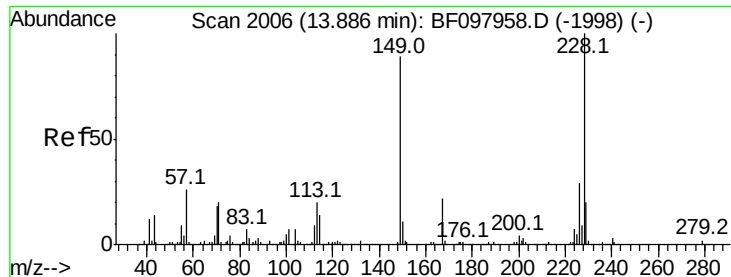

#83

Bis(2-ethylhexyl)phthalate

Concen: 21.124 ng

RT: 13.87 min Scan# 2004

Delta R.T. -0.01 min

Lab File: BF097992.D

Acq: 23 Aug 2017 12:29

Instrument :

BNA_F

ClientSampleId :

165-COMP


Tot Ion:149 Resp: 214362

Ion Ratio Lower Upper

149 100

167 24.4 21.0 31.4




279 2.5 1.9 2.9



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

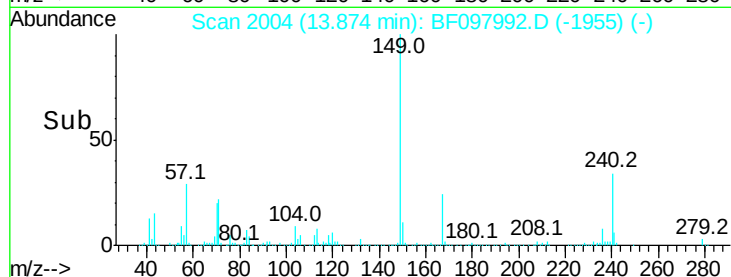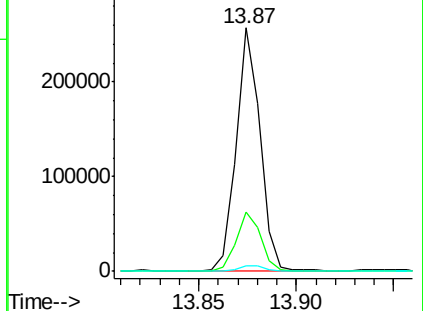

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.30 min Scan# 2246

Delta R.T. -0.01 min

Lab File: BF097992.D

Acq: 23 Aug 2017 12:29


Tgt Ion:264 Resp: 238690

Ion Ratio Lower Upper

264 100

260 23.9 19.5 29.3

265 21.6 17.2 25.8



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

