


Data Path : Z:\HPCHEM1\BNA F\Data\BF082317\
 Data File : BF097990.D
 Acq On : 23 Aug 2017 11:29
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 21 15:59:04 2017

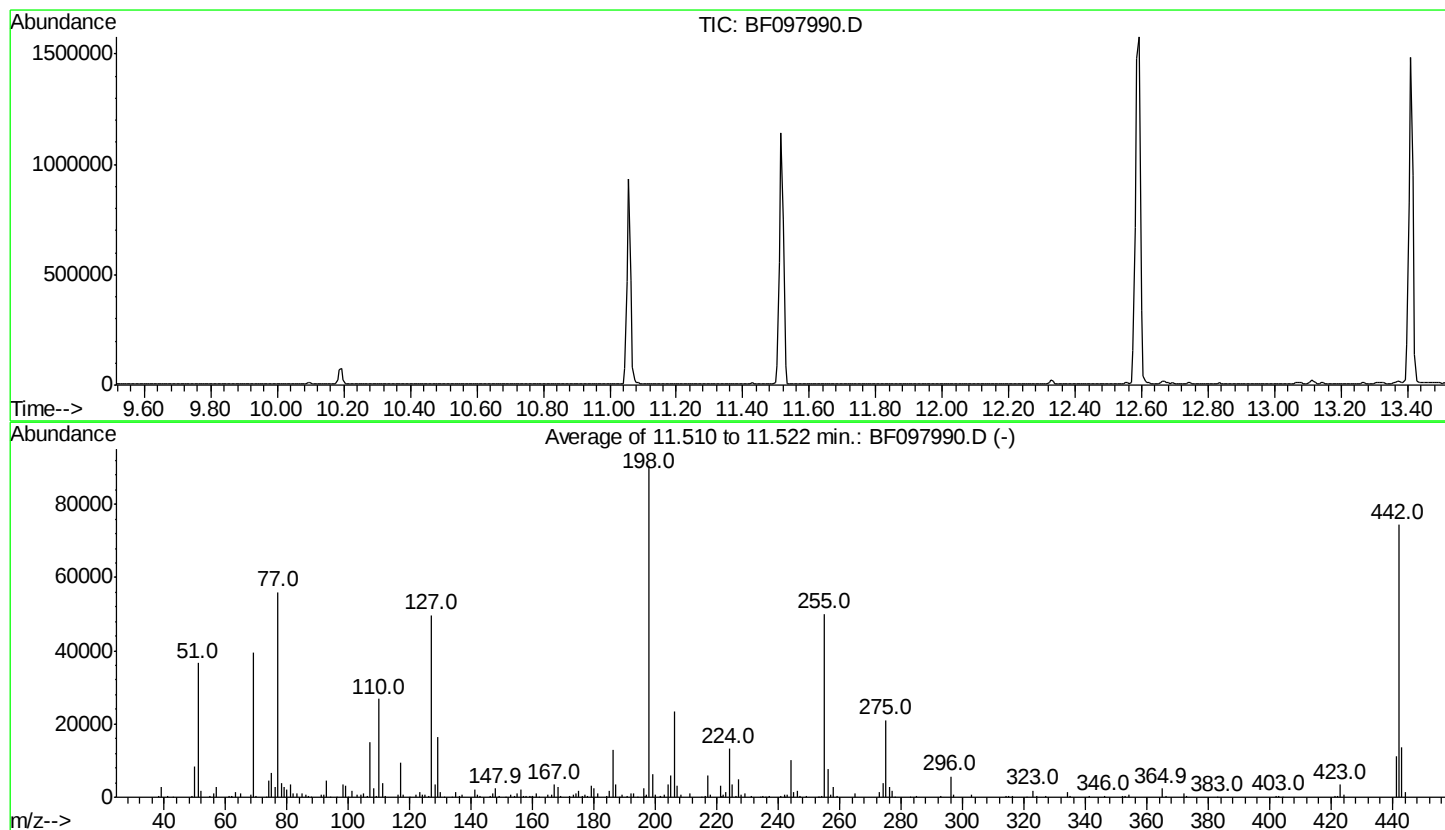

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	36597	PASS
68	69	0.00	2	1.9	755	PASS
69	198	0.00	100	43.5	39378	PASS
70	69	0.00	2	0.7	256	PASS
127	198	10	80	54.8	49648	PASS
197	198	0.00	2	0.9	797	PASS
198	198	100	100	100.0	90552	PASS
199	198	5	9	7.1	6438	PASS
275	198	10	60	23.2	21027	PASS
365	198	1	100	2.5	2304	PASS
441	442	0.01	24	14.9	11058	PASS
442	198	50	100	82.2	74392	PASS
443	442	15	24	18.2	13523	PASS