
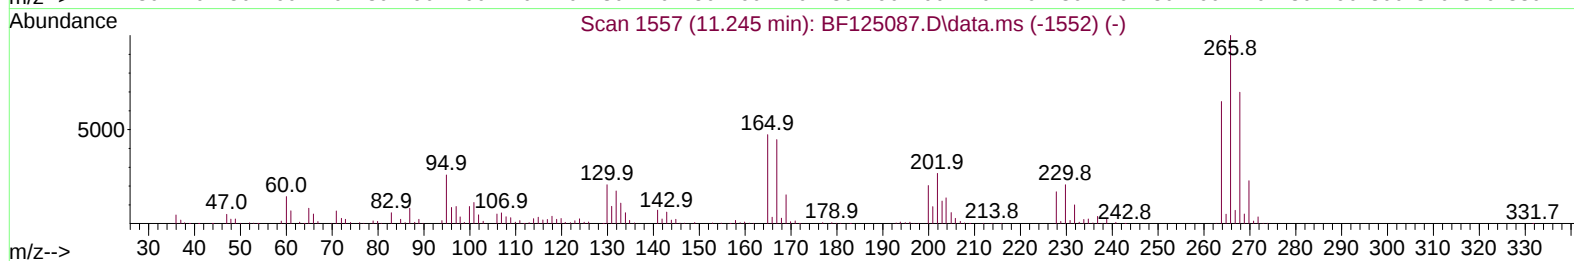
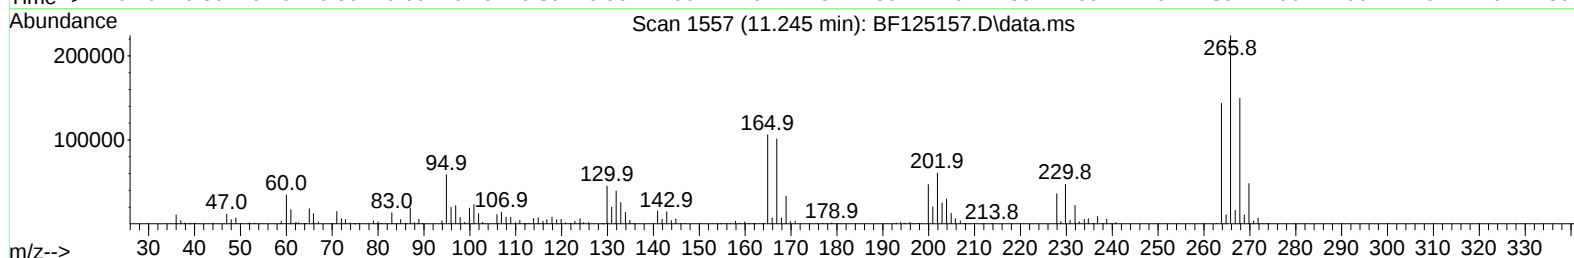


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082321\
Data File : BF125157.D
Acq On : 23 Aug 2021 16:11
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 06:27:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 10:15:49 2021
Response via : Initial Calibration

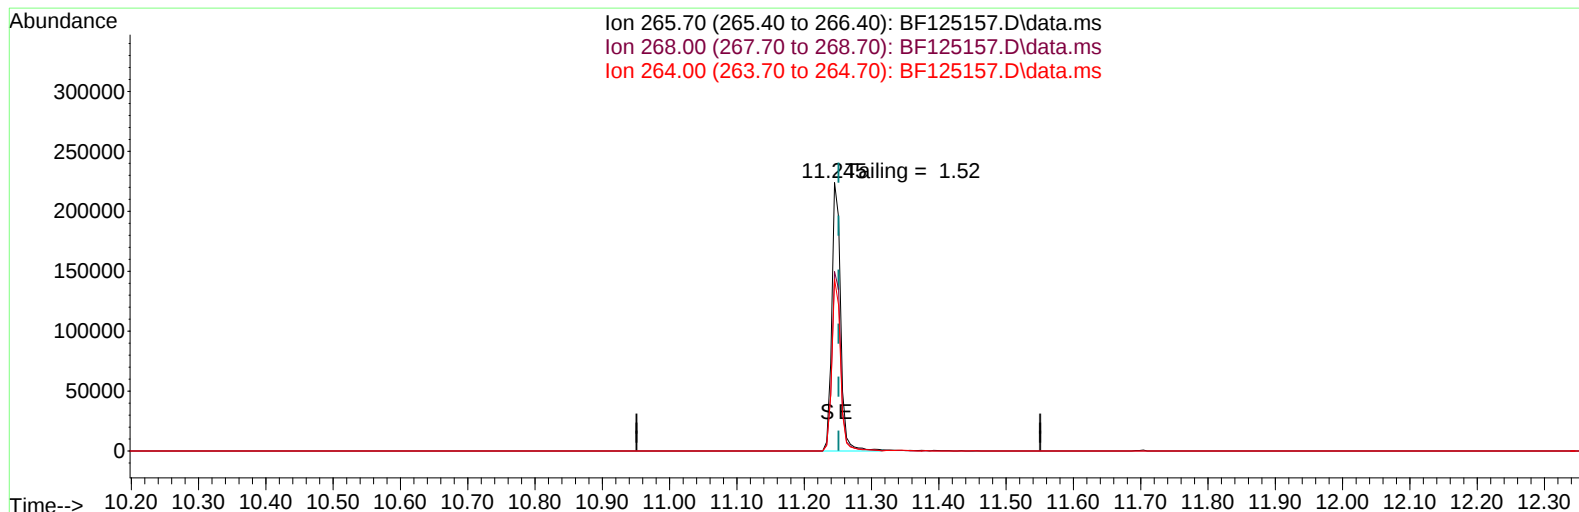

TIC: BF125157.D\data.ms

(70) Pentachlorophenol (C)




11.245min (-0.006) 106838.96 ng

response 206530

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	66.85
264.00	69.90	64.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082321\
Data File : BF125157.D
Acq On : 23 Aug 2021 16:11
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 06:27:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 10:15:49 2021
Response via : Initial Calibration

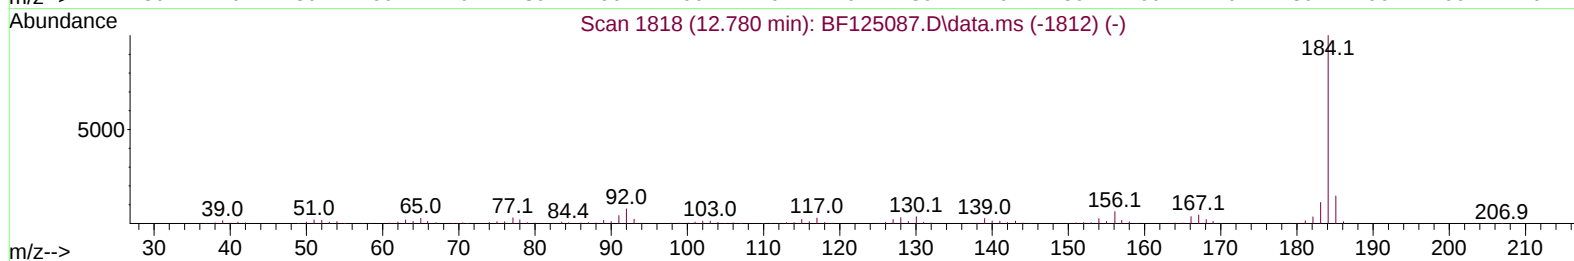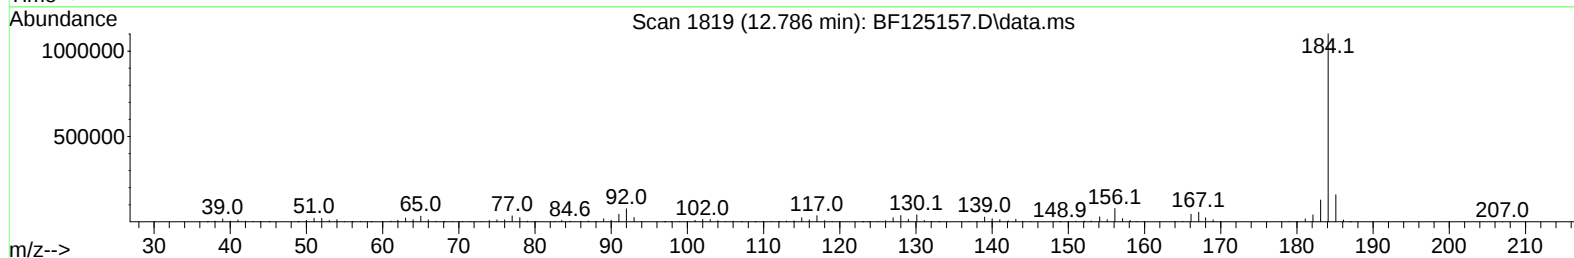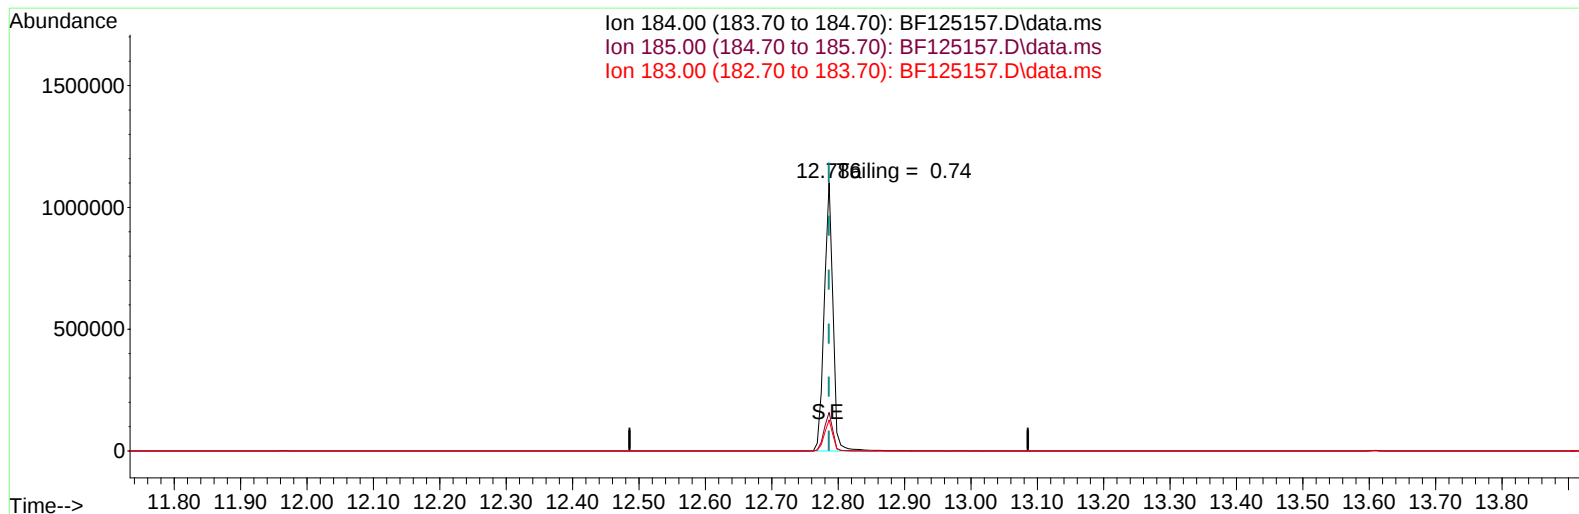

TIC: BF125157.D\data.ms

(77) Benzidine

12.786min (+ 0.000) 82747.36 ng

response 1011477

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.38
183.00	10.10	11.57
0.00	0.00	0.00