

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082321\
 Data File : BF125175.D
 Acq On : 24 Aug 2021 2:06
 Operator : JU/CG
 Sample : M3513-01 2X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TR-04-082121

Manual Integrations
 APPROVED

mohammad
 8/24/2021 11:20:17 AM

Quant Time: Aug 24 04:51:05 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 23 10:15:49 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.922	152	166373	20.000	ng	0.00
21) Naphthalene-d8	8.204	136	606875	20.000	ng	# 0.00
39) Acenaphthene-d10	9.963	164	287305	20.000	ng	0.00
64) Phenanthrene-d10	11.451	188	510646	20.000	ng	0.00
76) Chrysene-d12	14.098	240	342517	20.000	ng	# 0.00
86) Perylene-d12	15.603	264	269084	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.534	112	449023	40.850	ng	0.00
7) Phenol-d6	6.539	99	556843	39.170	ng	0.00
23) Nitrobenzene-d5	7.480	82	357787	29.681	ng	0.00
42) 2,4,6-Tribromophenol	10.751	330	135407	47.214	ng	0.00
45) 2-Fluorobiphenyl	9.280	172	615048	29.836	ng	0.00
79) Terphenyl-d14	13.039	244	640123	29.773	ng	0.00
Target Compounds						Qvalue
38) 1-Methylnaphthalene	9.016	142	45872	2.392	ng	92
49) Acenaphthylene	9.822	152	106173	3.871	ng	97
52) Acenaphthene	9.992	154	49512	2.912	ng	96
58) Fluorene	10.510	166	69088	3.819	ng	99
71) Phenanthrene	11.480	178	1439393	51.157	ng	97
72) Anthracene	11.527	178	206407	7.443	ng	99
73) Carbazole	11.680	167	98246	3.877	ng	99
75) Fluoranthene	12.674	202	2497908	89.471	ng	97
78) Pyrene	12.910	202	2951343	100.450	ng	94
81) Benzo(a)anthracene	14.092	228	1196747	48.493	ng	94
83) Chrysene	14.127	228	1255563	51.445	ng	95
87) Indeno(1,2,3-cd)pyrene	17.121	276	555382	28.650	ng	# 87
88) Benzo(b)fluoranthene	15.162	252	1278816m	65.051	ng	
89) Benzo(k)fluoranthene	15.186	252	357155m	19.469	ng	
90) Benzo(a)pyrene	15.545	252	950766m	54.751	ng	
91) Dibenzo(a,h)anthracene	17.133	278	130190m	7.769	ng	
92) Benzo(g,h,i)perylene	17.592	276	585548	36.241	ng	# 88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082321\
Data File : BF125175.D
Acq On : 24 Aug 2021 2:06
Operator : JU/CG
Sample : M3513-01 2X
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
TR-04-082121

Manual Integrations
APPROVED


mohammad
8/24/2021 11:20:17 AM

Quant Time: Aug 24 04:51:05 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 10:15:49 2021
Response via : Initial Calibration



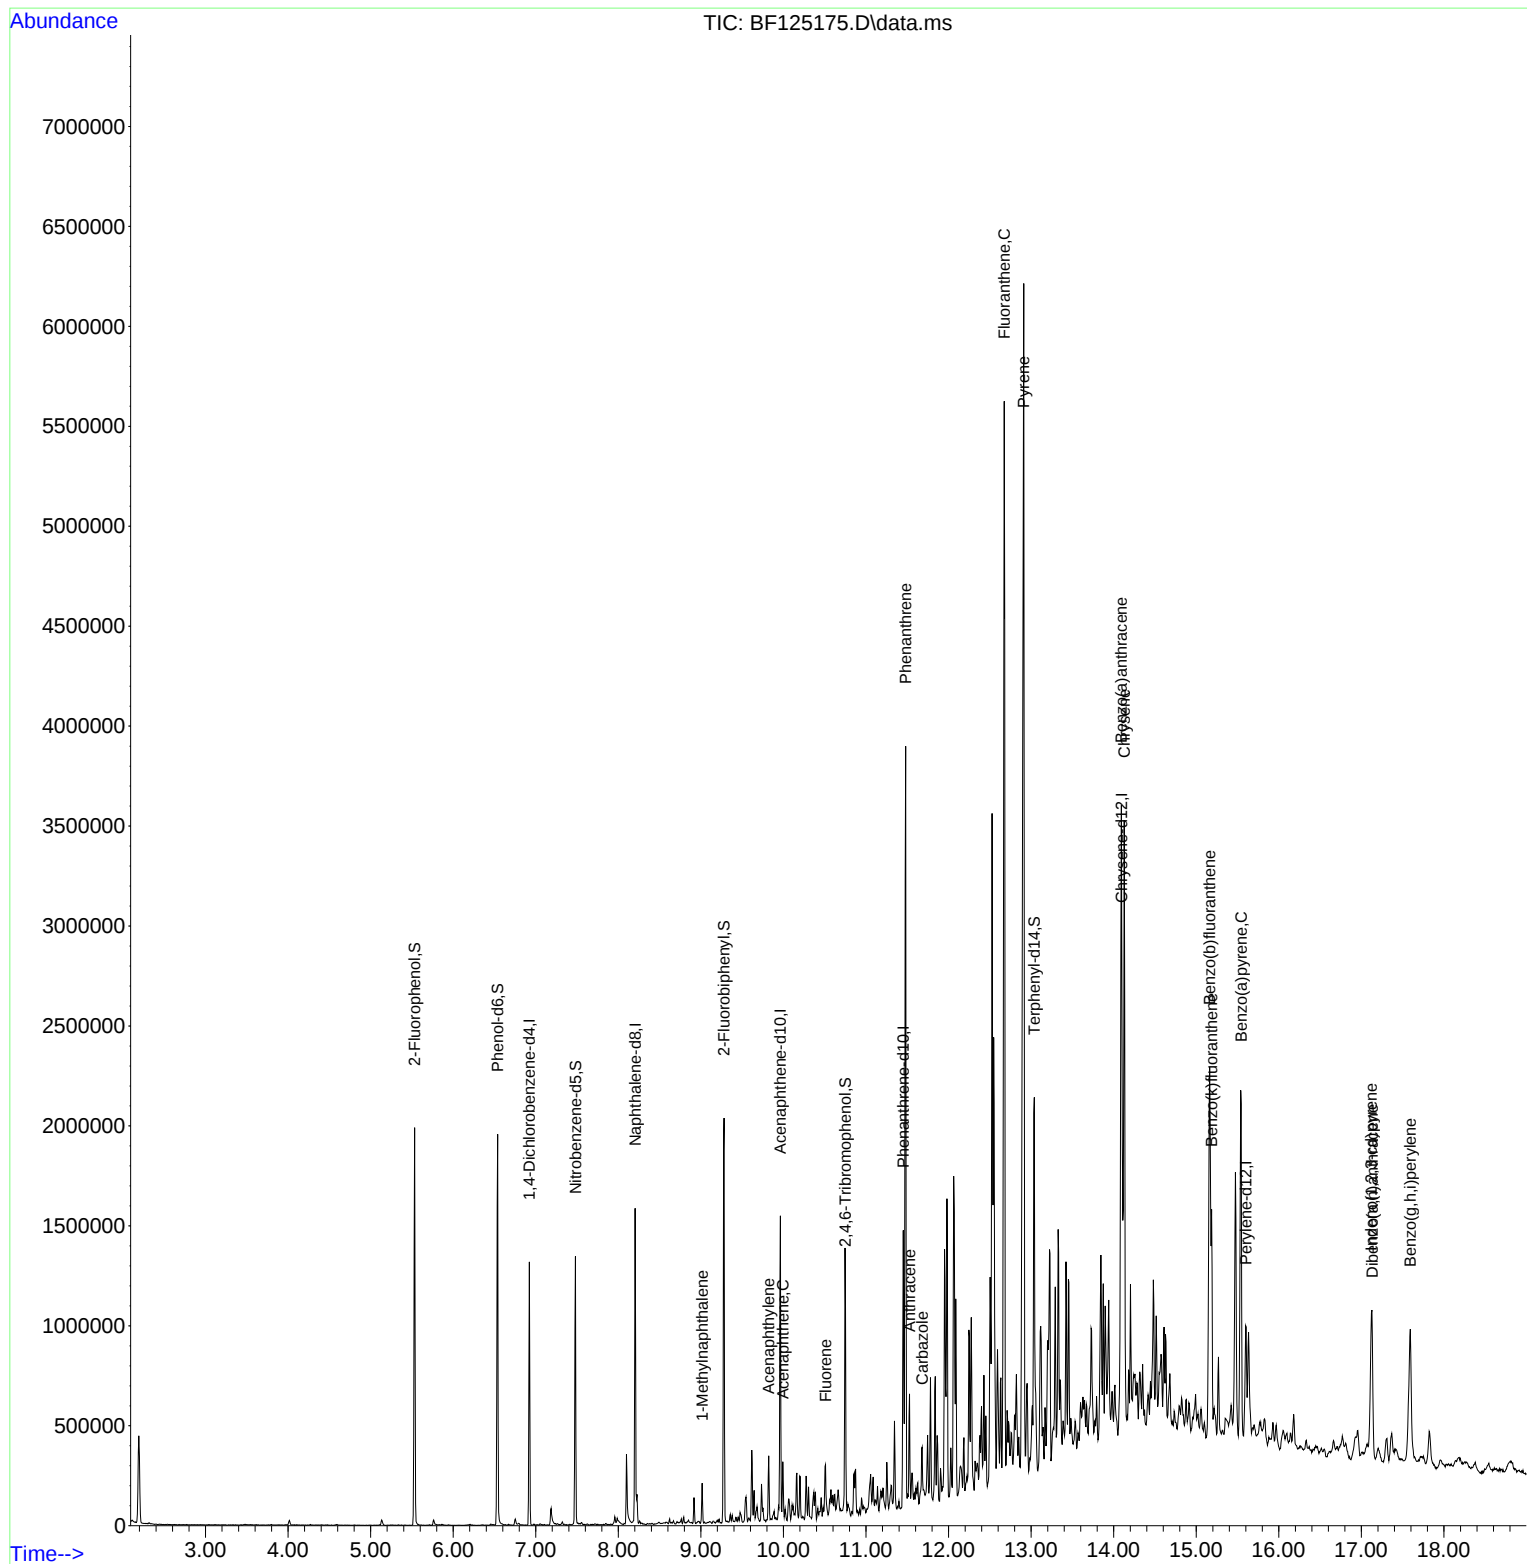





#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.922 min Scan# 822
Delta R.T. -0.006 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06





Tgt Ion:152 Resp: 166373
Ion Ratio Lower Upper
152 100
150 161.7 117.6 176.4
115 61.1 47.1 70.7

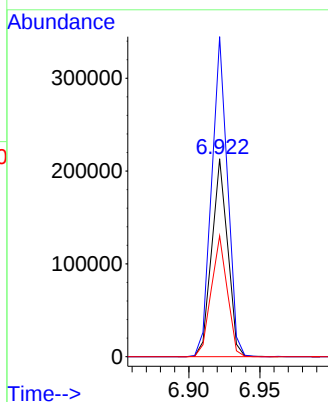

#5
2-Fluorophenol
Concen: 40.850 ng
RT: 5.534 min Scan# 586
Delta R.T. -0.006 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06




Tgt Ion:112 Resp: 449023
Ion Ratio Lower Upper
112 100
64 70.7 44.2 66.2#
63 38.2 26.2 39.2

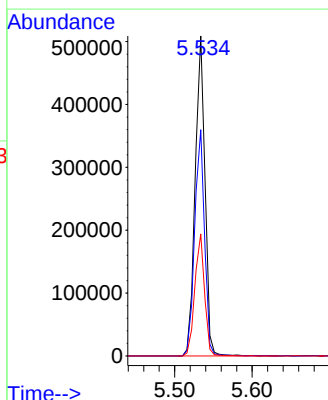

Instrument :
BNA_F
ClientSampleId :
TR-04-082121

Manual Integrations
APPROVED

mohammad
8/24/2021 11:20:17 AM







#7
Phenol-d6
Concen: 39.170 ng
RT: 6.539 min Scan# 757
Delta R.T. -0.006 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06

Tgt Ion: 99 Resp: 556843
Ion Ratio Lower Upper
99 100
42 22.5 23.5 35.3#
71 36.0 25.6 38.4

Instrument :
BNA_F
ClientSampleId :
TR-04-082121




Manual Integrations
APPROVED


mohammad
8/24/2021 11:20:17 AM

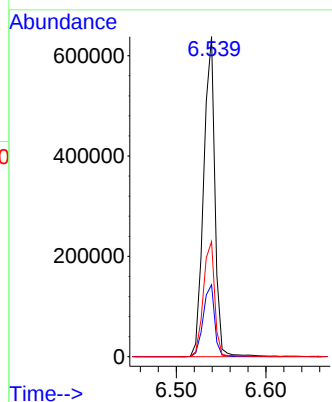

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.204 min Scan# 1040
Delta R.T. -0.006 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06

Tgt Ion: 136 Resp: 606875
Ion Ratio Lower Upper
136 100
137 11.3 9.8 14.6
54 10.6 6.4 9.6#
68 5.7 3.3 4.9#

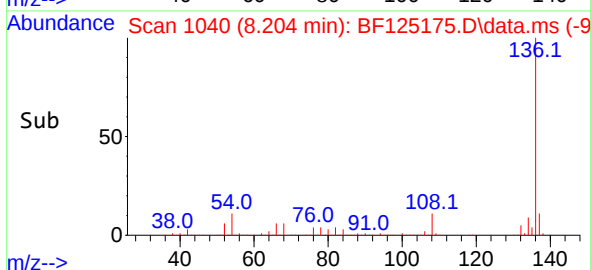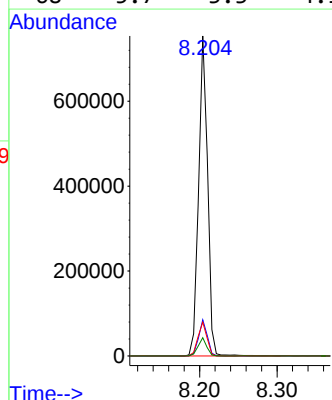

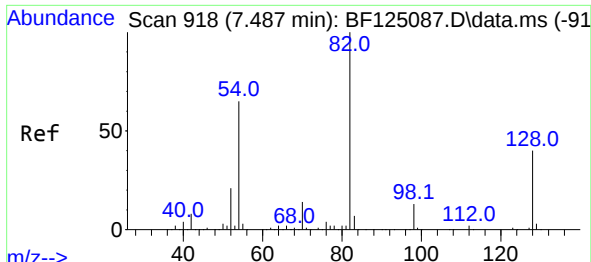





#23
Nitrobenzene-d5
Concen: 29.681 ng
RT: 7.480 min Scan# 917
Delta R.T. -0.006 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06

Instrument :
BNA_F
ClientSampleId :
TR-04-082121

Tgt Ion: 82 Resp: 357787
Ion Ratio Lower Upper
82 100
128 40.6 40.6 60.8
54 63.7 49.6 74.4




Manual Integrations
APPROVED


mohammad
8/24/2021 11:20:17 AM

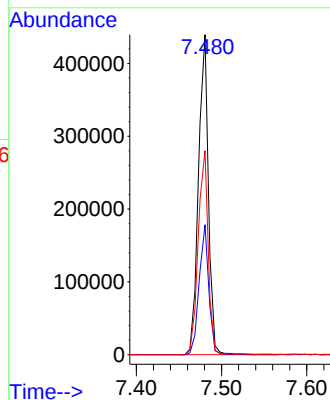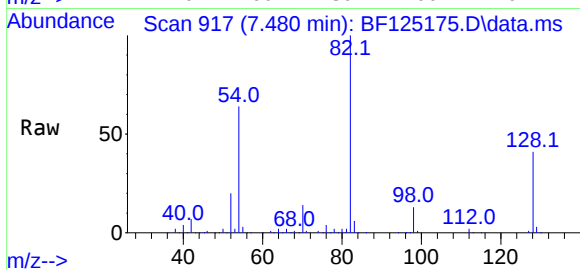

#38
1-Methylnaphthalene
Concen: 2.392 ng
RT: 9.016 min Scan# 1178
Delta R.T. -0.006 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06


Tgt Ion: 142 Resp: 45872
Ion Ratio Lower Upper
142 100
141 87.2 76.0 114.0

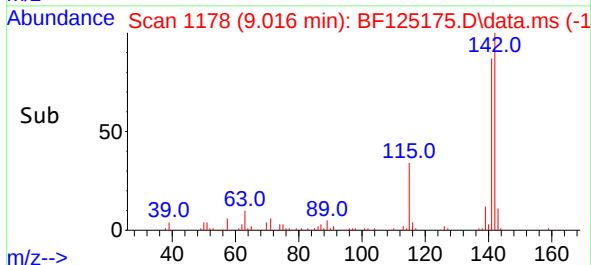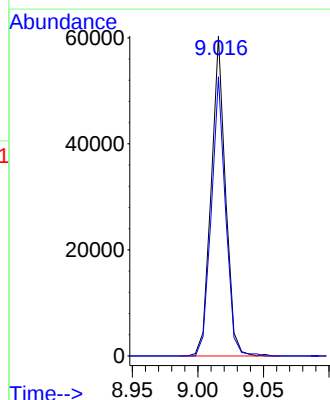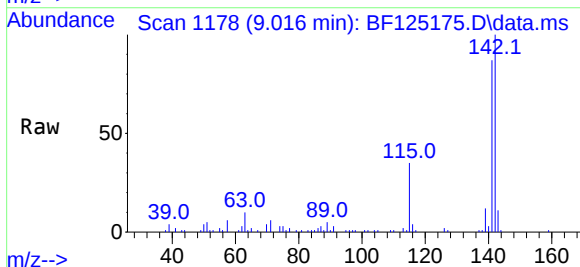

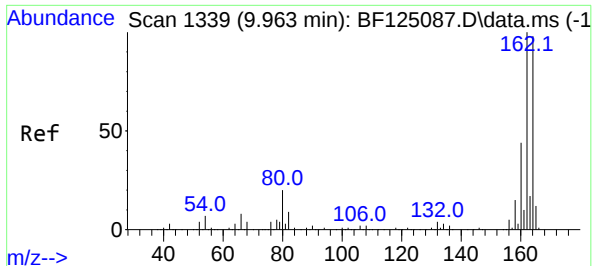

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.963 min Scan# 1339
Delta R.T. 0.000 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06




Instrument :
BNA_F
ClientSampleId :
TR-04-082121

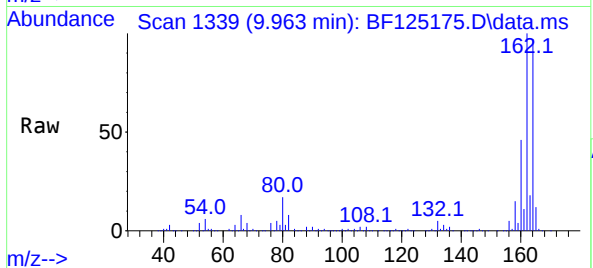


Tgt Ion:164 Resp: 287305
Ion Ratio Lower Upper
164 100
162 102.9 81.3 121.9
160 47.0 38.0 57.0

Manual Integrations
APPROVED



mohammad
8/24/2021 11:20:17 AM

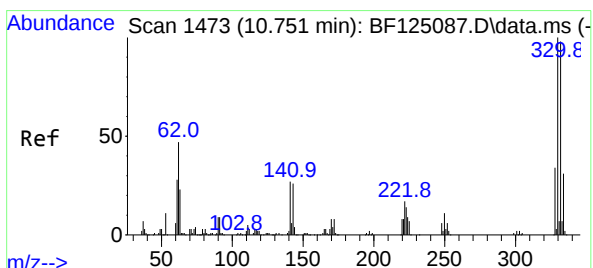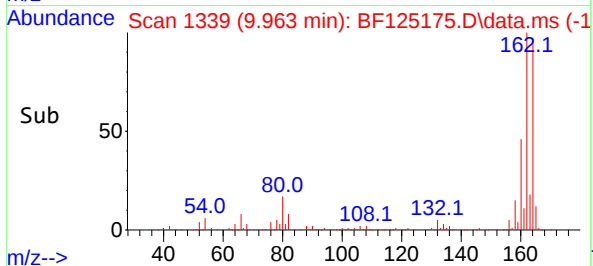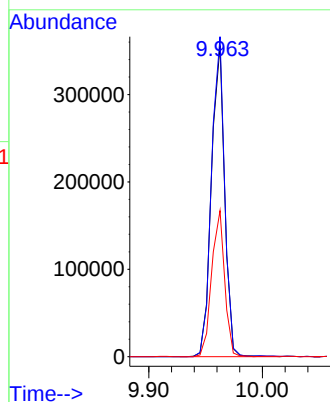


#42
2,4,6-Tribromophenol
Concen: 47.214 ng
RT: 10.751 min Scan# 1473
Delta R.T. -0.006 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06

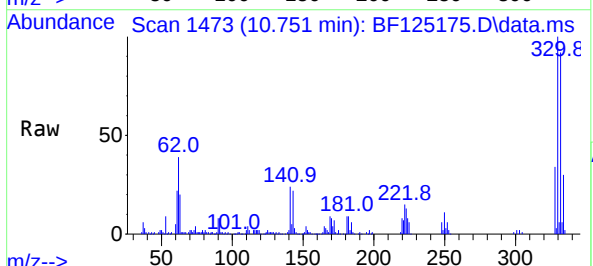


Tgt Ion:330 Resp: 135407
Ion Ratio Lower Upper
330 100
332 94.3 76.2 114.4
141 33.6 44.6 66.8#

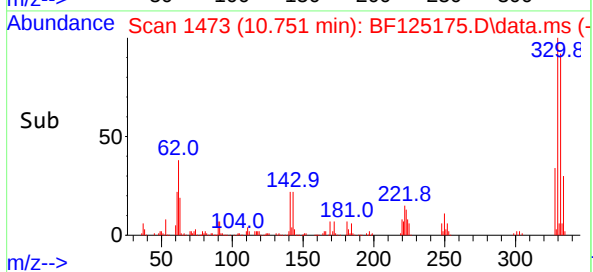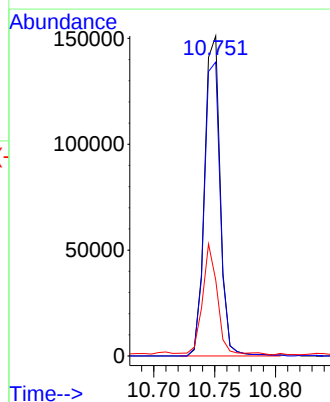



#45
2-Fluorobiphenyl
Concen: 29.836 ng
RT: 9.280 min Scan# 1223
Delta R.T. -0.006 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06




Instrument :
BNA_F
ClientSampleId :
TR-04-082121




Tgt Ion:172 Resp: 615048
Ion Ratio Lower Upper
172 100
171 33.8 26.5 39.7
170 23.0 18.8 28.2

Manual Integrations
APPROVED



mohammad
8/24/2021 11:20:17 AM

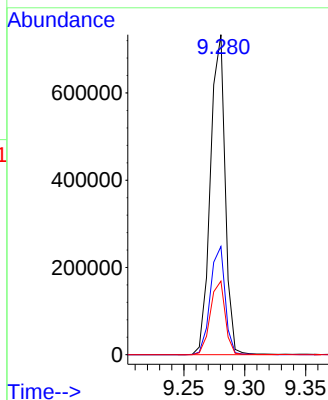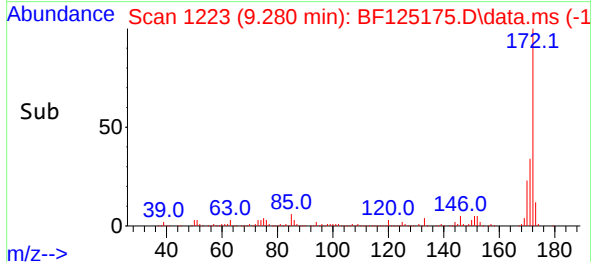


#49
Acenaphthylene
Concen: 3.871 ng
RT: 9.822 min Scan# 1315
Delta R.T. -0.006 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06




Tgt Ion:152 Resp: 106173
Ion Ratio Lower Upper
152 100
151 18.5 15.7 23.5
153 13.8 9.8 14.8

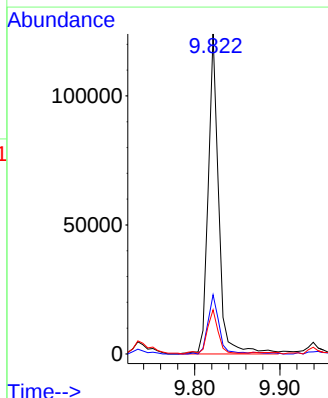



#52
Acenaphthene
Concen: 2.912 ng
RT: 9.992 min Scan# 1344
Delta R.T. -0.006 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06




Instrument :
BNA_F
ClientSampleId :
TR-04-082121




Tgt Ion:154 Resp: 49512
Ion Ratio Lower Upper
154 100
153 112.6 89.4 134.2
152 58.6 40.5 60.7

Manual Integrations
APPROVED



mohammad
8/24/2021 11:20:17 AM

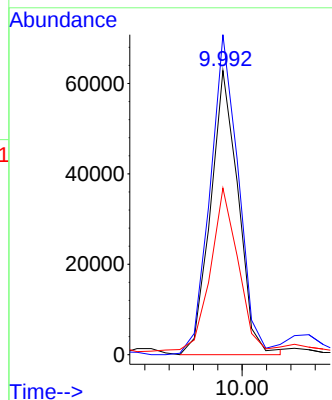


#58
Fluorene
Concen: 3.819 ng
RT: 10.510 min Scan# 1432
Delta R.T. -0.006 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06




Tgt Ion:166 Resp: 69088
Ion Ratio Lower Upper
166 100
165 96.3 78.1 117.1
167 14.5 11.1 16.7

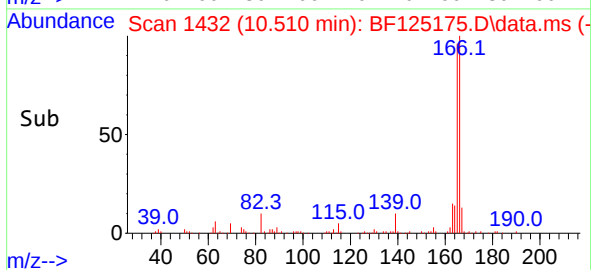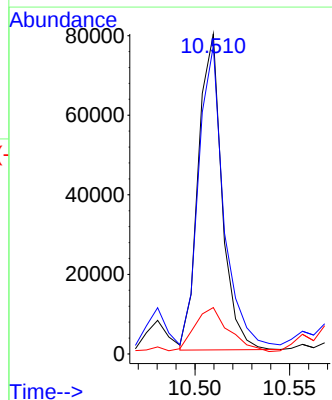



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.451 min Scan# 1592
Delta R.T. 0.000 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06




Instrument :
BNA_F
ClientSampleId :
TR-04-082121




Tgt Ion:188 Resp: 510646
Ion Ratio Lower Upper
188 100
94 8.6 6.7 10.1
80 9.5 7.5 11.3

Manual Integrations
APPROVED



mohammad
8/24/2021 11:20:17 AM

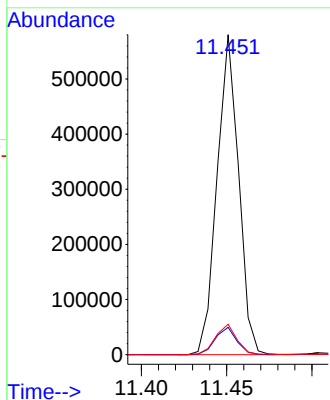


#71
Phenanthrene
Concen: 51.157 ng
RT: 11.480 min Scan# 1597
Delta R.T. -0.000 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06



Tgt Ion:178 Resp: 1439393
Ion Ratio Lower Upper
178 100
176 19.7 14.7 22.1
179 15.5 11.5 17.3

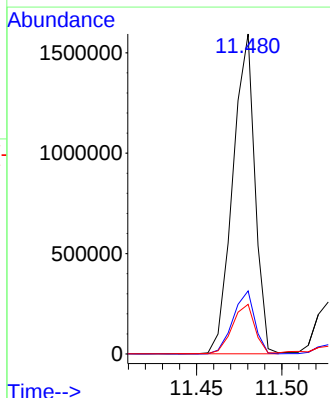







#72
 Anthracene
 Concen: 7.443 ng
 RT: 11.527 min Scan# 1605
 Delta R.T. 0.000 min
 Lab File: BF125175.D
 Acq: 24 Aug 2021 2:06

Instrument :
 BNA_F
 ClientSampleId :
 TR-04-082121

Tgt Ion:178 Resp: 206407
 Ion Ratio Lower Upper
 178 100
 176 17.9 14.3 21.5
 179 14.7 12.2 18.4




Manual Integrations
 APPROVED


mohammad
 8/24/2021 11:20:17 AM

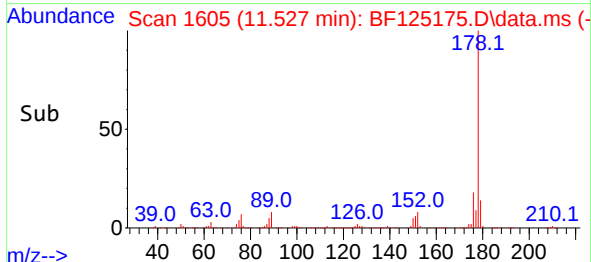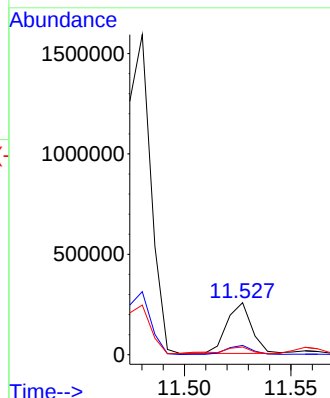

#73
 Carbazole
 Concen: 3.877 ng
 RT: 11.680 min Scan# 1631
 Delta R.T. 0.000 min
 Lab File: BF125175.D
 Acq: 24 Aug 2021 2:06

Tgt Ion:167 Resp: 98246
 Ion Ratio Lower Upper
 167 100
 166 22.1 17.4 26.0
 139 12.9 11.0 16.4

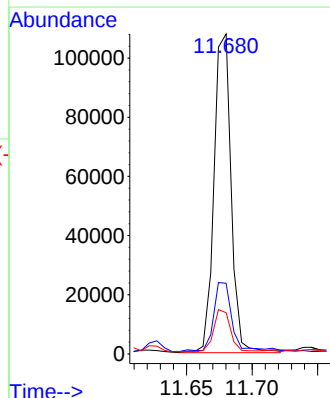







#75
Fluoranthene
Concen: 89.471 ng
RT: 12.674 min Scan# 1800
Delta R.T. 0.006 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06

Tgt Ion:202 Resp: 2497908
Ion Ratio Lower Upper
202 100
101 10.6 0.0 30.7
203 18.7 0.0 36.3

Instrument :
BNA_F
ClientSampleId :
TR-04-082121




Manual Integrations
APPROVED


mohammad
8/24/2021 11:20:17 AM

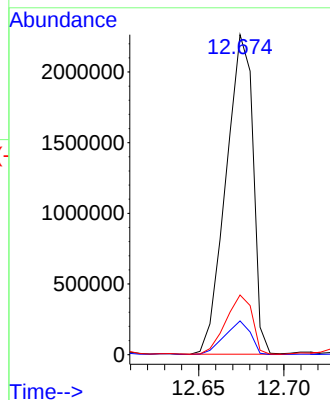

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.098 min Scan# 2042
Delta R.T. 0.000 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06

Tgt Ion:240 Resp: 342517
Ion Ratio Lower Upper
240 100
120 10.2 10.8 16.2#
236 25.9 21.6 32.4

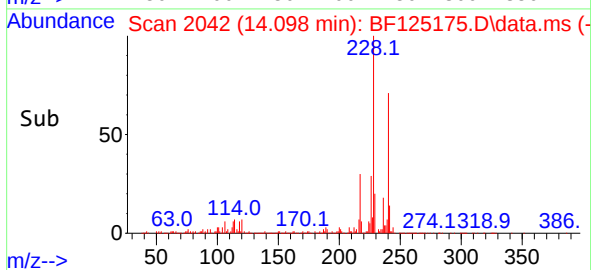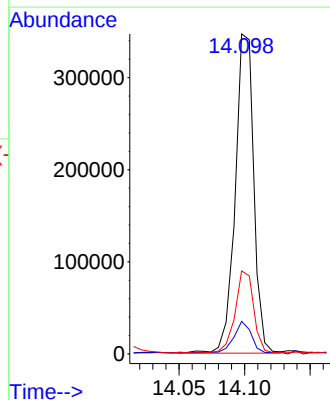







#78
Pyrene
Concen: 100.450 ng
RT: 12.910 min Scan# 1840
Delta R.T. 0.012 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06

Tgt Ion:202 Resp: 2951343
Ion Ratio Lower Upper
202 100
200 22.0 15.3 22.9
203 18.9 13.4 20.0

Instrument :
BNA_F
ClientSampleId :
TR-04-082121




Manual Integrations
APPROVED


mohammad
8/24/2021 11:20:17 AM

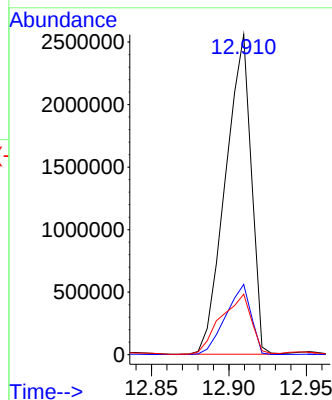

#79
Terphenyl-d14
Concen: 29.773 ng
RT: 13.039 min Scan# 1862
Delta R.T. 0.000 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06


Tgt Ion:244 Resp: 640123
Ion Ratio Lower Upper
244 100
212 6.4 5.9 8.9
122 8.0 9.0 13.4#

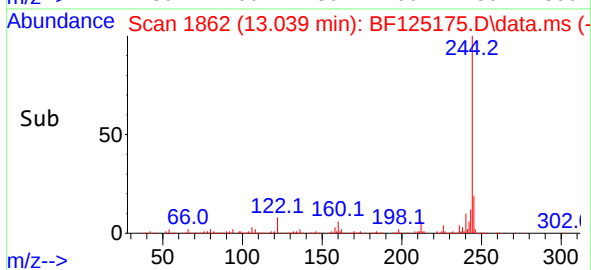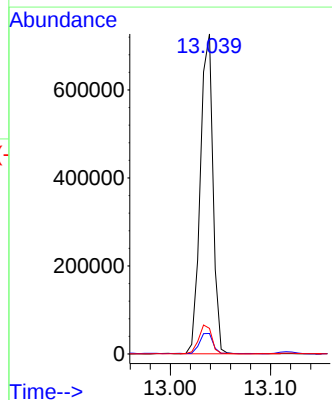



#81
Benzo(a)anthracene
Concen: 48.493 ng
RT: 14.092 min Scan# 2041
Delta R.T. 0.006 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06



Instrument :
BNA_F
ClientSampleId :
TR-04-082121

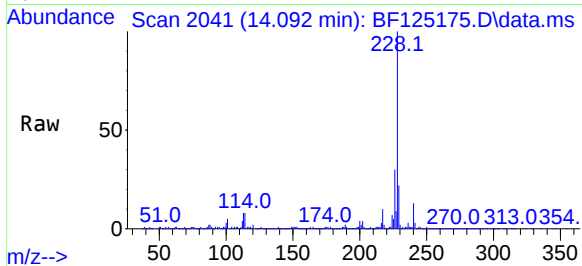


Tgt Ion:228 Resp: 1196747
Ion Ratio Lower Upper
228 100
226 30.1 21.6 32.4
229 21.8 15.6 23.4

Manual Integrations
APPROVED



mohammad
8/24/2021 11:20:17 AM

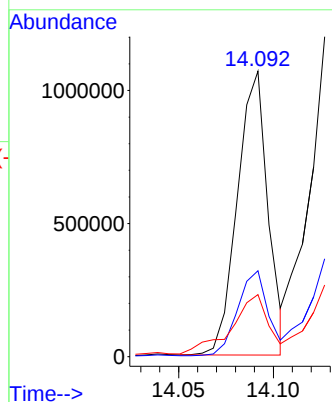


#83
Chrysene
Concen: 51.445 ng
RT: 14.127 min Scan# 2047
Delta R.T. 0.006 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06

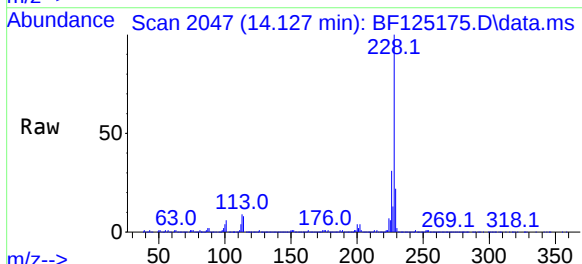


Tgt Ion:228 Resp: 1255563
Ion Ratio Lower Upper
228 100
226 30.6 22.6 34.0
229 22.4 15.9 23.9

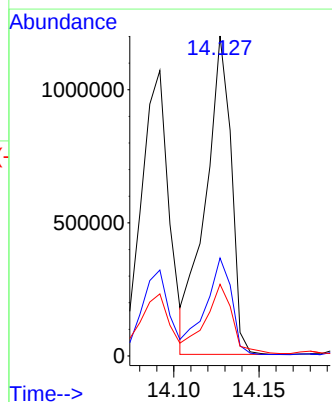



#86
Perylene-d12
Concen: 20.000 ng
RT: 15.603 min Scan# 2298
Delta R.T. 0.006 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06




Instrument :
BNA_F
ClientSampleId :
TR-04-082121

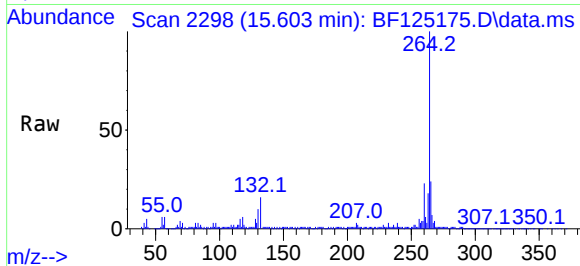


Tgt Ion:264 Resp: 269084
Ion Ratio Lower Upper
264 100
260 23.5 19.6 29.4
265 23.7 17.2 25.8

Manual Integrations
APPROVED



mohammad
8/24/2021 11:20:17 AM

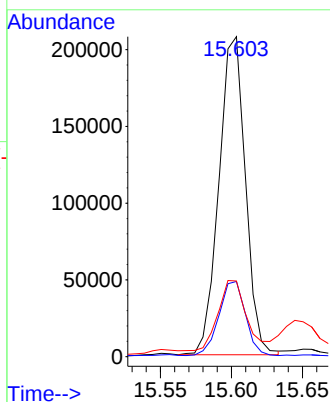


#87
Indeno(1,2,3-cd)pyrene
Concen: 28.650 ng
RT: 17.121 min Scan# 2556
Delta R.T. 0.000 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06

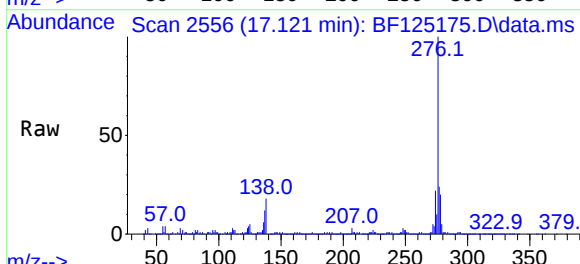


Tgt Ion:276 Resp: 555382
Ion Ratio Lower Upper
276 100
138 17.5 24.1 36.1#
277 23.8 18.8 28.2

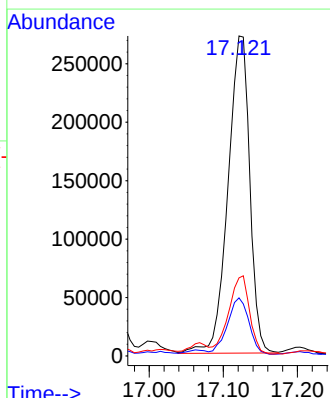



#88
Benzo(b)fluoranthene
Concen: 65.051 ng m
RT: 15.162 min Scan# 2223
Delta R.T. 0.006 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06




Instrument :
BNA_F
ClientSampleId :
TR-04-082121




Tgt Ion:252 Resp: 1278816
Ion Ratio Lower Upper
252 100
253 23.1 16.8 25.2
125 9.4 9.8 14.8#

Manual Integrations
APPROVED



mohammad
8/24/2021 11:20:17 AM

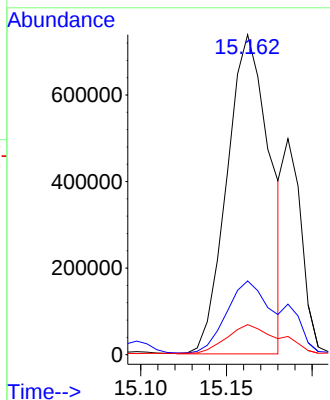


#89
Benzo(k)fluoranthene
Concen: 19.469 ng m
RT: 15.186 min Scan# 2227
Delta R.T. 0.000 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06




Tgt Ion:252 Resp: 357155
Ion Ratio Lower Upper
252 100
253 23.4 17.8 26.8
125 8.5 7.2 10.8

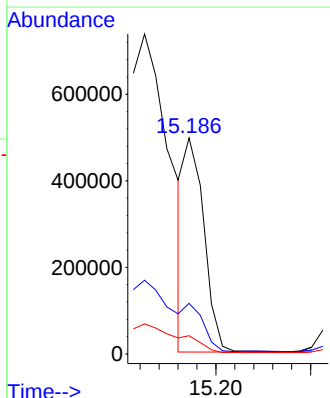



#90
Benzo(a)pyrene
Concen: 54.751 ng m
RT: 15.545 min Scan# 2288
Delta R.T. 0.012 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06




Instrument :
BNA_F
ClientSampleId :
TR-04-082121




Tgt Ion:252 Resp: 950766
Ion Ratio Lower Upper
252 100
253 22.3 18.4 27.6
125 7.9 9.9 14.9#

Manual Integrations
APPROVED



mohammad
8/24/2021 11:20:17 AM

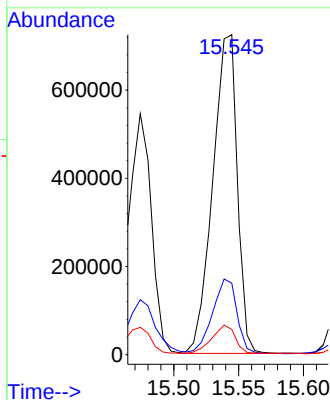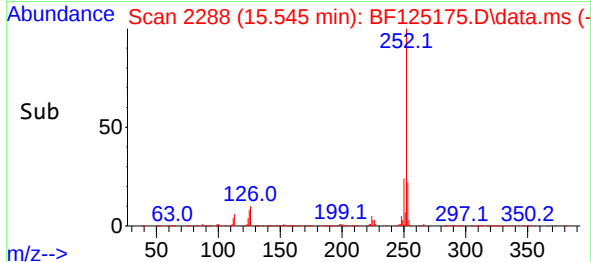


#91
Dibenzo(a,h)anthracene
Concen: 7.769 ng m
RT: 17.133 min Scan# 2558
Delta R.T. -0.006 min
Lab File: BF125175.D
Acq: 24 Aug 2021 2:06



Tgt Ion:278 Resp: 130190
Ion Ratio Lower Upper
278 100
139 14.1 14.9 22.3#
279 27.8 19.7 29.5

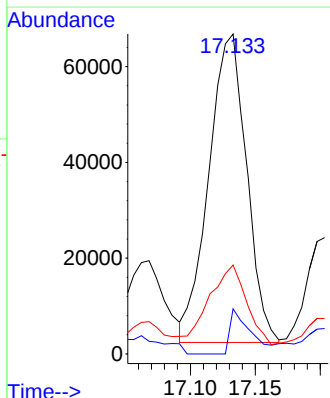



#92
 Benzo(g,h,i)perylene
 Concen: 36.241 ng
 RT: 17.592 min Scan# 2636
 Delta R.T. 0.006 min
 Lab File: BF125175.D
 Acq: 24 Aug 2021 2:06

Tgt Ion: 276 Resp: 585548
 Ion Ratio Lower Upper
 276 100
 277 23.9 22.0 33.0
 138 18.5 22.2 33.4#

Instrument :
 BNA_F
 ClientSampleId :
 TR-04-082121

Manual Integrations
 APPROVED

mohammad
 8/24/2021 11:20:17 AM

