
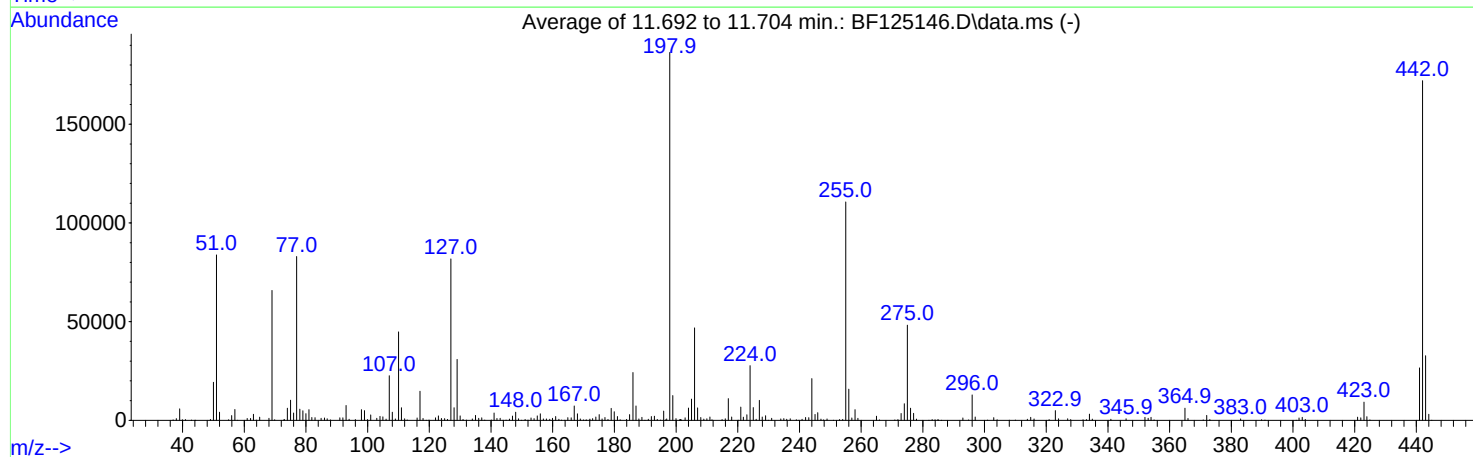


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082321\
 Data File : BF125146.D
 Acq On : 23 Aug 2021 9:14
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 23 10:15:49 2021

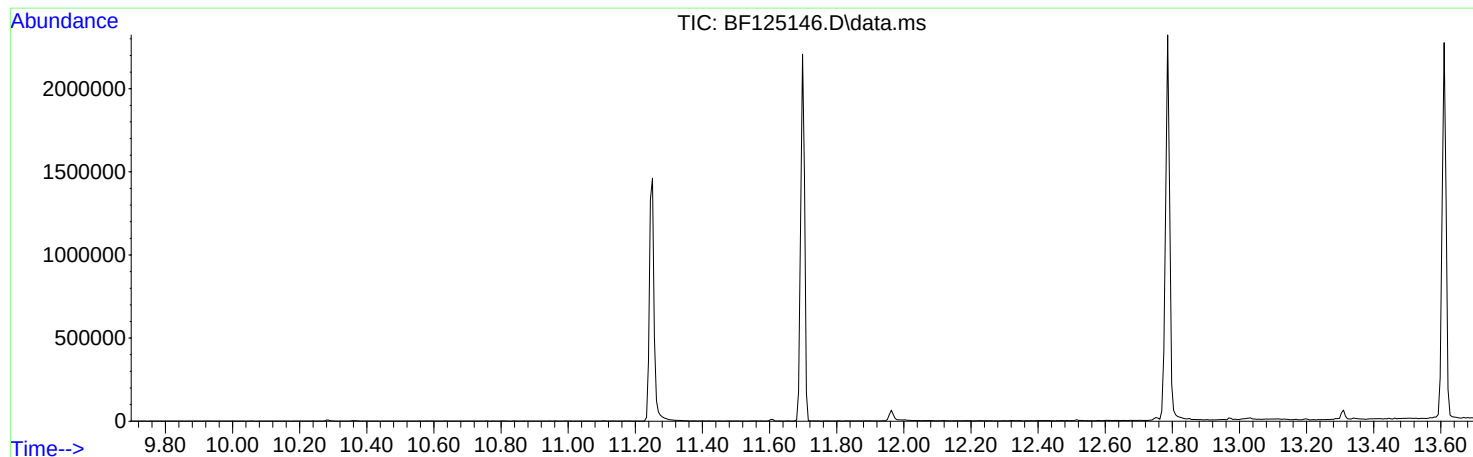




AutoFind: Scans 1633, 1634, 1635; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	83821	PASS
68	69	0.00	2	1.6	1038	PASS
69	198	0.00	100	35.3	65781	PASS
70	69	0.00	2	0.5	298	PASS
127	198	10	80	43.9	81797	PASS
197	198	0.00	2	0.4	740	PASS
198	198	100	100	100.0	186325	PASS
199	198	5	9	6.7	12535	PASS
275	198	10	60	25.9	48189	PASS
365	198	1	100	3.3	6132	PASS
441	198	0.01	100	14.3	26619	PASS
442	442	50	100	100.0	172048	PASS
443	442	15	24	19.0	32767	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082321\
 Data File : BF125146.D
 Acq On : 23 Aug 2021 9:14
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 23 09:51:27 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 18 17:03:50 2021
 Response via : Initial Calibration

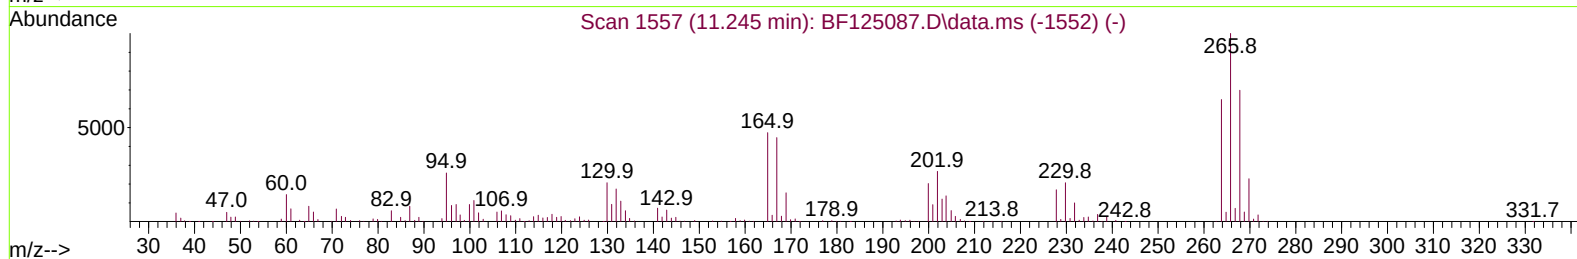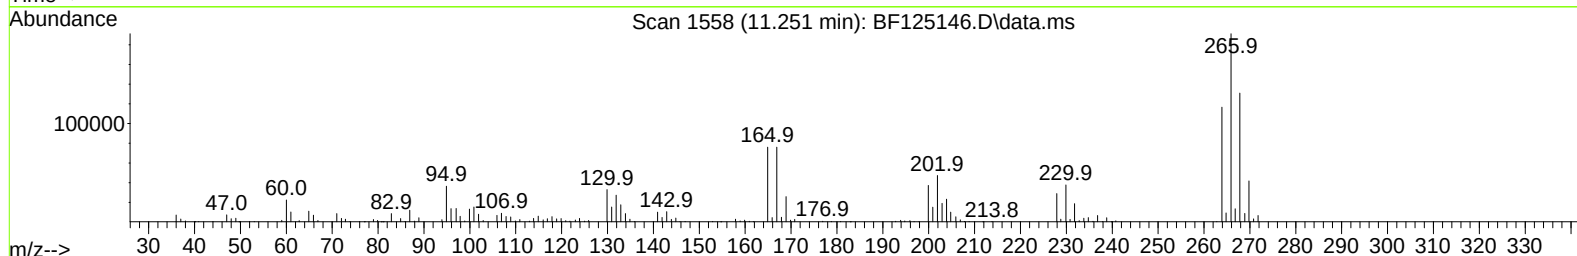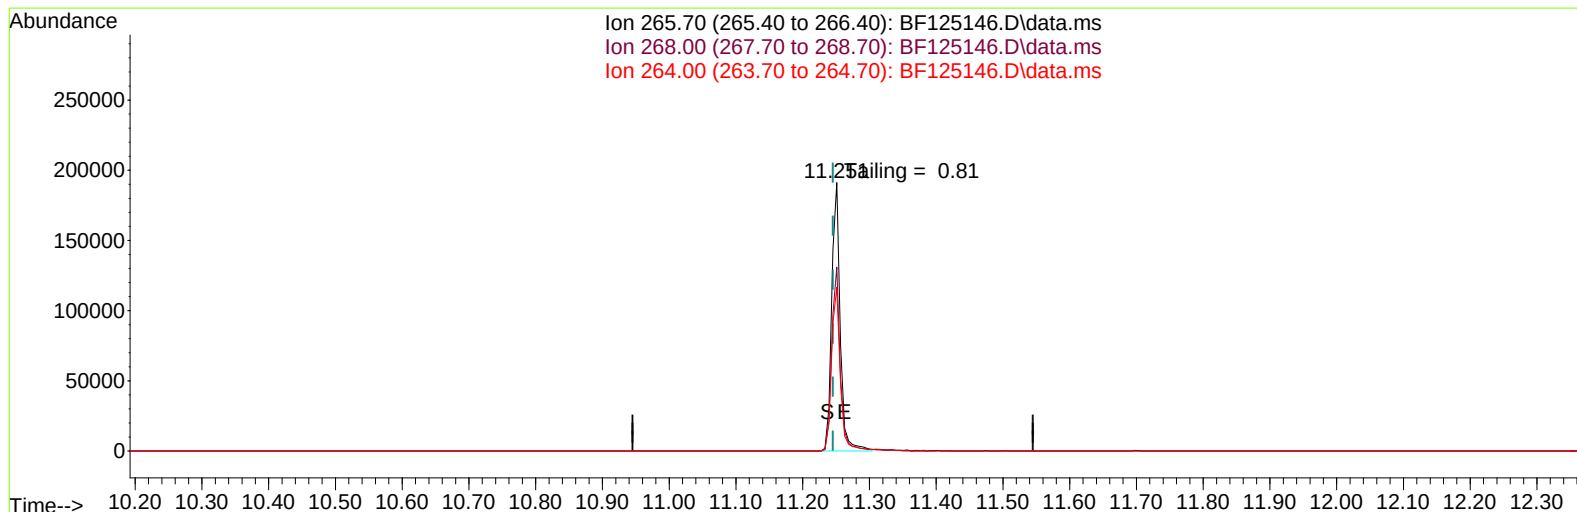

TIC: BF125146.D\data.ms

(70) Pentachlorophenol (C)

11.251min (+ 0.006) 56528.21 ng




response 172882

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	68.48
264.00	69.90	60.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082321\
Data File : BF125146.D
Acq On : 23 Aug 2021 9:14
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 23 09:51:27 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 18 17:03:50 2021
Response via : Initial Calibration

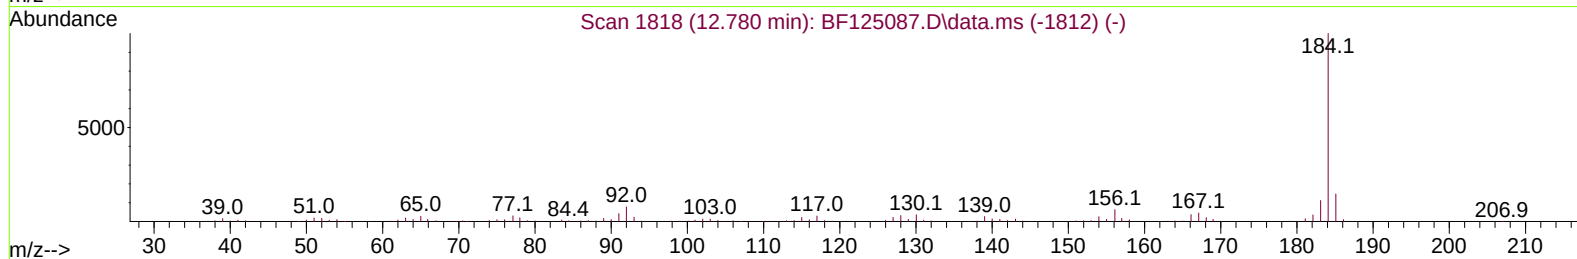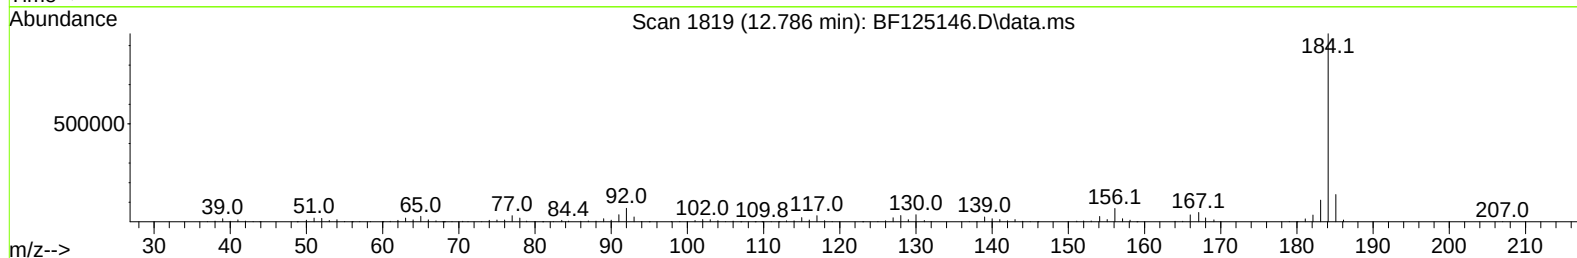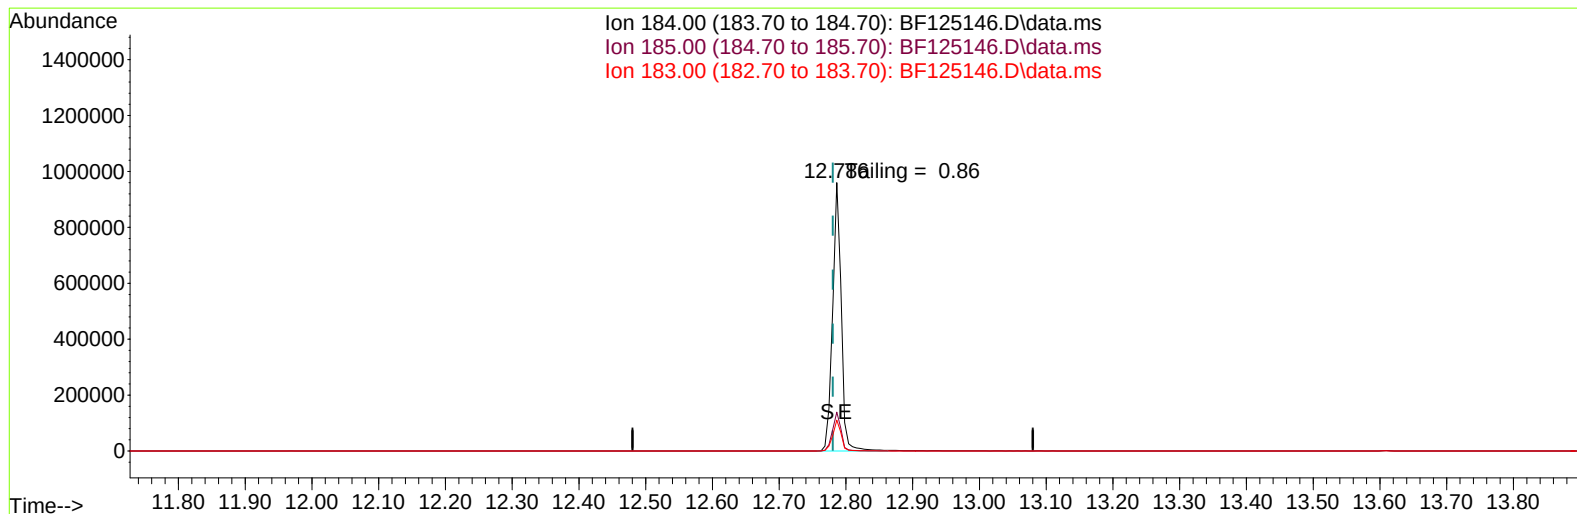

TIC: BF125146.D\data.ms

(77) Benzidine

12.786min (+ 0.006) 86062.40 ng

response 874662

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.49
183.00	10.10	11.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/23/2021	BNA_F	<u>BF125146.D</u>
Compound Name	Response	Retention Time
DDT	362701	13.61
DDD	12248	13.31
DDE	1453	12.969
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13701	376402	3.64

Instrument :
BNA_F
ClientSampleId :
DFTPP