
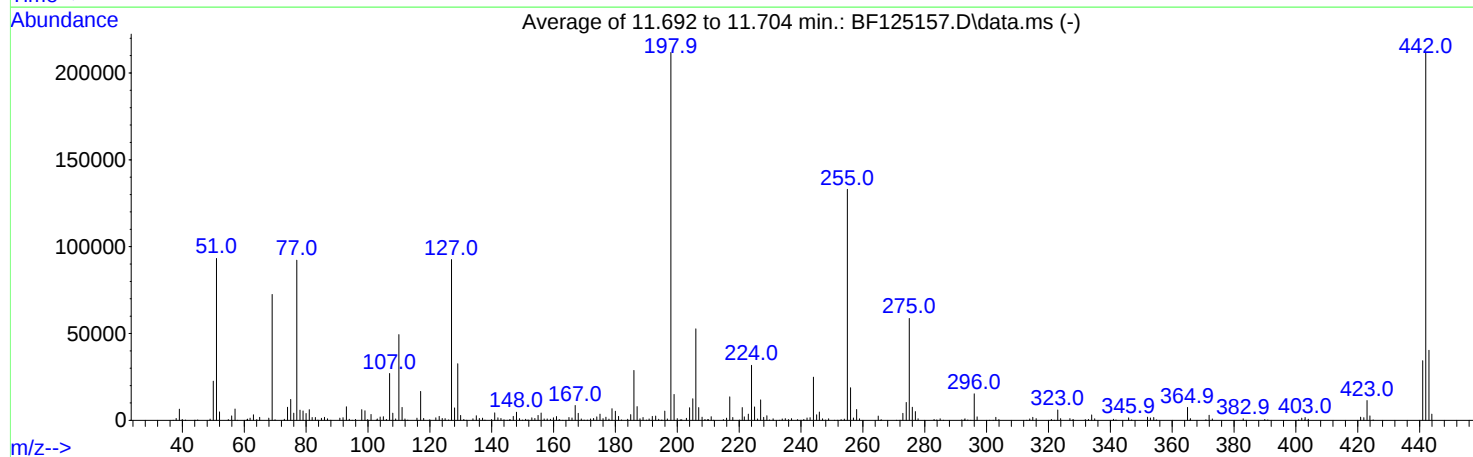


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082321\
 Data File : BF125157.D
 Acq On : 23 Aug 2021 16:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 24 12:39:21 2021

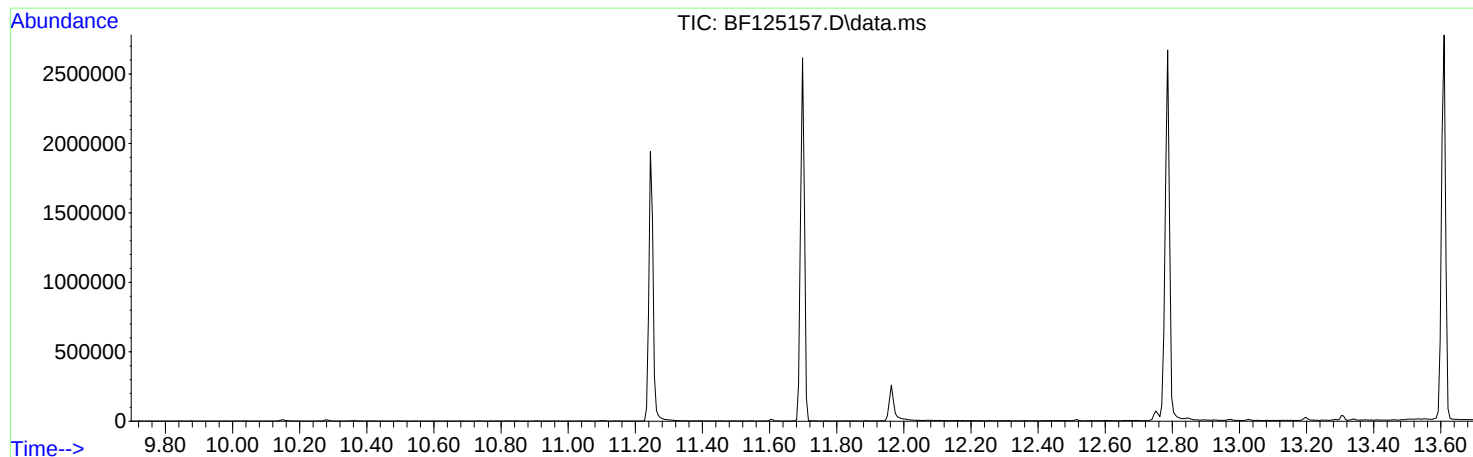




AutoFind: Scans 1633, 1634, 1635; Background Corrected with Scan 1628

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.0	93261	PASS
68	69	0.00	2	1.7	1260	PASS
69	198	0.00	100	34.3	72536	PASS
70	69	0.00	2	0.5	329	PASS
127	198	10	80	43.7	92579	PASS
197	198	0.00	2	0.4	874	PASS
198	198	100	100	100.0	211776	PASS
199	198	5	9	7.0	14906	PASS
275	198	10	60	27.7	58715	PASS
365	198	1	100	3.5	7431	PASS
441	198	0.01	100	16.2	34391	PASS
442	442	50	100	100.0	211571	PASS
443	442	15	24	19.1	40365	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082321\
 Data File : BF125157.D
 Acq On : 23 Aug 2021 16:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 24 06:27:18 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 23 10:15:49 2021
 Response via : Initial Calibration

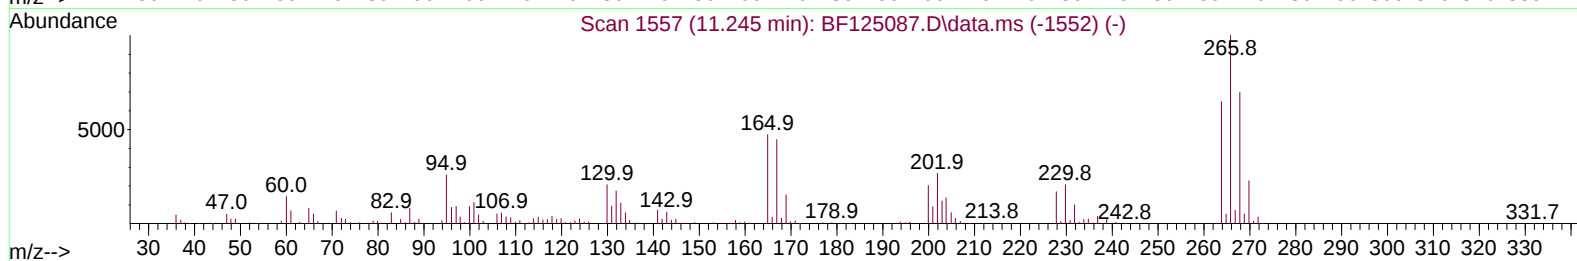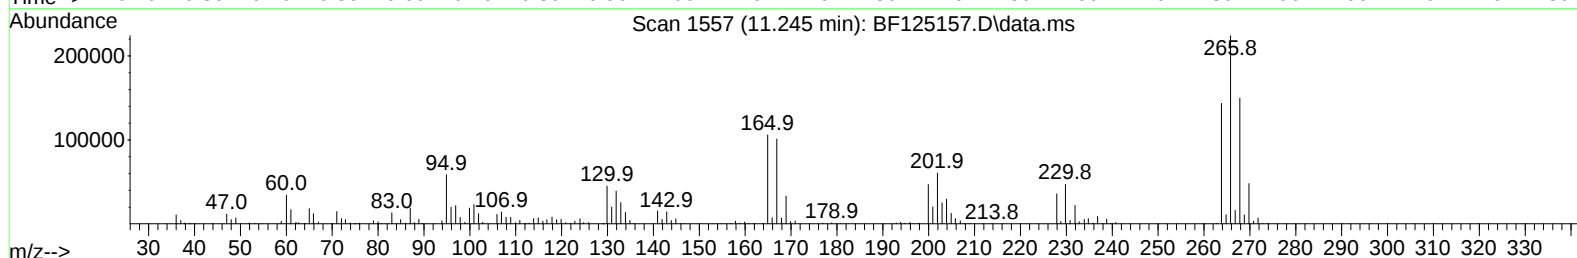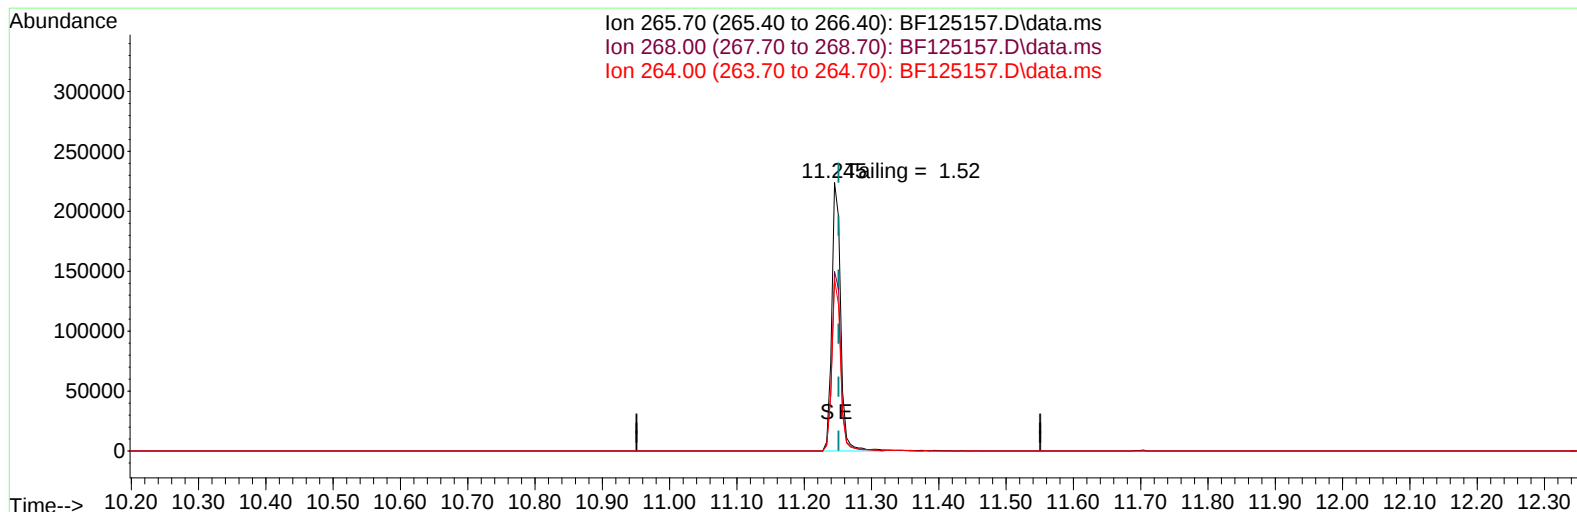

TIC: BF125157.D\data.ms

(70) Pentachlorophenol (C)

11.245min (-0.006) 106838.96 ng




response 206530

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	66.85
264.00	69.90	64.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082321\
Data File : BF125157.D
Acq On : 23 Aug 2021 16:11
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 24 06:27:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 10:15:49 2021
Response via : Initial Calibration

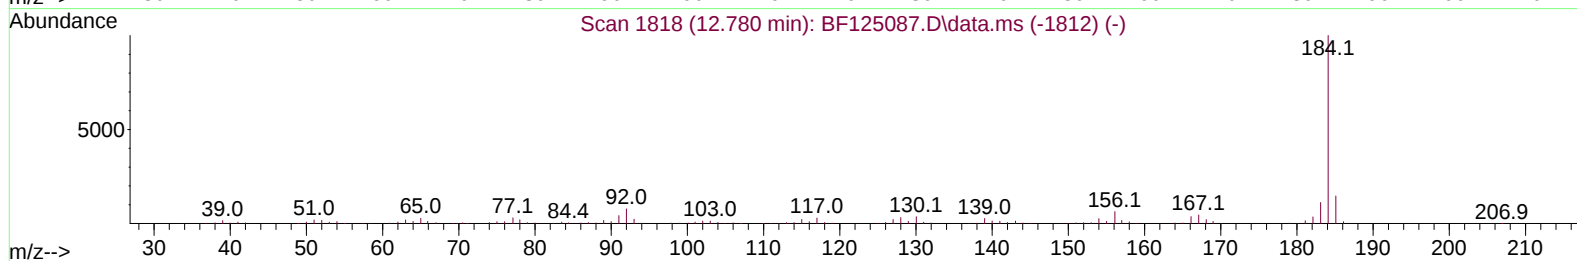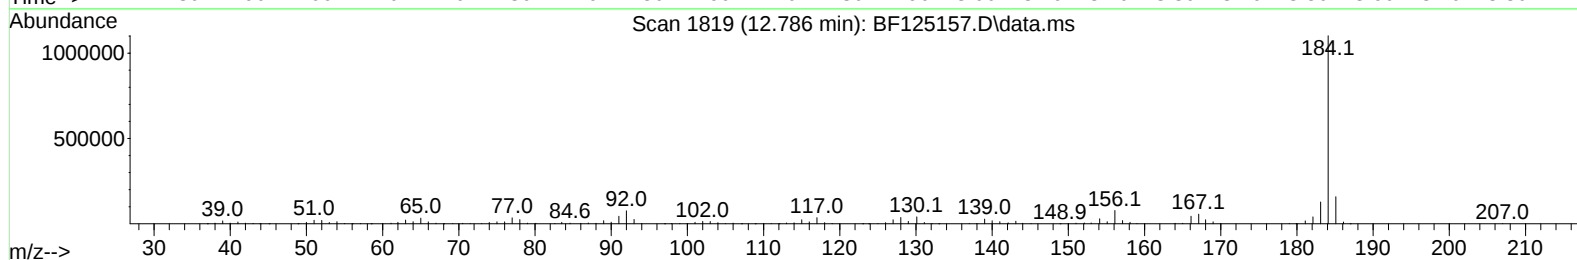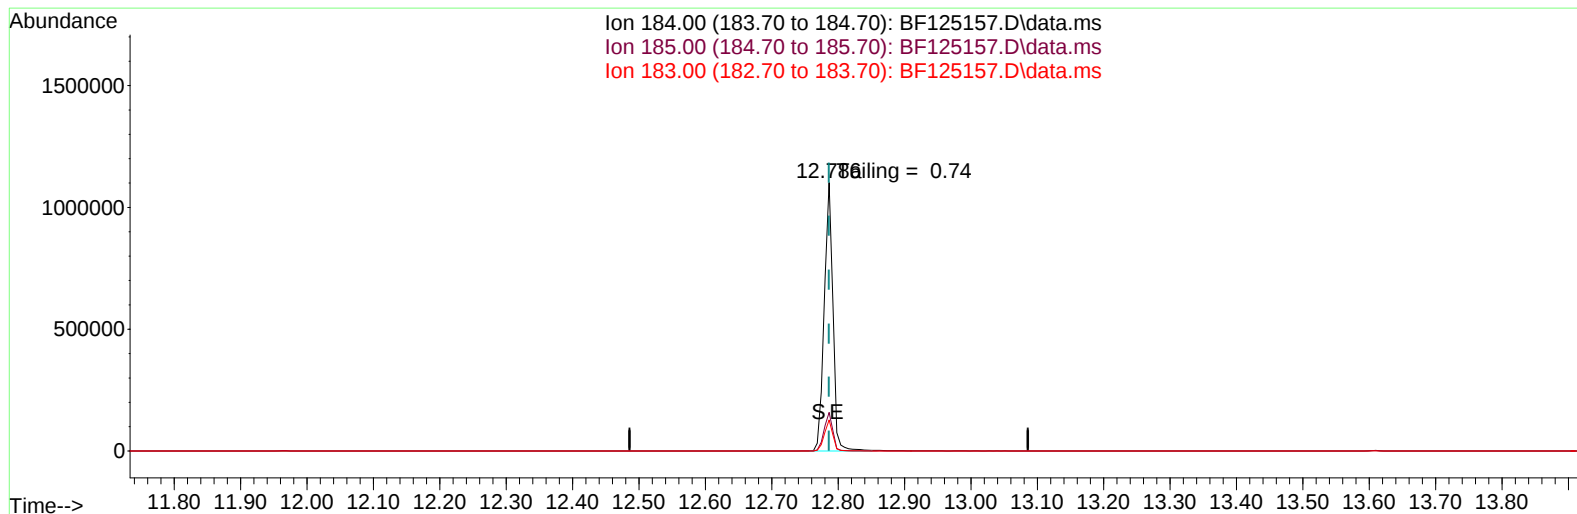

TIC: BF125157.D\data.ms

(77) Benzidine

12.786min (+ 0.000) 82747.36 ng

response 1011477

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.38
183.00	10.10	11.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/23/2021	BNA_F	<u>BF125157.D</u>
Compound Name	Response	Retention Time
DDT	469038	13.61
DDD	9162	13.304
DDE	1366	12.969
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10528	479566	2.20

Instrument :
BNA_F
ClientSampleId :
DFTPP