
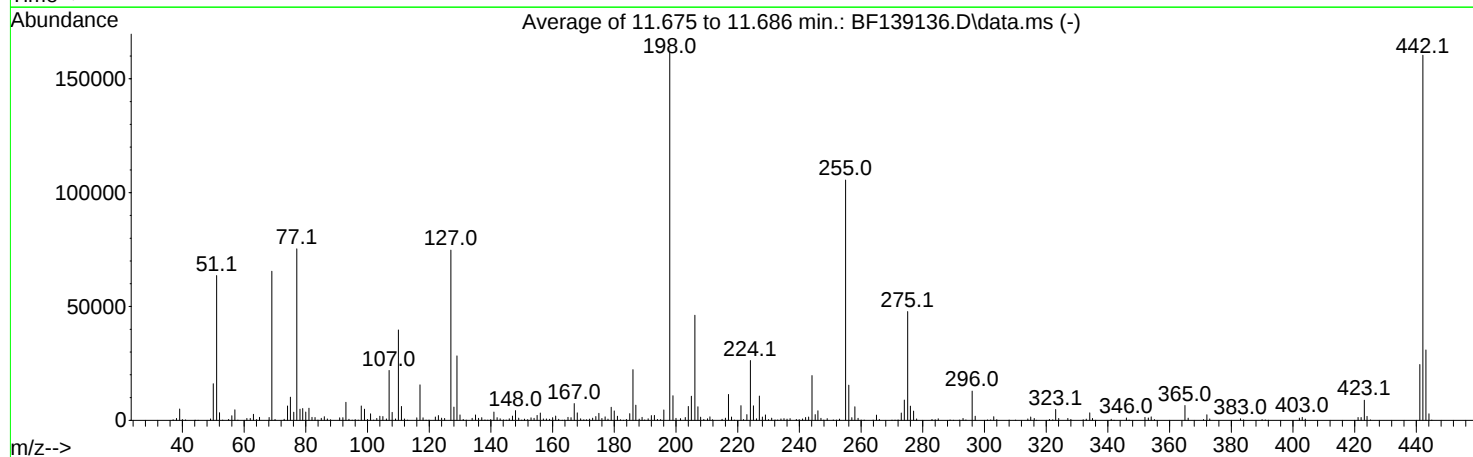


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082324\
Data File : BF139136.D
Acq On : 23 Aug 2024 09:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 21 01:25:05 2024

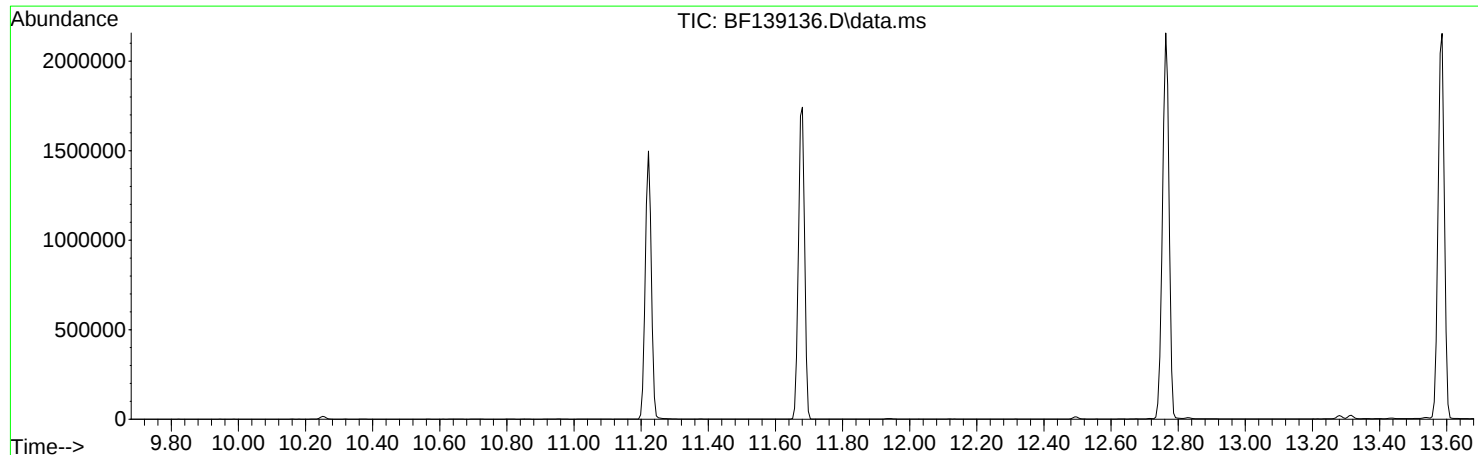

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.3	63568	PASS
68	69	0.00	2	1.9	1260	PASS
69	198	0.00	100	40.5	65475	PASS
70	69	0.00	2	0.6	407	PASS
127	198	10	80	46.3	74800	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	161560	PASS
199	198	5	9	6.7	10815	PASS
275	198	10	60	29.6	47789	PASS
365	198	1	100	4.0	6509	PASS
441	198	0.01	100	15.2	24523	PASS
442	442	50	100	100.0	160384	PASS
443	442	15	24	19.3	30925	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/23/2024	BNA_F	<u>BF139136.D</u>
Compound Name	Response	Retention Time
DDT	538322	13.586
DDD	10400	13.28
DDE	246	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10646	548968	1.94

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082324\
Data File : BF139136.D
Acq On : 23 Aug 2024 09:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 23 20:11:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

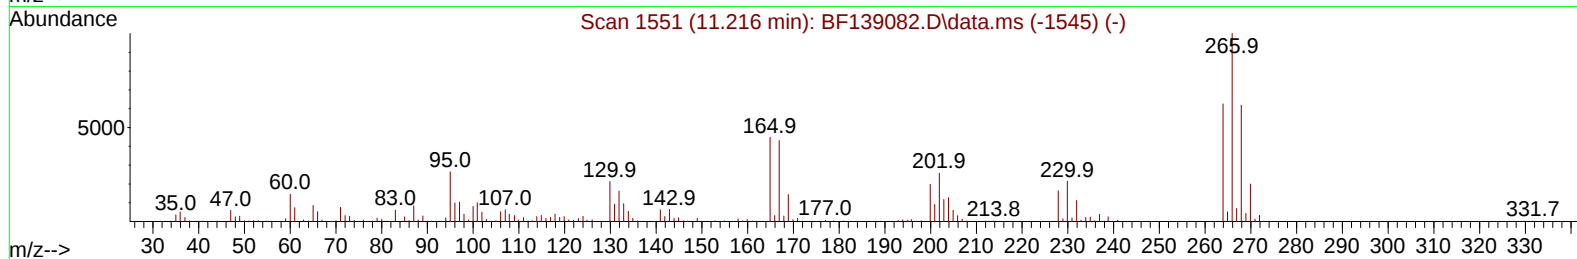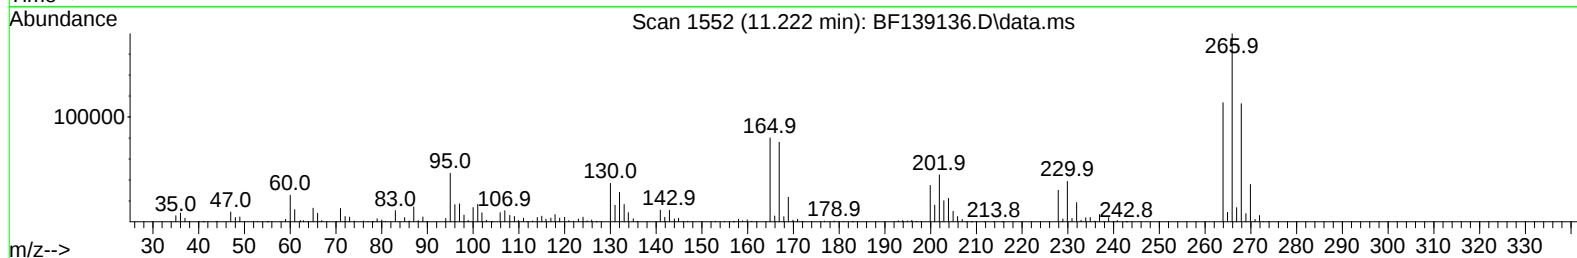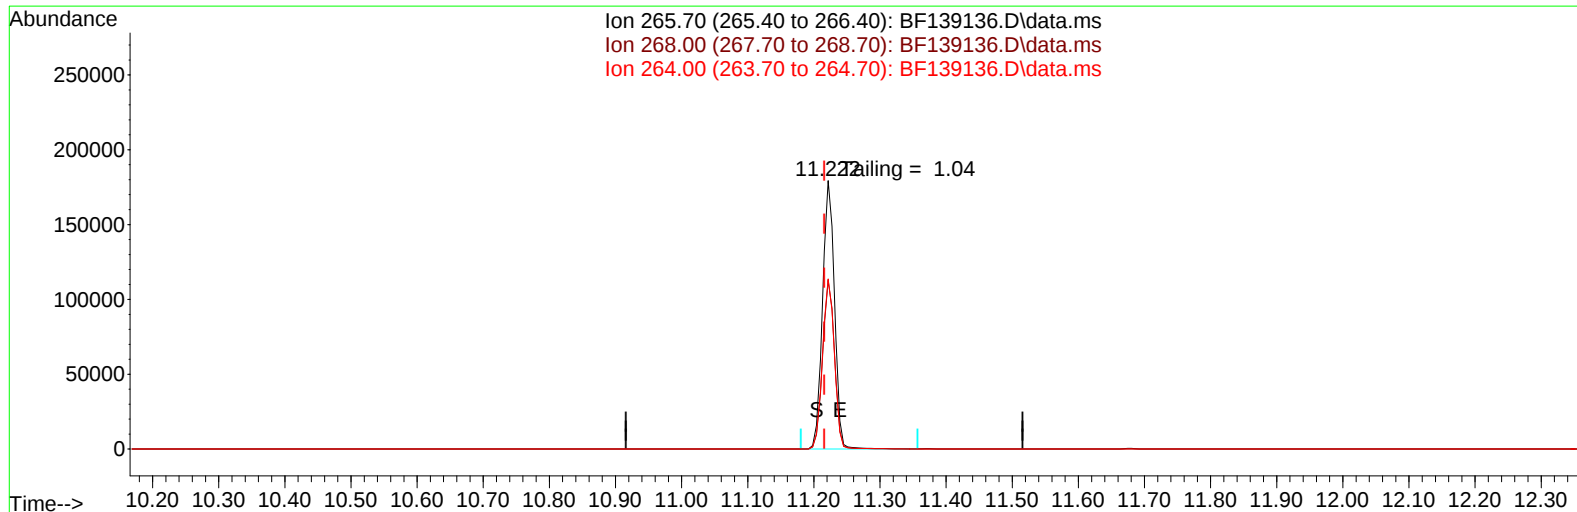

TIC: BF139136.D\data.ms

(70) Pentachlorophenol (C)

11.222min (+ 0.006) 38019.28 ng




response 226665

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	62.82
264.00	62.50	63.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082324\
Data File : BF139136.D
Acq On : 23 Aug 2024 09:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 23 11:12:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 21 01:25:05 2024
Response via : Initial Calibration

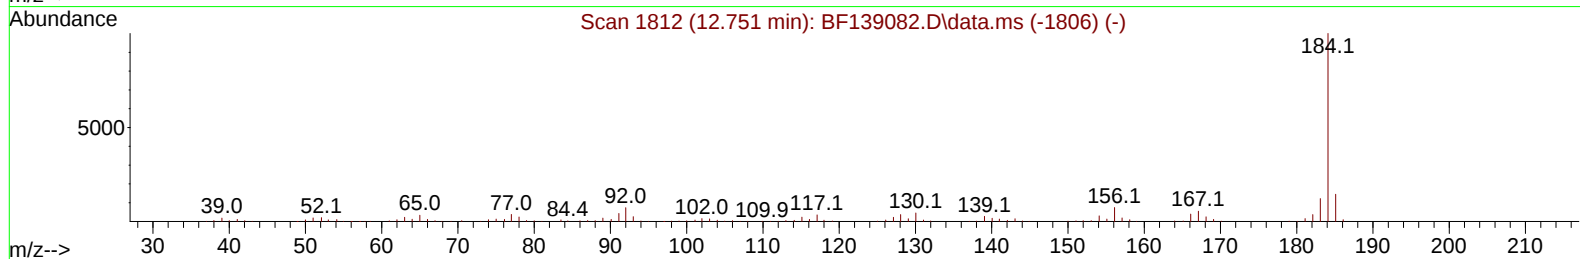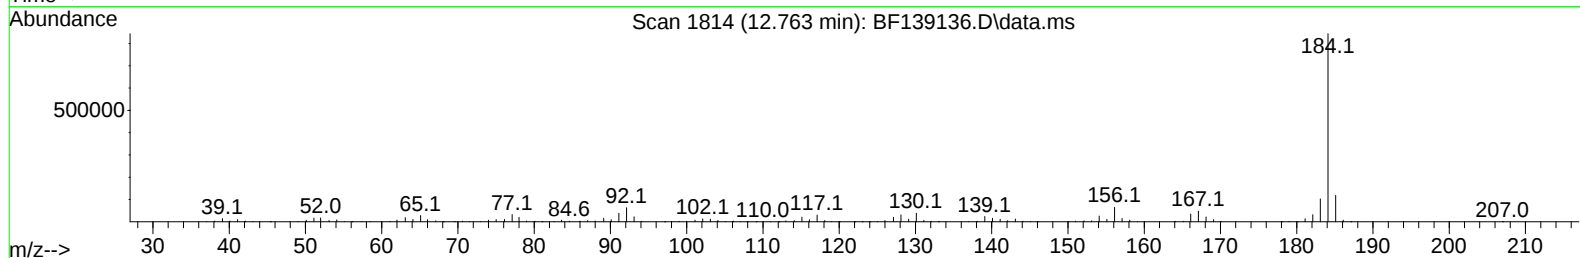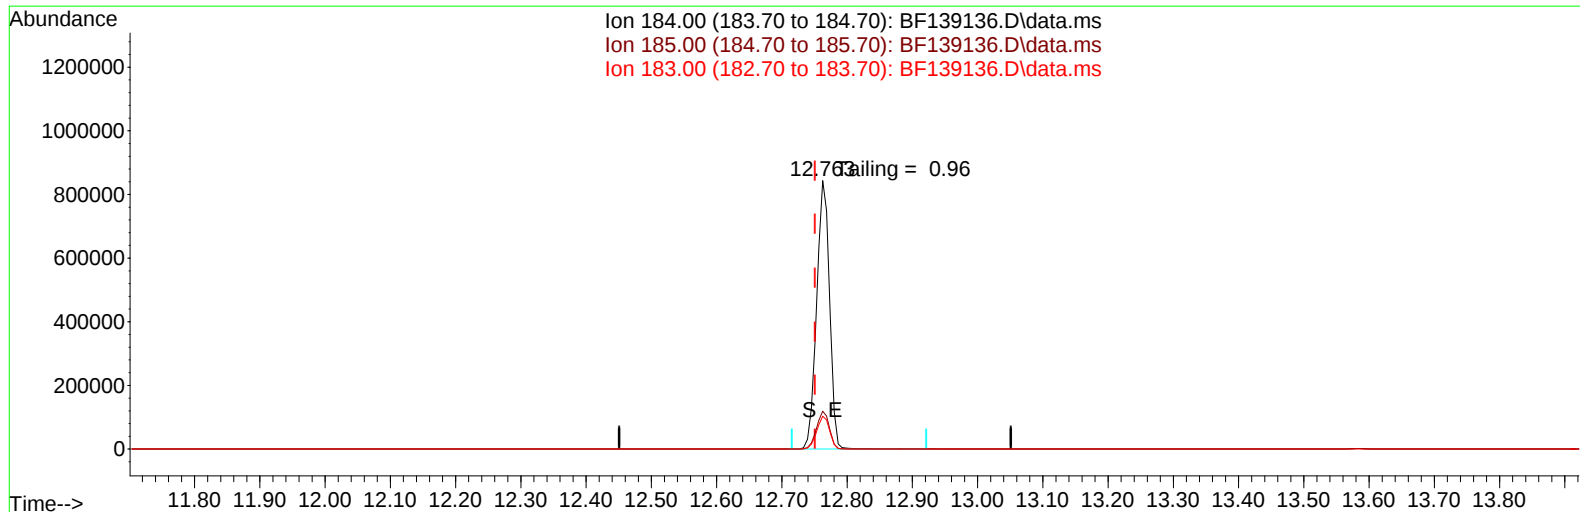

TIC: BF139136.D\data.ms

(77) Benzidine

12.763min (+ 0.012) 0.00 ng

response 1161177

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.08
183.00	12.20	12.21
0.00	0.00	0.00