
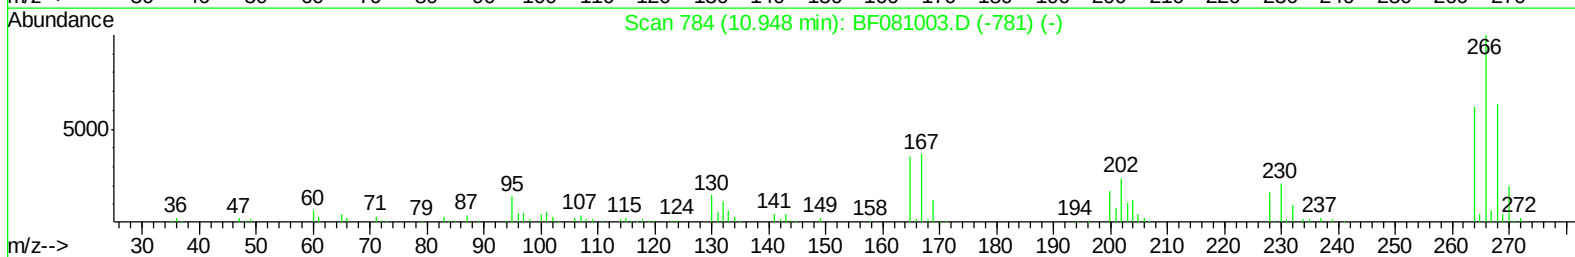
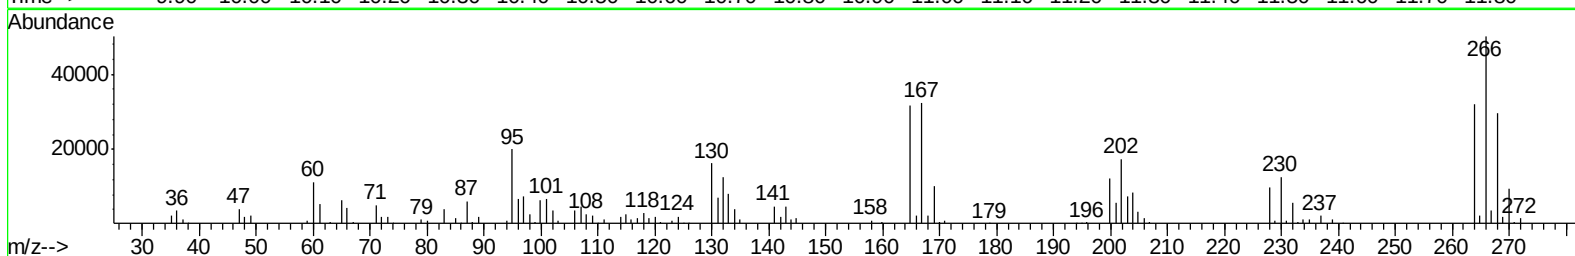


Data Path : Z:\HPCHEM1\BNA_F\Data\BF082415\
Data File : BF081161.D
Acq On : 24 Aug 2015 10:31
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 01:15:21 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 24 13:58:19 2015
Response via : Initial Calibration

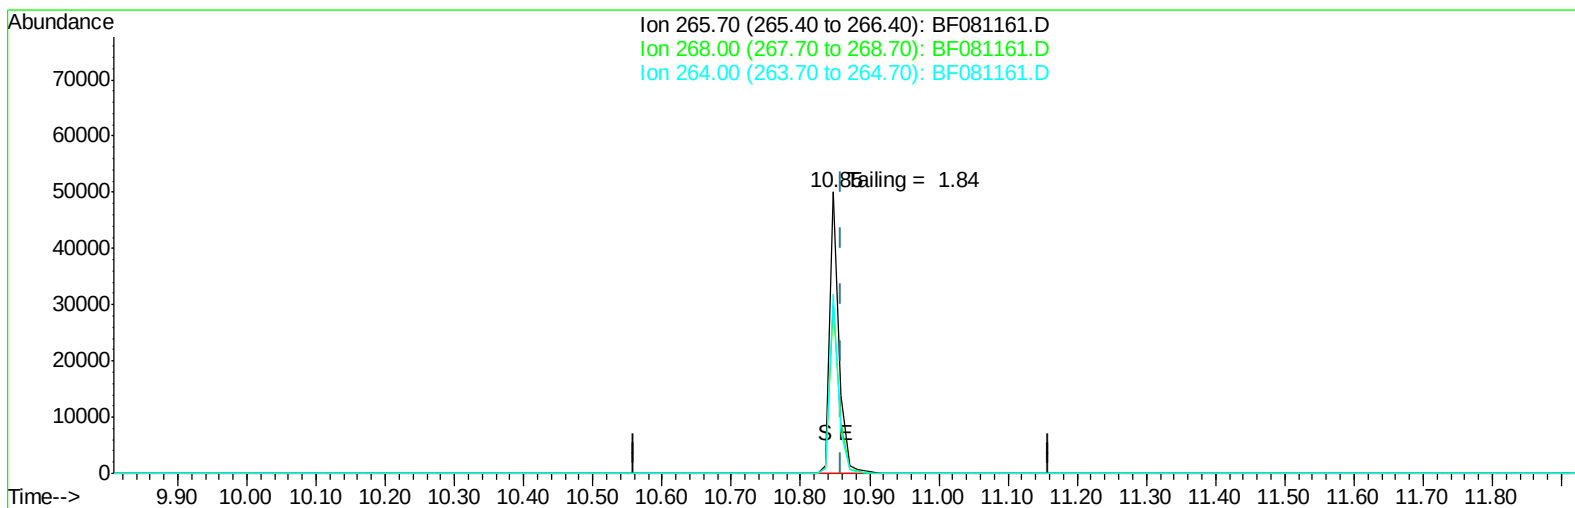

TIC: BF081161.D

(69) Pentachlorophenol (C)




10.848min (-0.011) 0.00ng

response 46702

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	59.38
264.00	63.20	63.83
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF082415\
Data File : BF081161.D
Acq On : 24 Aug 2015 10:31
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 01:15:21 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 24 13:58:19 2015
Response via : Initial Calibration

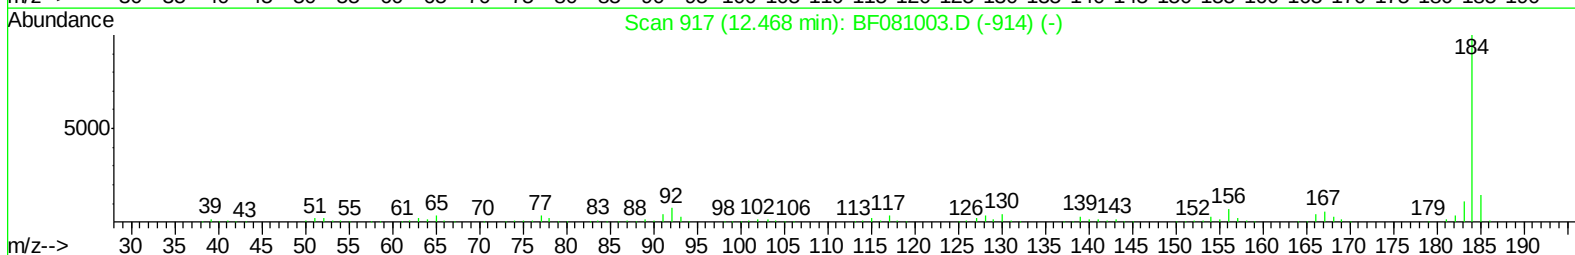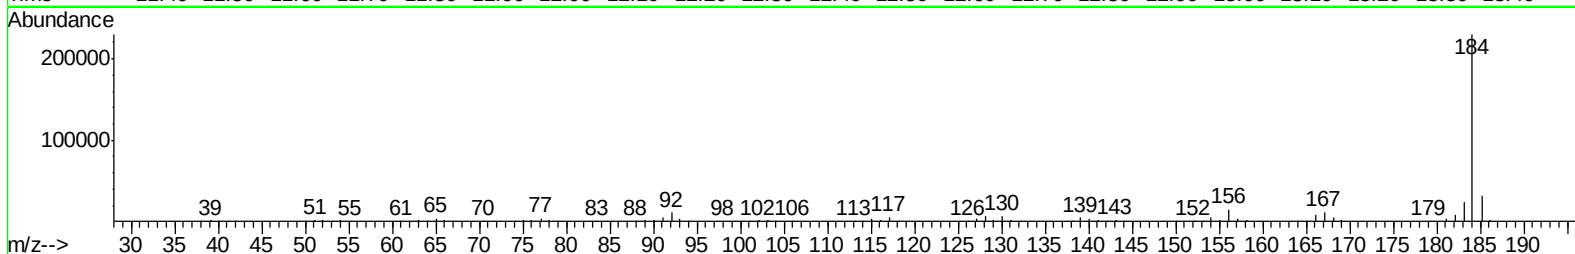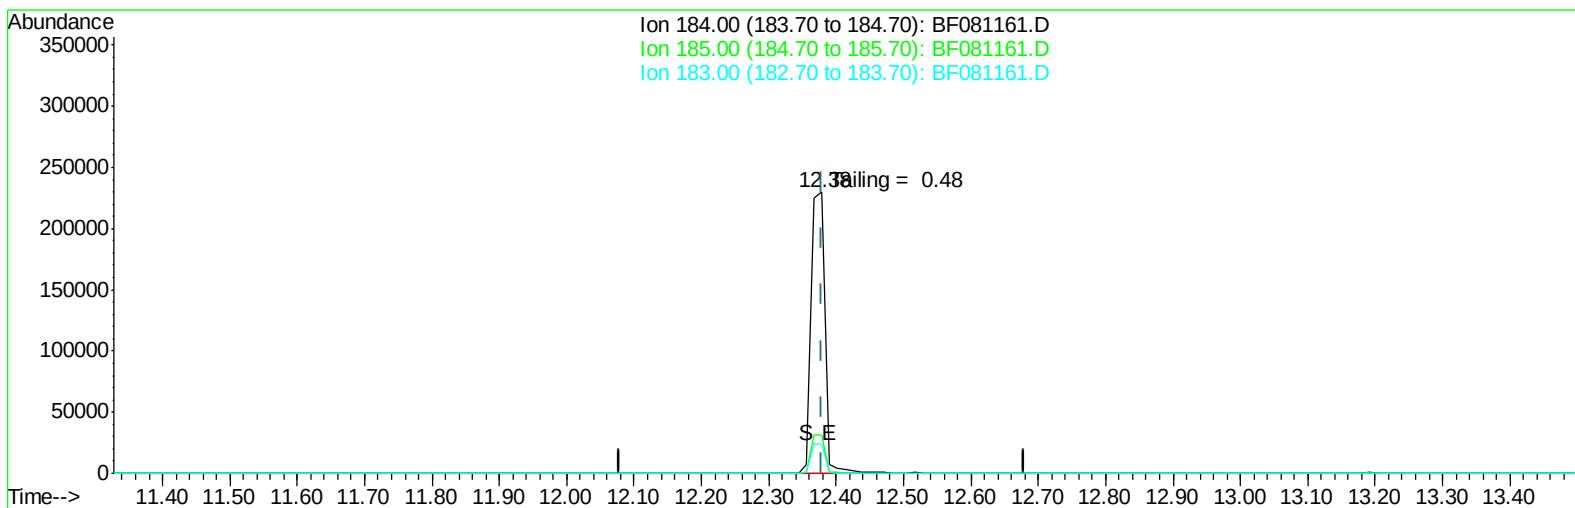

TIC: BF081161.D

(76) Benzidine

12.379min (-0.000) 0.00ng

response 330700

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	13.58
183.00	11.10	10.67
0.00	0.00	0.00