

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082415\
 Data File : BF081185.D
 Acq On : 25 Aug 2015 00:08
 Operator : UM/IZ
 Sample : G3386-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P001-BF003-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.642	238	241	254	rVB	602915	994038	63.84%	7.013%
2	5.110	279	282	284	rBV	1287585	1498511	96.23%	10.571%
3	5.533	316	319	321	rBV	20846	18454	1.19%	0.130%
4	6.185	373	376	379	rBV	1373178	1349979	86.70%	9.524%
5	6.299	384	386	389	rBV	1130017	1358800	87.26%	9.586%
6	6.539	405	407	409	rBV	502521	408416	26.23%	2.881%
7	6.699	418	421	423	rBV	960221	1042127	66.93%	7.352%
8	7.110	454	457	459	rBV	1061182	1006753	64.65%	7.102%
9	7.819	517	519	522	rBV	365000	484291	31.10%	3.416%
10	8.905	611	614	616	rBV	1734868	1557148	100.00%	10.985%
11	9.305	647	649	651	rBV	263225	233861	15.02%	1.650%
12	9.568	669	672	674	rBV	634469	547770	35.18%	3.864%
13	10.345	738	740	743	rBV2	758186	809572	51.99%	5.711%
14	10.494	751	753	757	rBV	28718	31794	2.04%	0.224%
15	10.939	787	792	793	rBV	19607	21247	1.36%	0.150%
16	11.031	798	800	803	rVV2	445242	530851	34.09%	3.745%
17	12.619	936	939	941	rBV	1559886	1388759	89.19%	9.797%
18	13.648	1027	1029	1031	rBV	594023	512614	32.92%	3.616%
19	14.505	1102	1104	1106	rBV	17019	16589	1.07%	0.117%
20	14.985	1143	1146	1148	rBV	258000	363549	23.35%	2.565%




Sum of corrected areas: 14175123

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082415\
Data File : BF081185.D
Acq On : 25 Aug 2015 00:08
Operator : UM/IZ
Sample : G3386-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-BF003-01

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

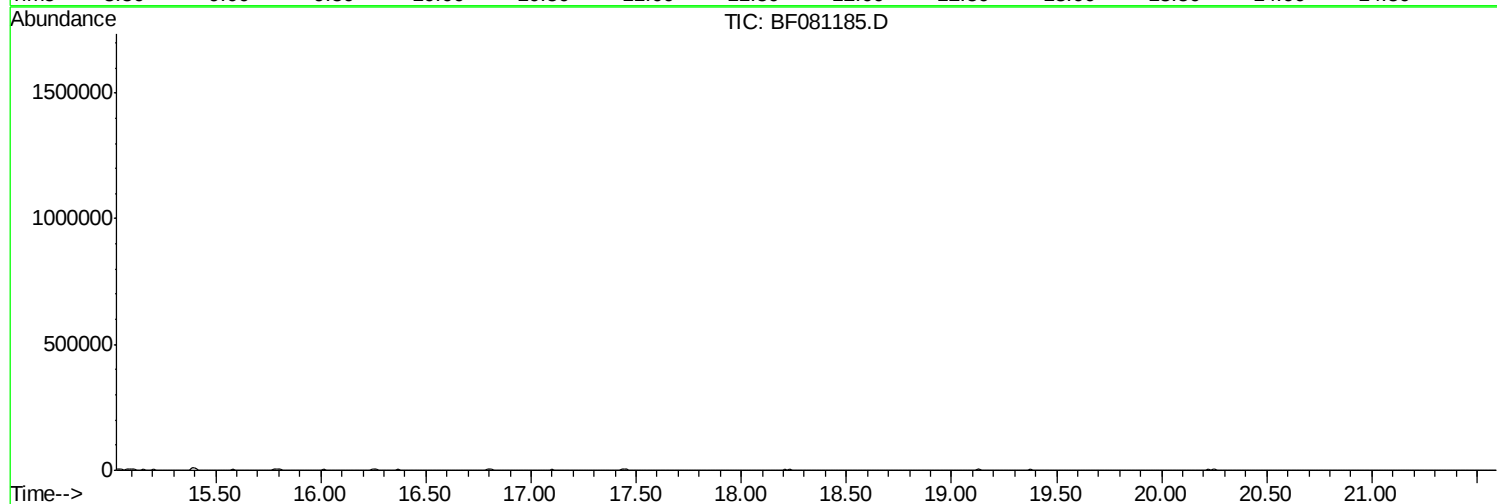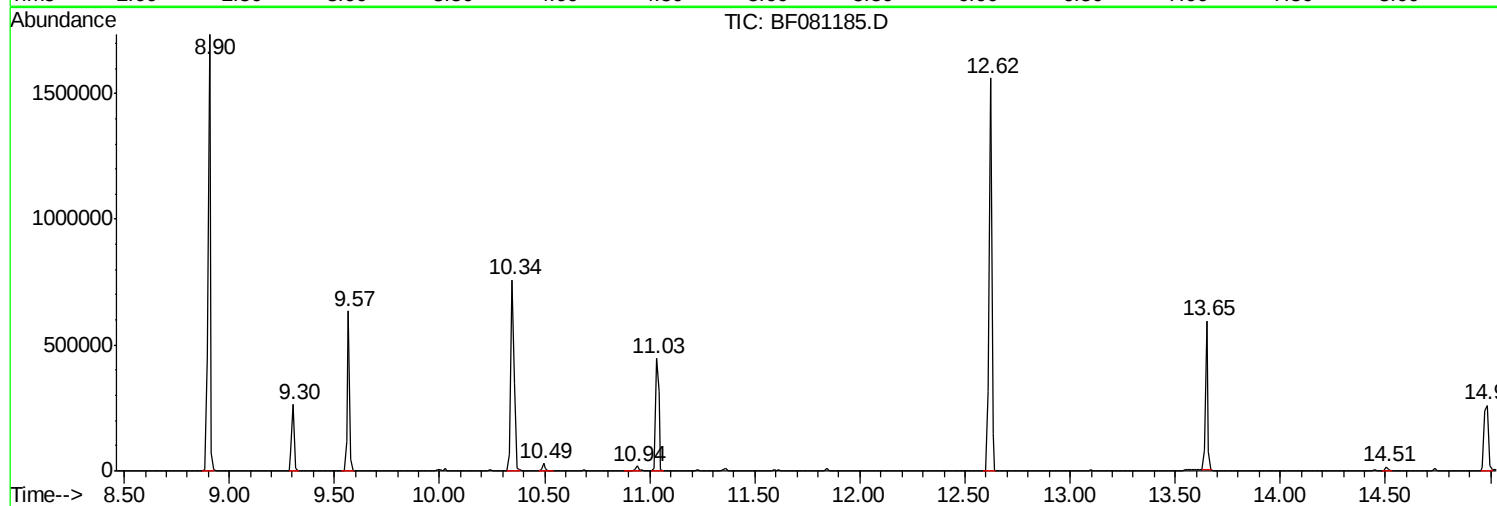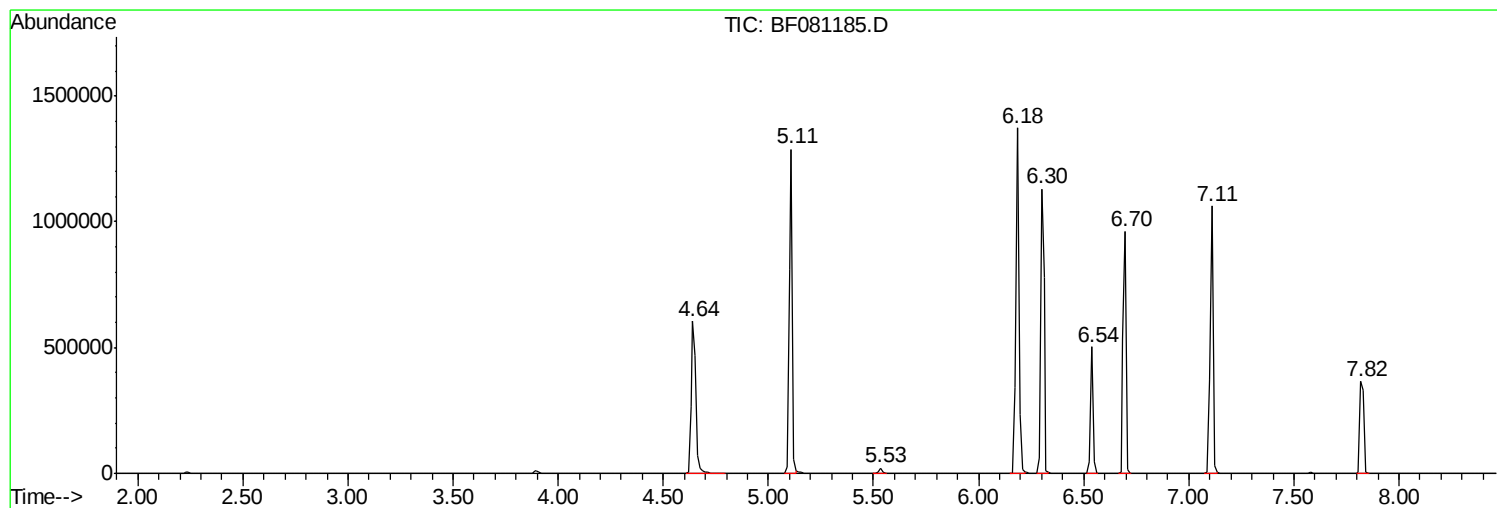

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082415\
Data File : BF081185.D
Acq On : 25 Aug 2015 00:08
Operator : UM/IZ
Sample : G3386-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-BF003-01










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.64	48.68 ng	994038	1,4-Dichlorobenzene-d4	6.54

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2			Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	42
3			3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33
4			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	33
5			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	32

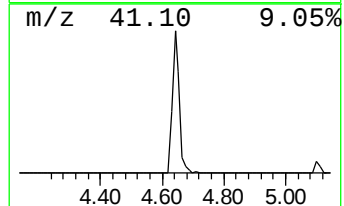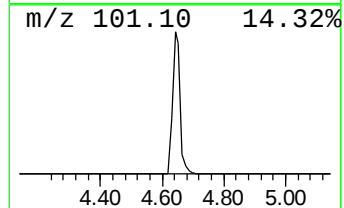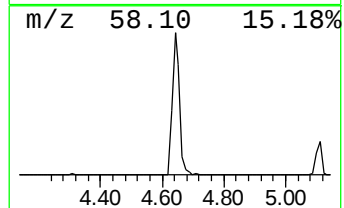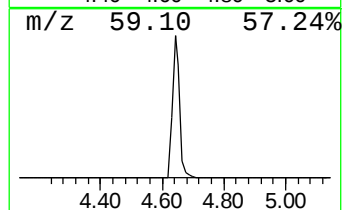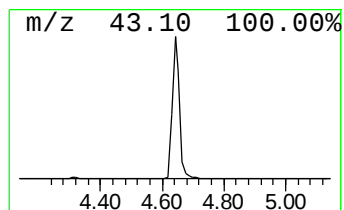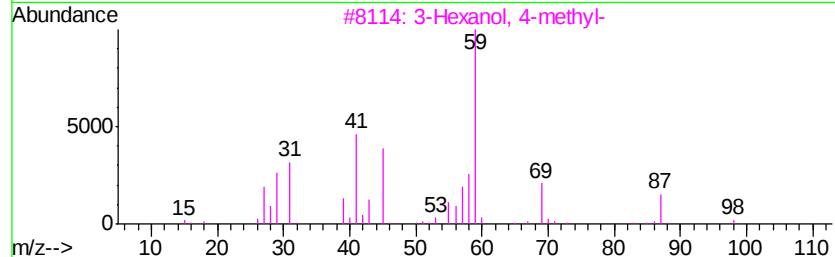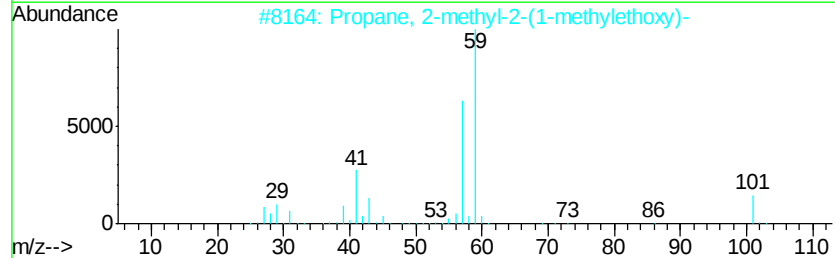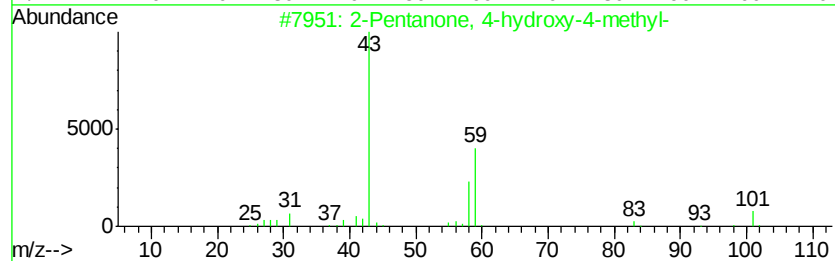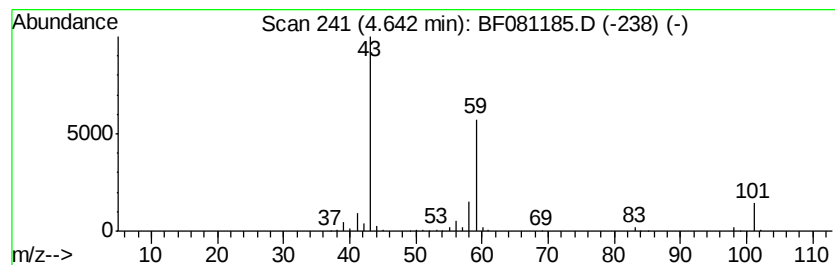

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082415\
Data File : BF081185.D
Acq On : 25 Aug 2015 00:08
Operator : UM/IZ
Sample : G3386-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-BF003-01










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.30 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.30	66.54 ng	1358800	1,4-Dichlorobenzene-d4	6.54

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
3		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12

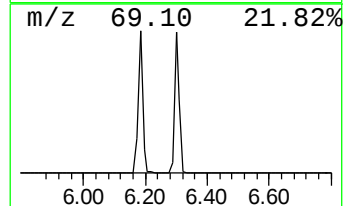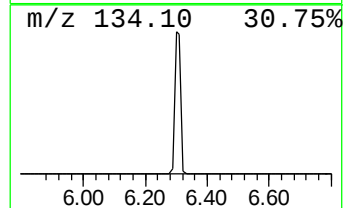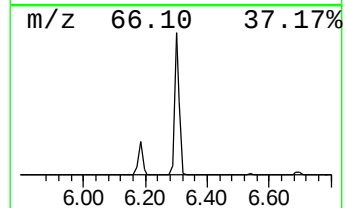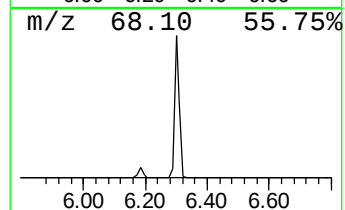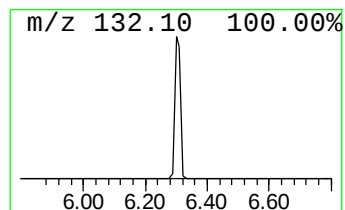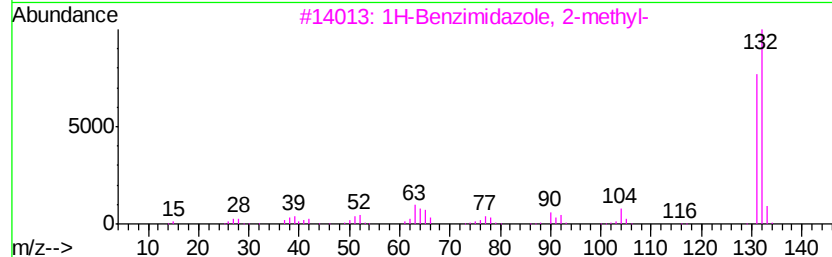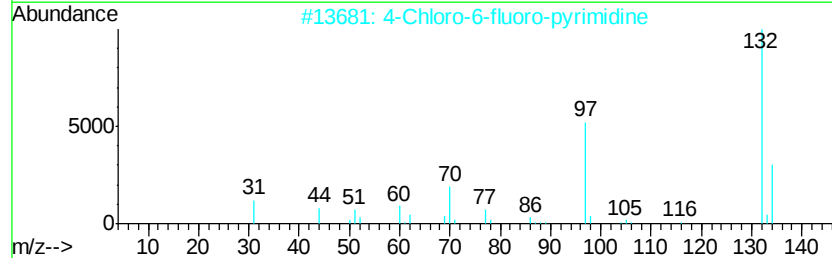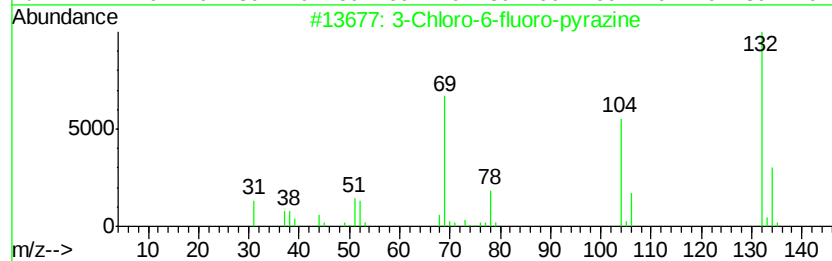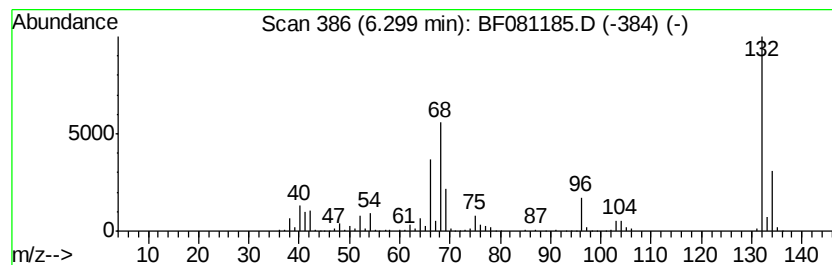

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082415\
Data File : BF081185.D
Acq On : 25 Aug 2015 00:08
Operator : UM/IZ
Sample : G3386-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-BF003-01

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.64	48.7	ng	994038	1	6.54	408416	20.0
unknown6.30	6.30	66.5	ng	1358800	1	6.54	408416	20.0