


Data Path : Z:\HPCHEM1\BNA_F\Data\BF082415\
 Data File : BF081161.D
 Acq On : 24 Aug 2015 10:31
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 24 13:58:19 2015

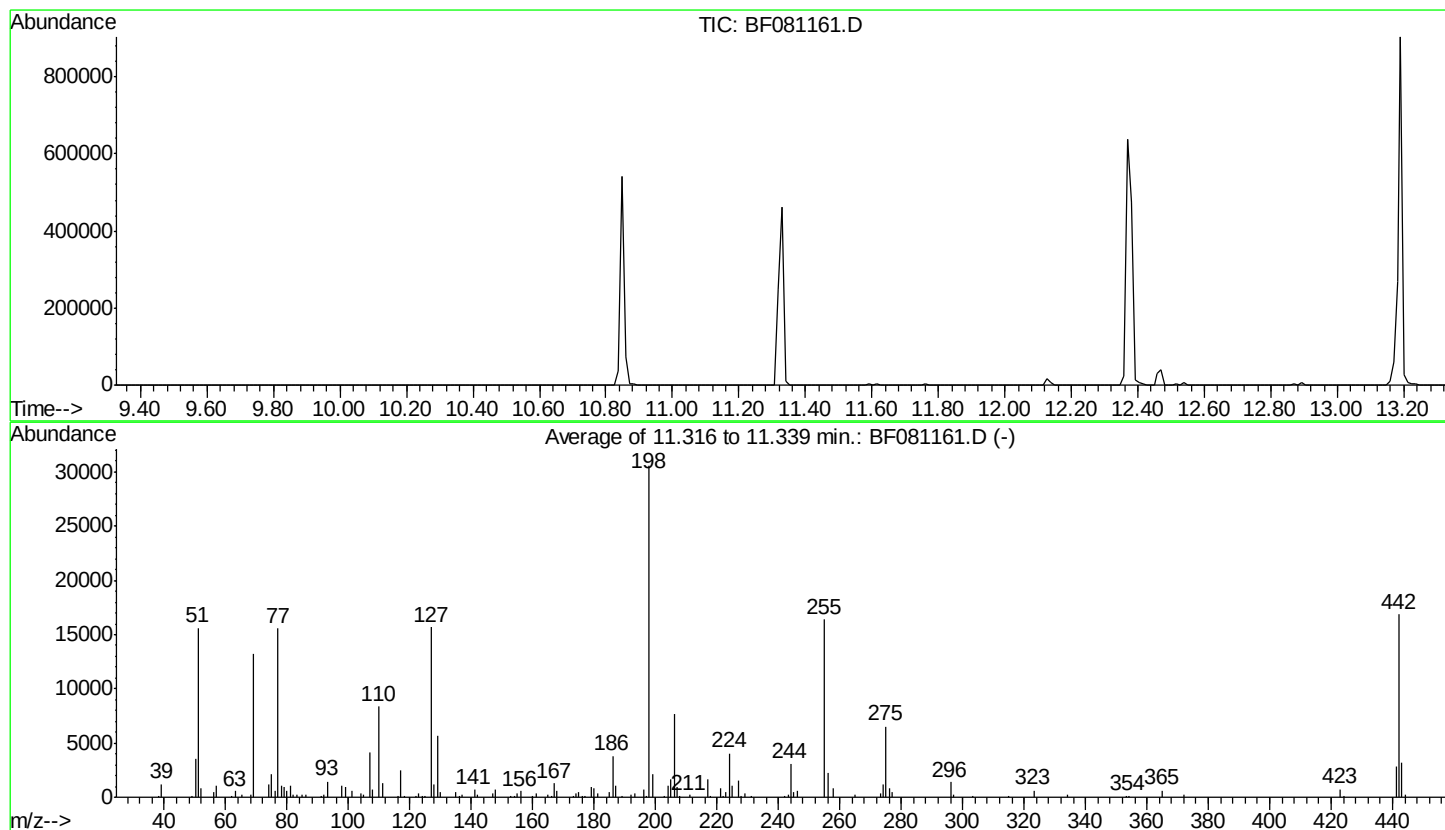

AutoFind: Scans 825, 826, 827; Background Corrected with Scan 822

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.1	15621	PASS
68	69	0.00	2	1.7	218	PASS
69	198	0.00	100	43.1	13181	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.3	15680	PASS
197	198	0.00	2	0.4	120	PASS
198	198	100	100	100.0	30582	PASS
199	198	5	9	7.0	2149	PASS
275	198	10	60	21.2	6494	PASS
365	198	1	100	1.9	591	PASS
441	442	0.01	24	17.0	2866	PASS
442	198	50	100	55.2	16870	PASS
443	442	15	24	18.6	3137	PASS