

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082416\
 Data File : BF089888.D
 Acq On : 24 Aug 2016 21:20
 Operator : UM/SJ
 Sample : H4577-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FB01-081816

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.655	5	6	14	rVV	245763	450118	3.41%	0.483%
2	1.770	14	16	50	rVB	3657314	7324341	55.51%	7.860%
3	4.787	278	280	290	rVB	665253	833457	6.32%	0.894%
4	5.233	316	319	322	rBV	4589950	4873633	36.93%	5.230%
5	6.296	410	412	414	rBV	3988339	3144553	23.83%	3.375%
6	6.433	421	424	426	rBV	9295105	9727005	73.71%	10.438%
7	6.662	442	444	447	rBV	2582705	2436741	18.47%	2.615%
8	6.822	455	458	461	rBV	9644294	8369695	63.43%	8.982%
9	7.233	491	494	496	rBV	6630225	6351960	48.14%	6.817%
10	7.953	555	557	559	rVB	4123245	3459123	26.21%	3.712%
11	9.039	649	652	654	rBV	12730095	13195579	100.00%	14.161%
12	9.702	708	710	713	rBV	4491727	3830394	29.03%	4.111%
13	10.491	776	779	781	rBV	7009673	7392245	56.02%	7.933%
14	11.176	837	839	842	rBV	4070246	3603315	27.31%	3.867%
15	12.777	976	979	981	rBV	10453049	12847715	97.36%	13.787%
16	13.817	1068	1070	1073	rBV	3148837	3042733	23.06%	3.265%
17	15.257	1193	1196	1199	rBV	2002966	2302388	17.45%	2.471%


Sum of corrected areas: 93184995

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082416\
Data File : BF089888.D
Acq On : 24 Aug 2016 21:20
Operator : UM/SJ
Sample : H4577-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB01-081816

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

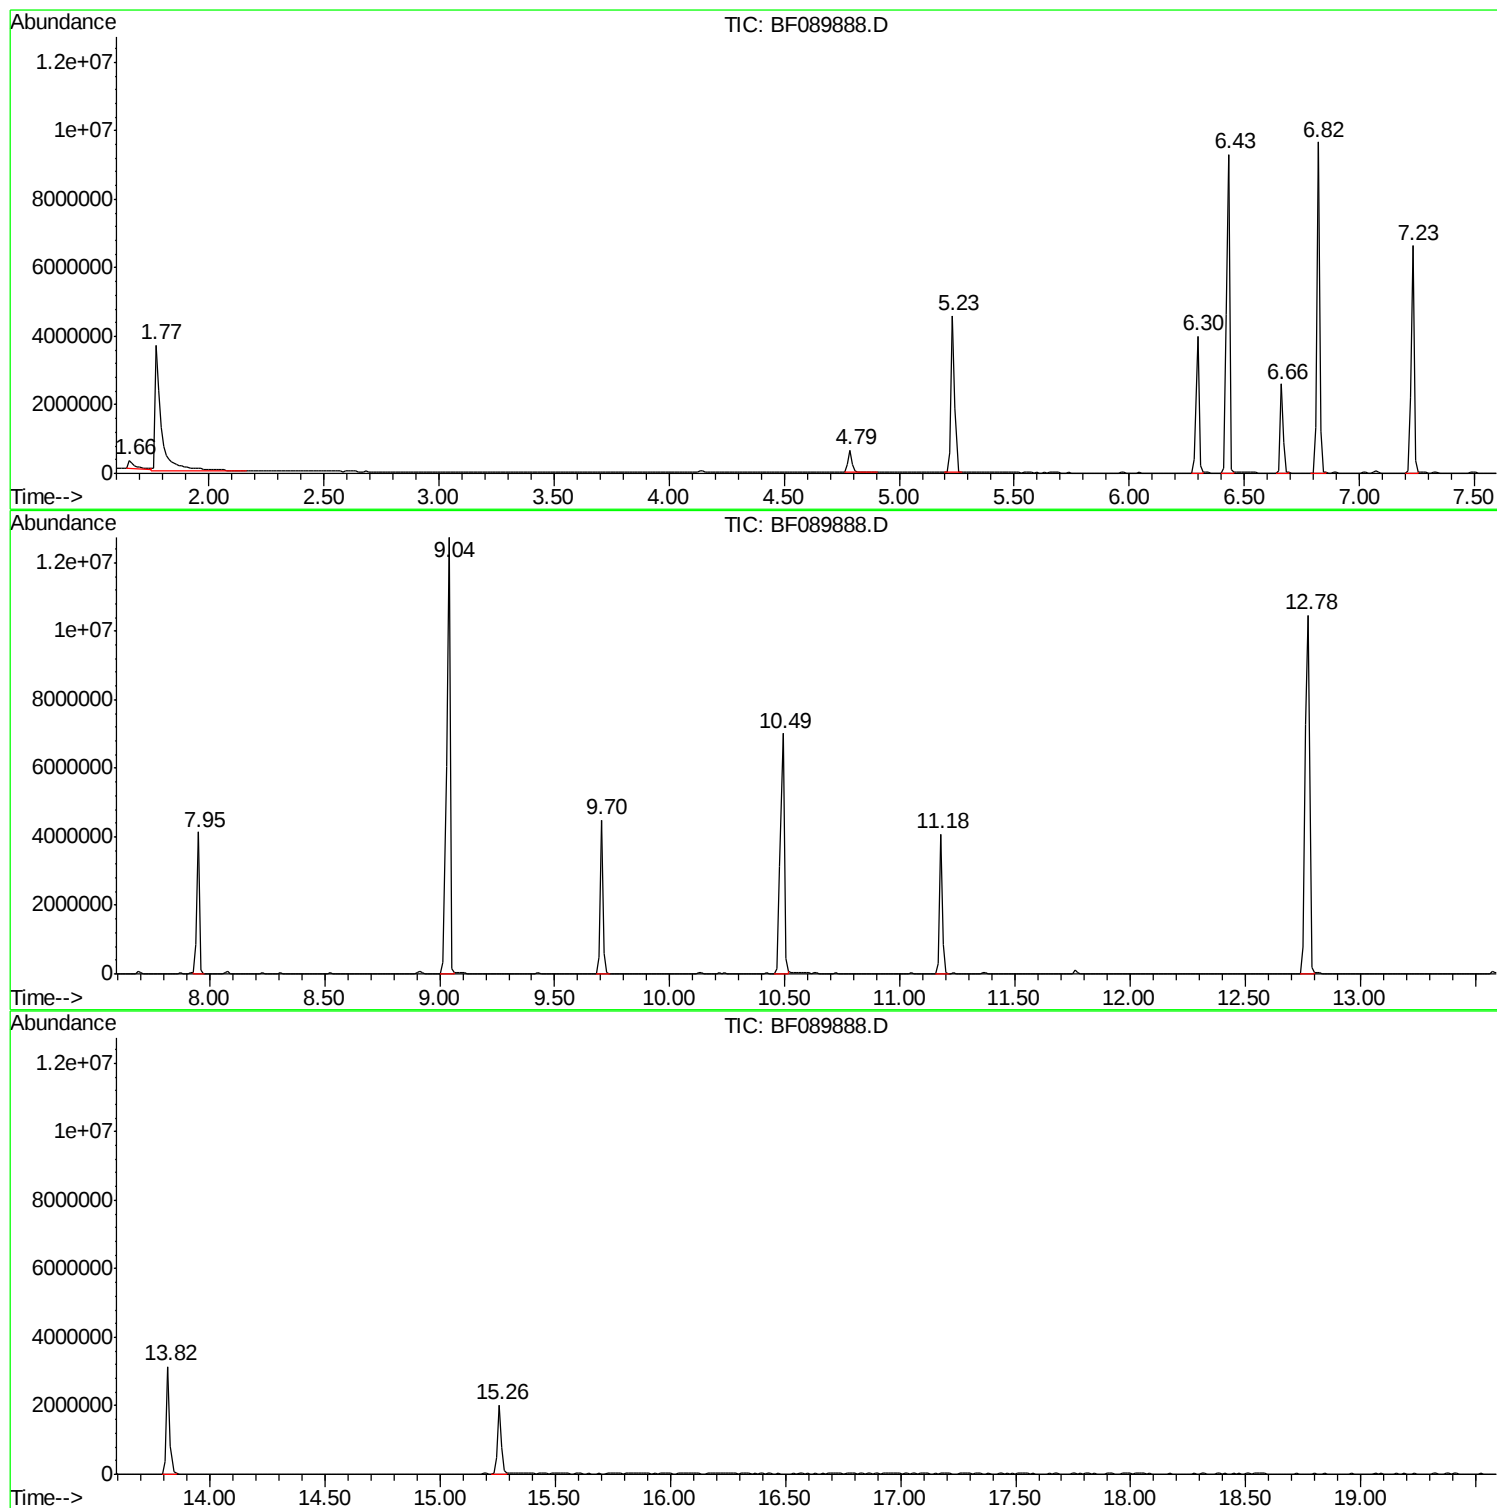

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082416\
Data File : BF089888.D
Acq On : 24 Aug 2016 21:20
Operator : UM/SJ
Sample : H4577-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB01-081816









Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.79	6.84 ng	833457	1,4-Dichlorobenzene-d4	6.66

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2			Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	25
3			Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9
4			5-Hexen-2-one	98	C6H10O	000109-49-9	9
5			(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9

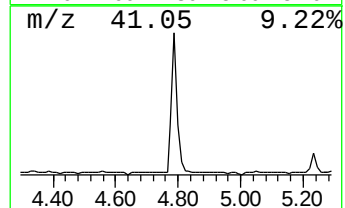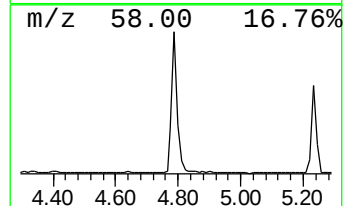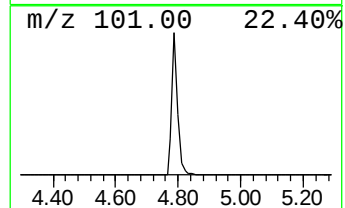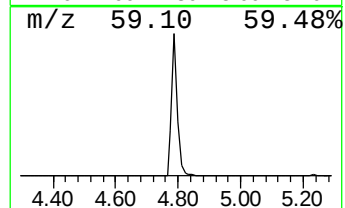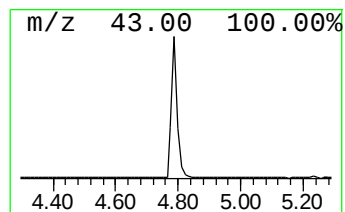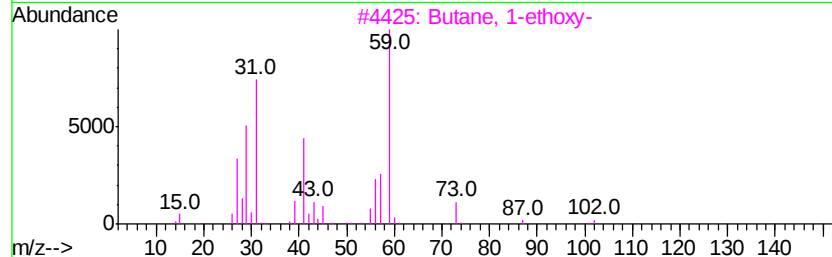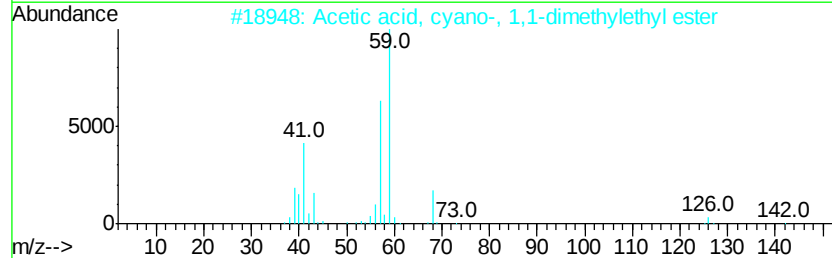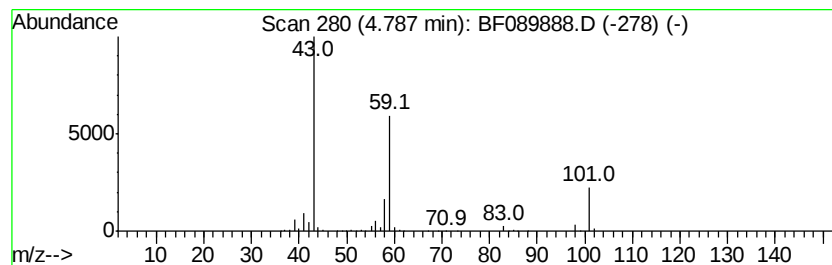

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082416\
Data File : BF089888.D
Acq On : 24 Aug 2016 21:20
Operator : UM/SJ
Sample : H4577-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB01-081816









Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown6.43 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.43	79.84 ng	9727010	1,4-Dichlorobenzene-d4	6.66

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	12
4		Amphetaminil	250	C17H18N2	017590-01-1	12
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

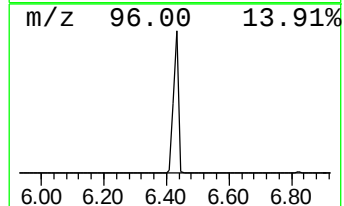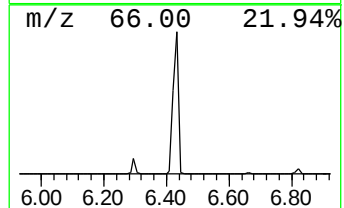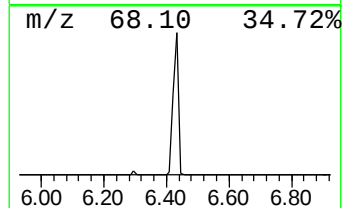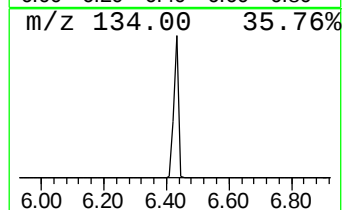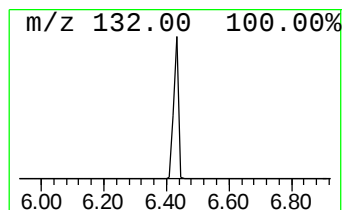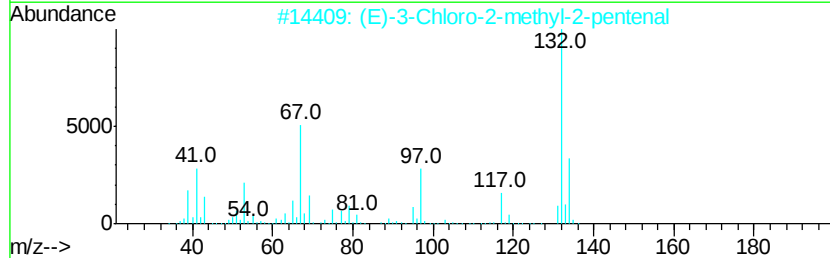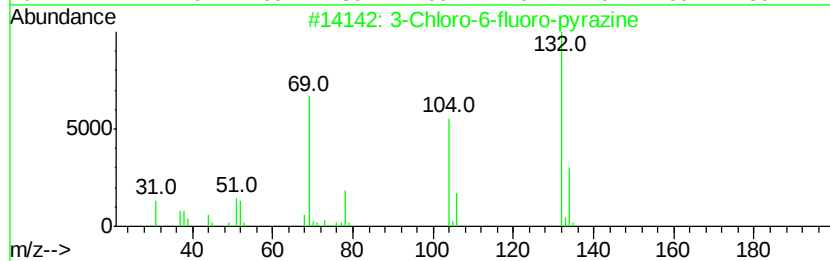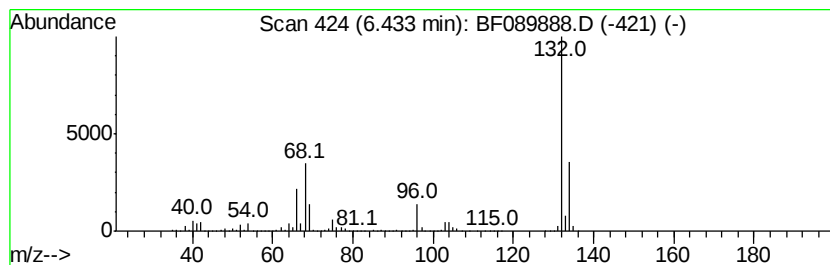

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082416\
Data File : BF089888.D
Acq On : 24 Aug 2016 21:20
Operator : UM/SJ
Sample : H4577-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB01-081816

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.79	6.8	ng	833457	1	6.66	2436740	20.0
unknown6.43	6.43	79.8	ng	9727010	1	6.66	2436740	20.0