


Data Path : Z:\HPCHEM1\BNA F\Data\BF082416\
 Data File : BF089864.D
 Acq On : 24 Aug 2016 10:37
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 19 14:02:57 2016

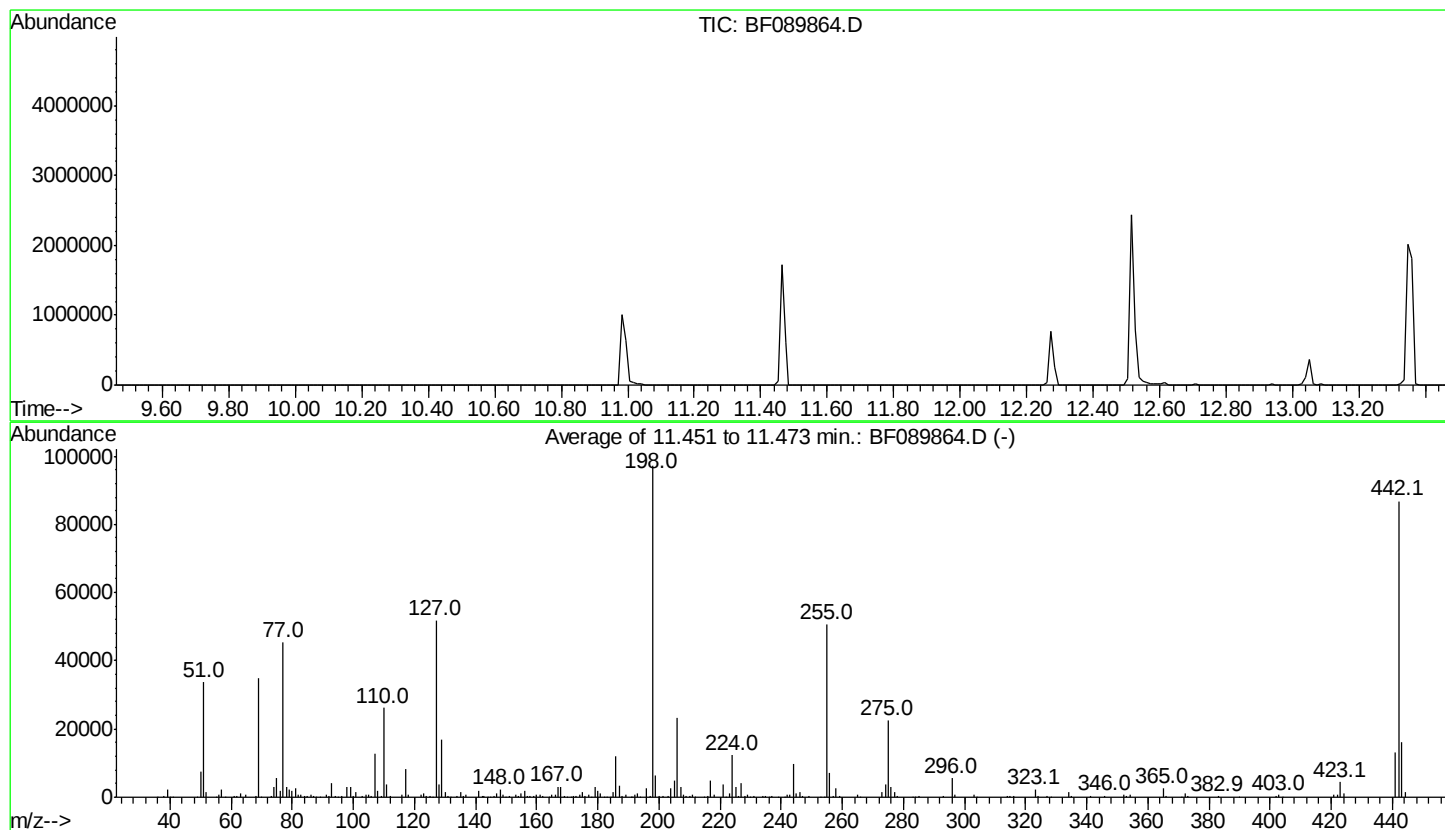

AutoFind: Scans 863, 864, 865; Background Corrected with Scan 860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	33747	PASS
68	69	0.00	2	1.6	553	PASS
69	198	0.00	100	36.0	34950	PASS
70	69	0.00	2	0.5	167	PASS
127	198	10	80	53.2	51715	PASS
197	198	0.00	2	0.4	355	PASS
198	198	100	100	100.0	97206	PASS
199	198	5	9	6.8	6562	PASS
275	198	10	60	23.0	22343	PASS
365	198	1	100	2.6	2531	PASS
441	442	0.01	24	15.4	13328	PASS
442	198	50	100	89.2	86728	PASS
443	442	15	24	18.8	16335	PASS