


Data Path : Z:\HPCHEM1\BNA F\DATA\BF082416\
 Data File : BF089891.D
 Acq On : 25 Aug 2016 00:13
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 19 14:02:57 2016

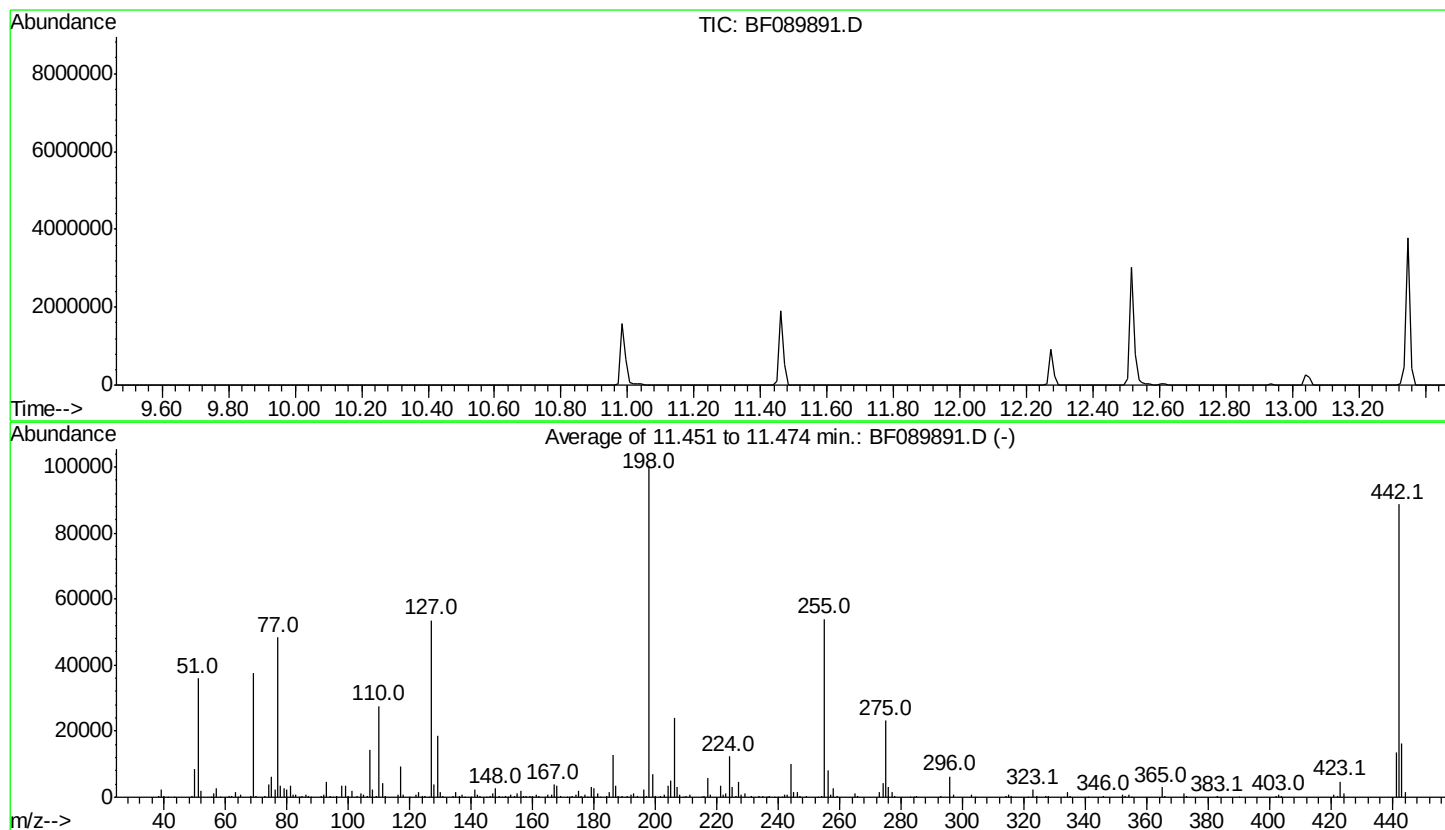

AutoFind: Scans 863, 864, 865; Background Corrected with Scan 860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	35912	PASS
68	69	0.00	2	1.4	509	PASS
69	198	0.00	100	37.5	37657	PASS
70	69	0.00	2	0.6	212	PASS
127	198	10	80	53.3	53493	PASS
197	198	0.00	2	0.4	432	PASS
198	198	100	100	100.0	100379	PASS
199	198	5	9	6.9	6917	PASS
275	198	10	60	23.0	23079	PASS
365	198	1	100	3.0	3018	PASS
441	442	0.01	24	15.3	13568	PASS
442	198	50	100	88.2	88581	PASS
443	442	15	24	18.6	16442	PASS