
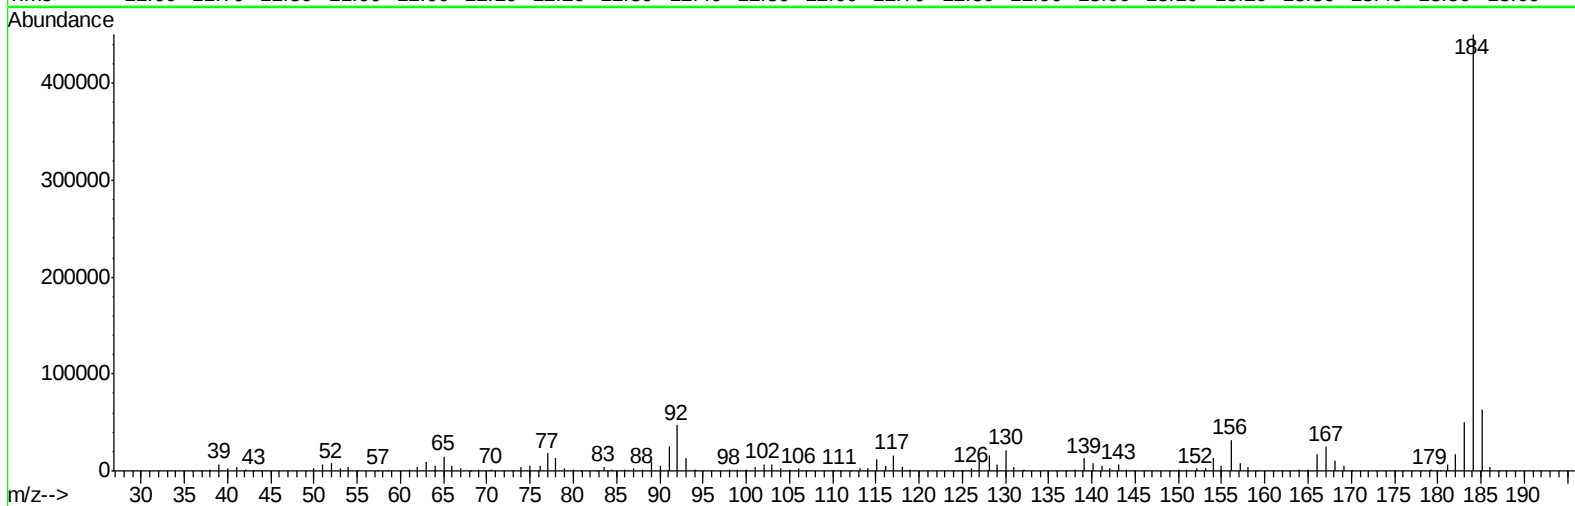


Data Path : Z:\HPCHEM1\BNA F\DATA\BF082417\
Data File : BF098000.D
Acq On : 24 Aug 2017 14:22
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 04:07:48 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

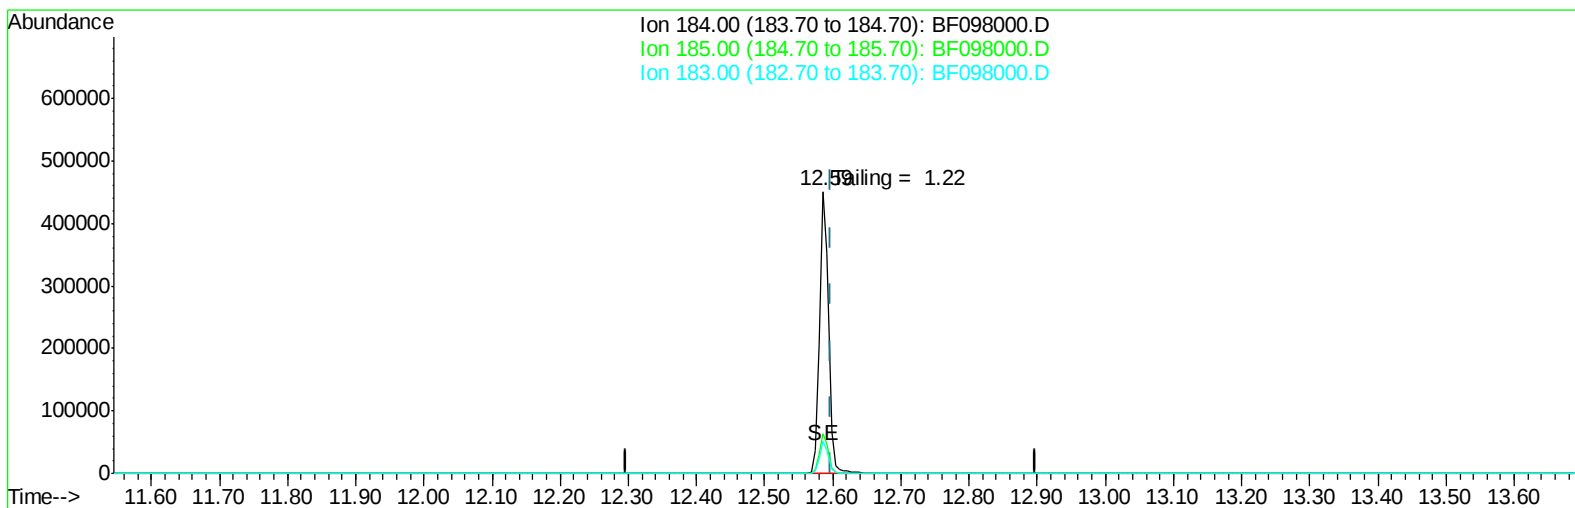

TIC: BF098000.D

(76) Benzidine




12.586min (-0.012) 8610.48ng

response 407103

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.17#
183.00	12.20	11.23
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082417\
Data File : BF098000.D
Acq On : 24 Aug 2017 14:22
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 04:07:48 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 21 15:59:04 2017
Response via : Initial Calibration

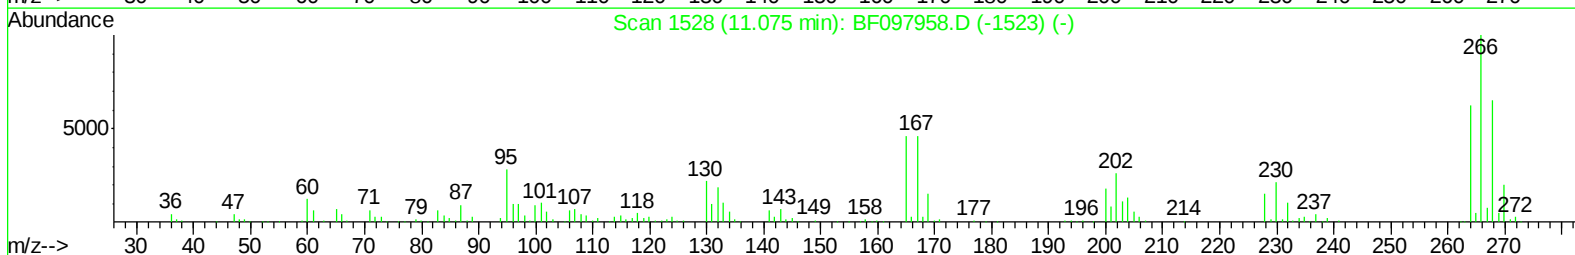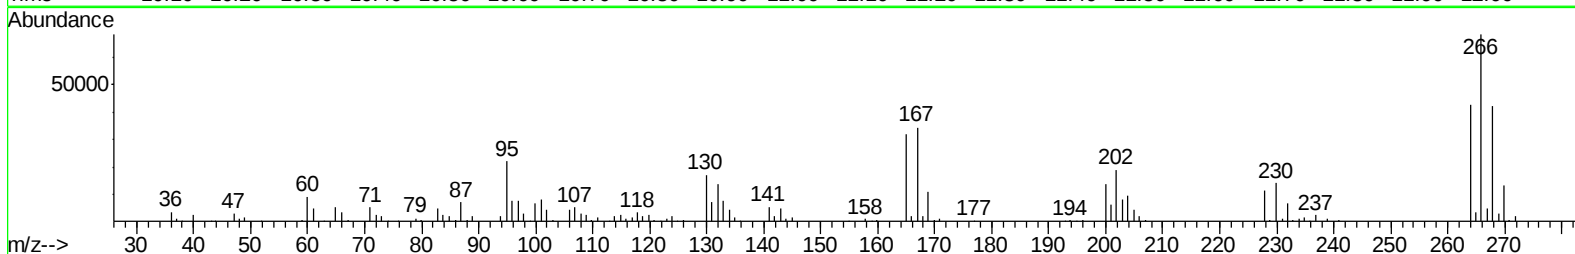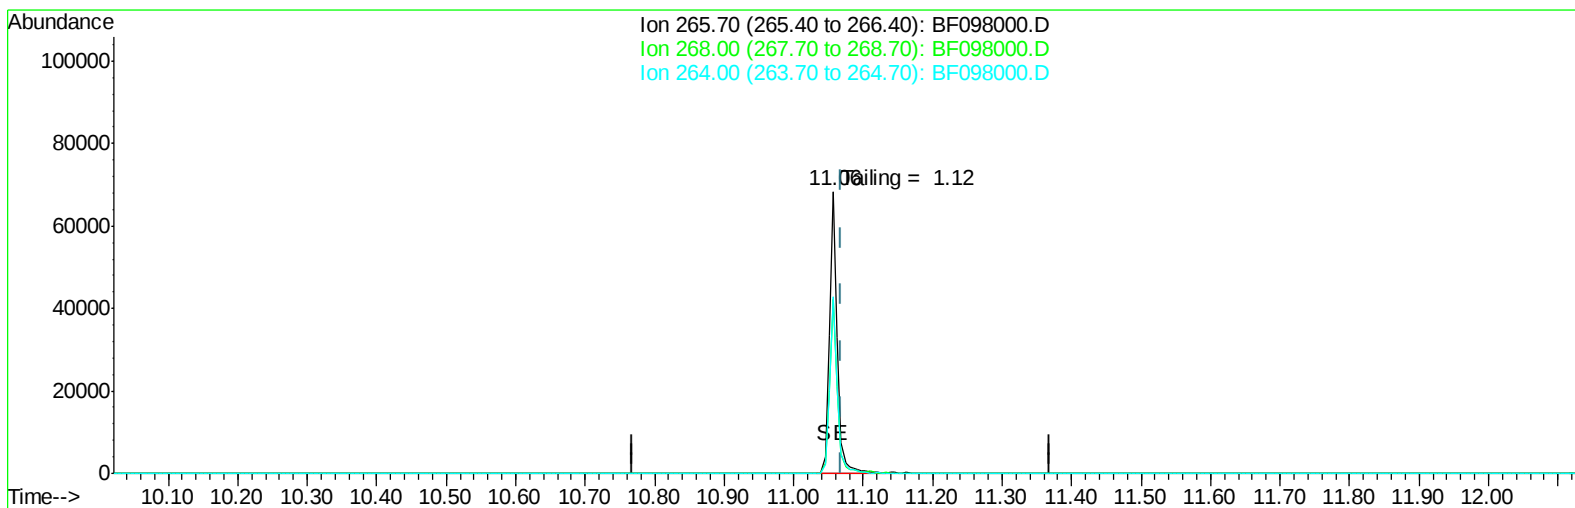

TIC: BF098000.D

(69) Pentachlorophenol (C)

11.057min (-0.012) 34056.40ng

response 54855

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.05
264.00	64.60	62.78
0.00	0.00	0.00