
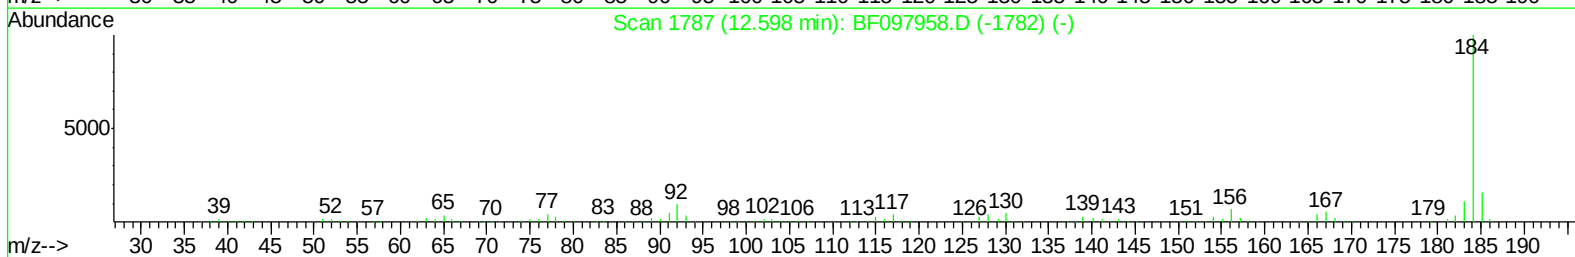
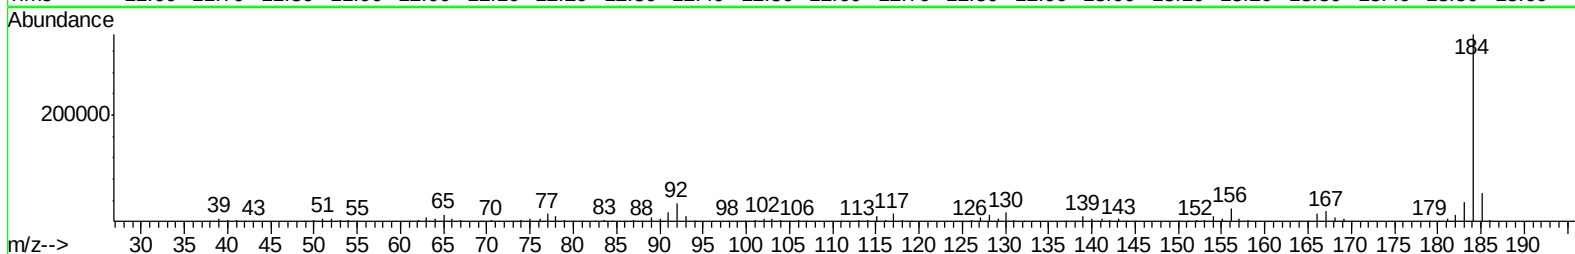


Data Path : Z:\HPCHEM1\BNA F\DATA\BF082417\  
 Data File : BF098026.D  
 Acq On : 25 Aug 2017 3:03  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 04:10:19 2017  
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Aug 21 15:59:04 2017  
 Response via : Initial Calibration

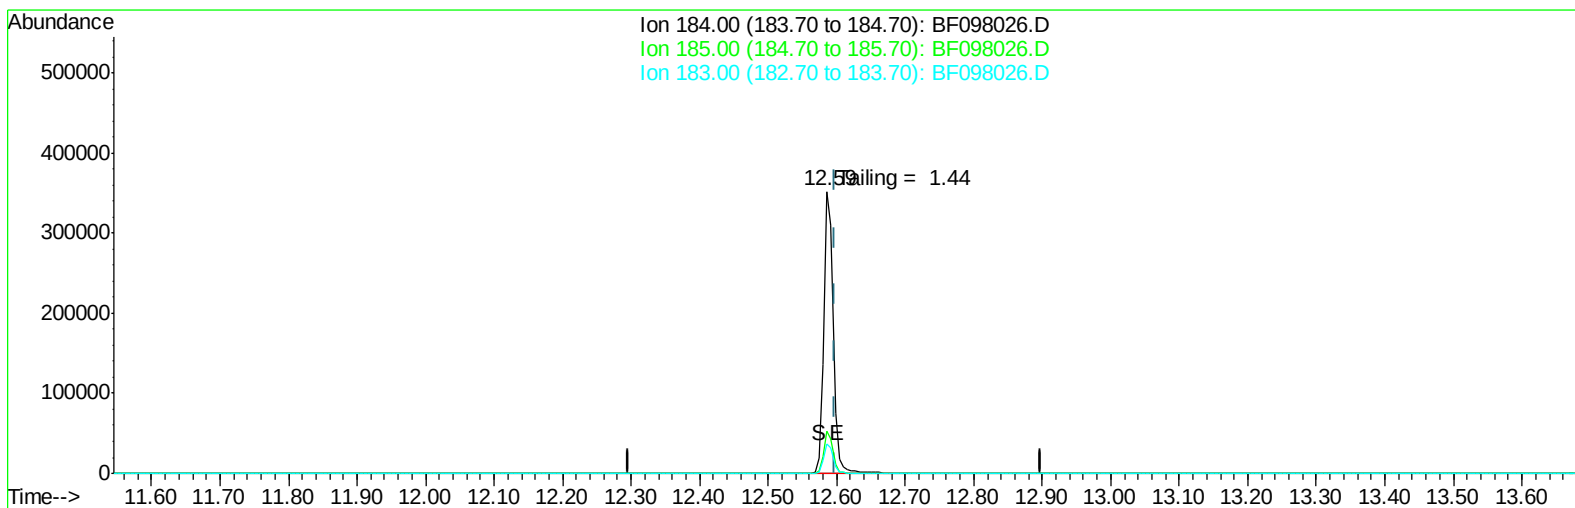

TIC: BF098026.D

(76) Benzidine




12.586min (-0.012) 8753.48ng

response 332928

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 19.40 | 15.19# |
| 183.00 | 12.20 | 10.51  |
| 0.00   | 0.00  | 0.00   |

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082417\  
Data File : BF098026.D  
Acq On : 25 Aug 2017 3:03  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 04:10:19 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 21 15:59:04 2017  
Response via : Initial Calibration

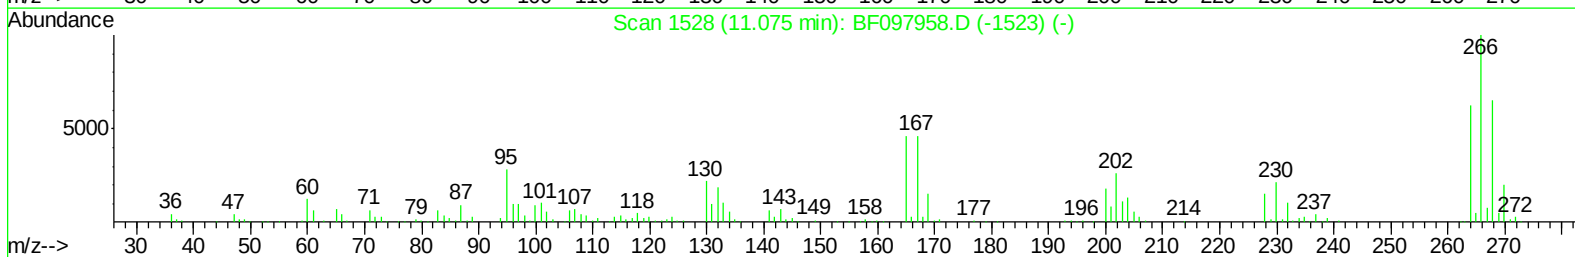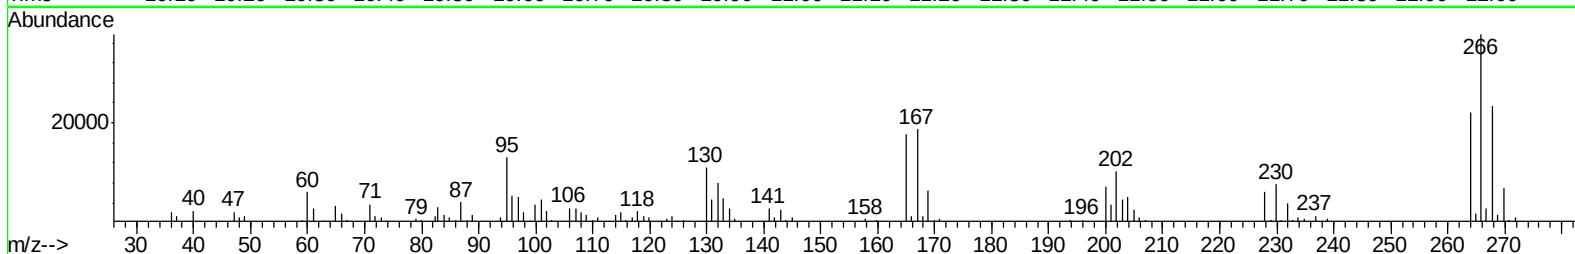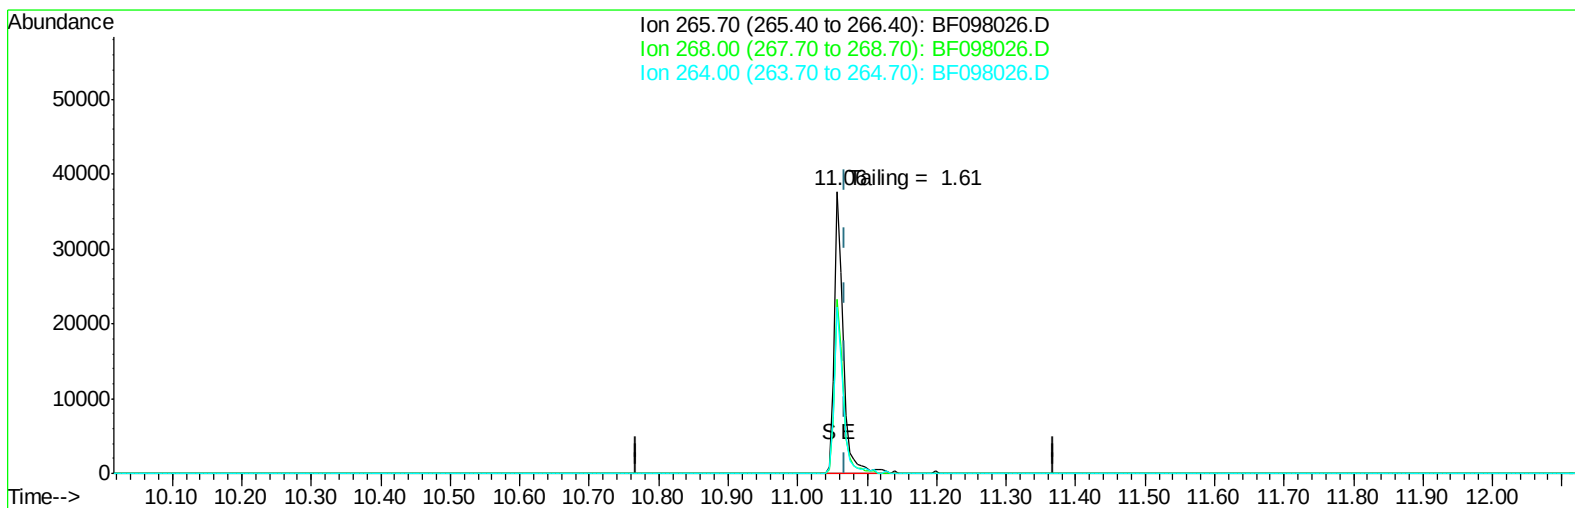

TIC: BF098026.D

(69) Pentachlorophenol (C)

11.057min (-0.012) 0.00ng

response 33205

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 62.04 |
| 264.00 | 64.60 | 58.89 |
| 0.00   | 0.00  | 0.00  |