


Data Path : Z:\HPCHEM1\BNA F\Data\BF082417\
 Data File : BF098026.D
 Acq On : 25 Aug 2017 3:03
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 21 15:59:04 2017

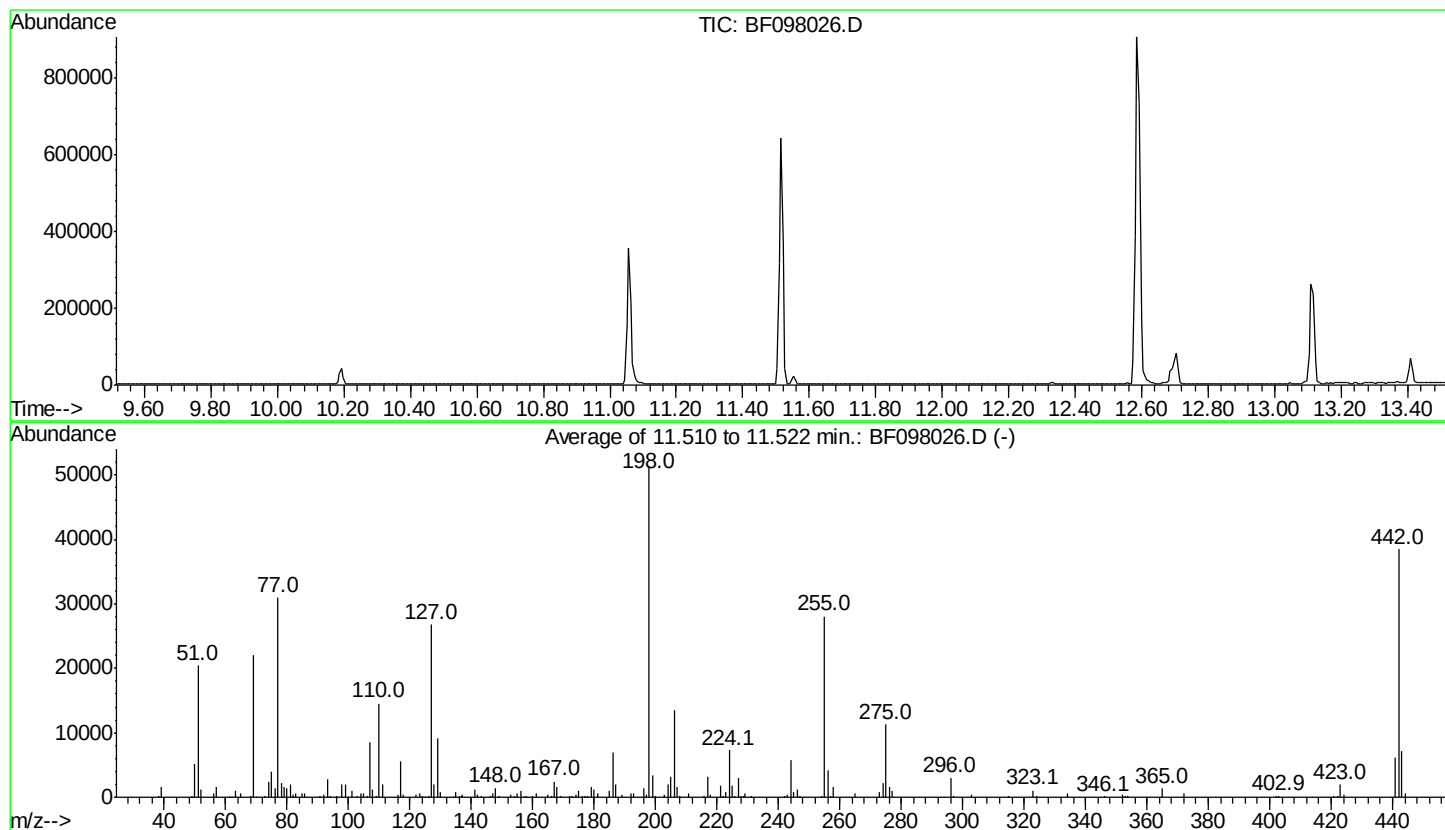

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	20415	PASS
68	69	0.00	2	0.9	191	PASS
69	198	0.00	100	42.8	22026	PASS
70	69	0.00	2	0.5	104	PASS
127	198	10	80	52.1	26773	PASS
197	198	0.00	2	0.9	485	PASS
198	198	100	100	100.0	51424	PASS
199	198	5	9	6.8	3474	PASS
275	198	10	60	21.9	11276	PASS
365	198	1	100	2.6	1347	PASS
441	442	0.01	24	16.2	6225	PASS
442	198	50	100	74.8	38441	PASS
443	442	15	24	18.7	7188	PASS