
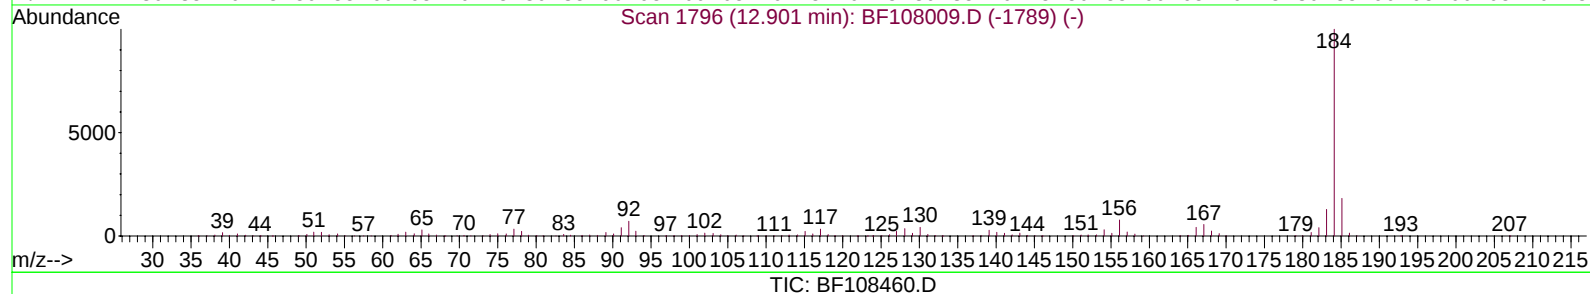
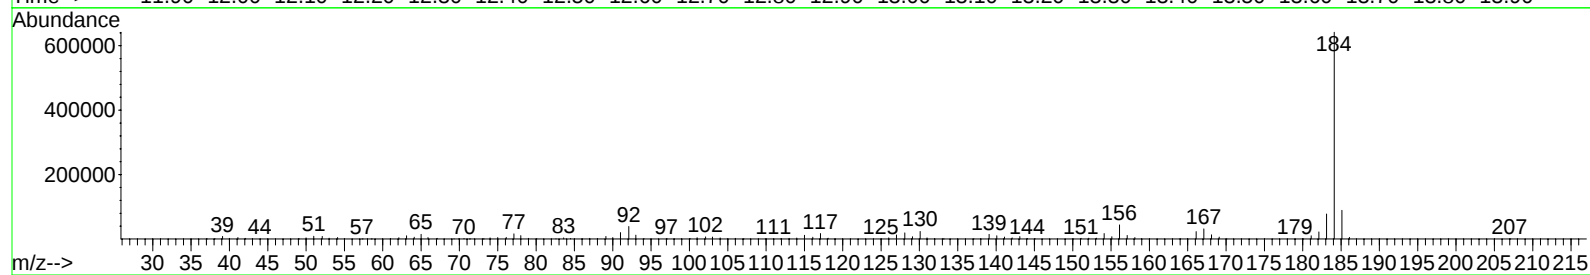


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF082418\
Data File : BF108460.D
Acq On : 24 Aug 2018 13:43
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 17:21:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 22 11:01:45 2018
Response via : Initial Calibration

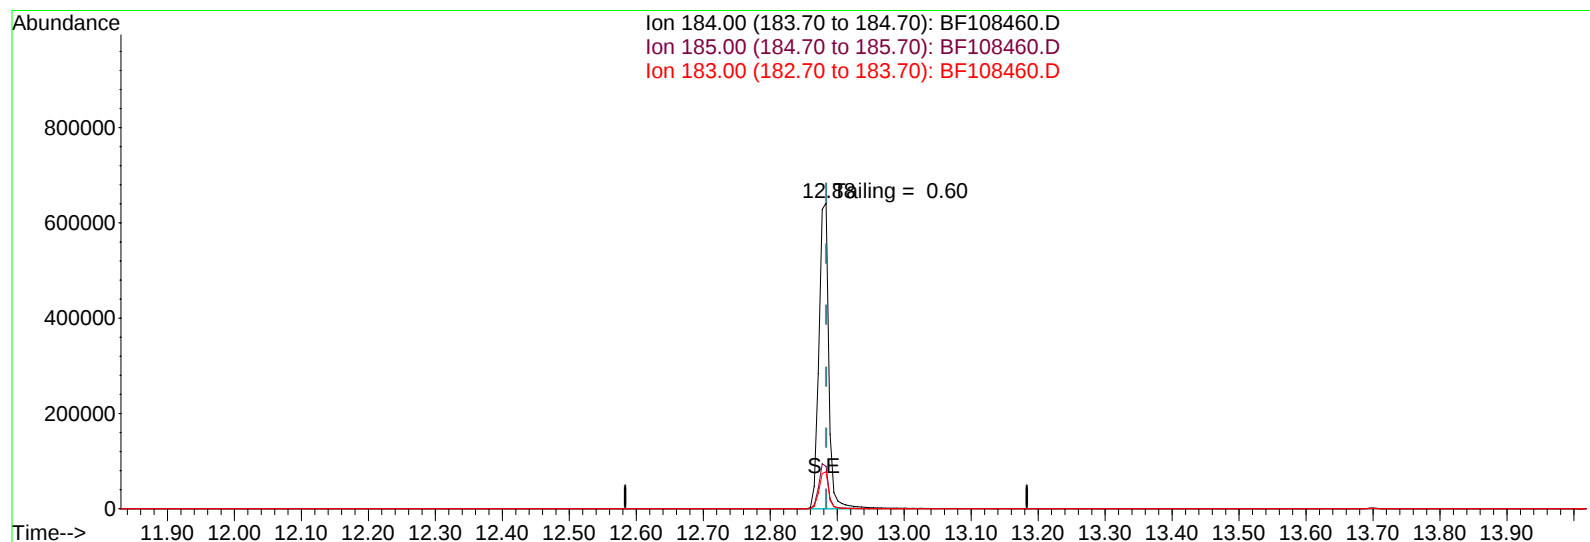

(76) Benzidine




12.883min (-0.000) 0.00ng

response 659596

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.86
183.00	11.60	12.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF082418\
Data File : BF108460.D
Acq On : 24 Aug 2018 13:43
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 17:21:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 22 11:01:45 2018
Response via : Initial Calibration

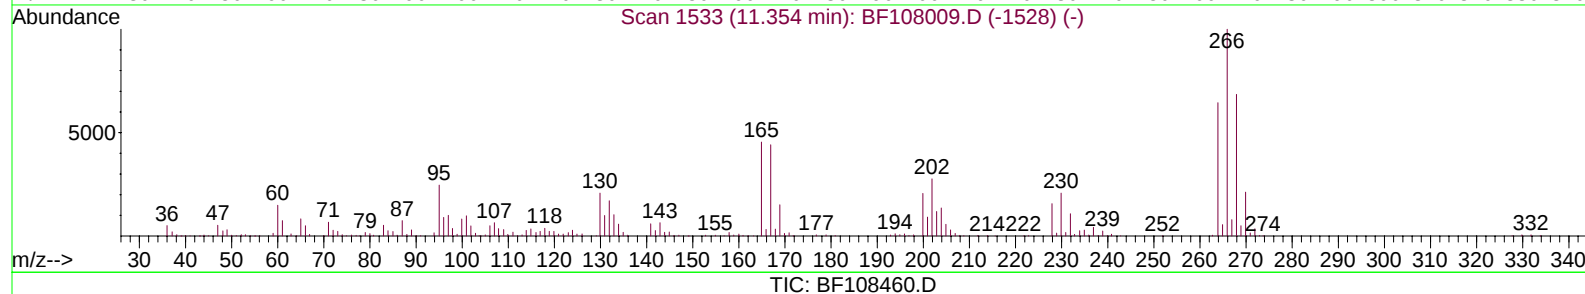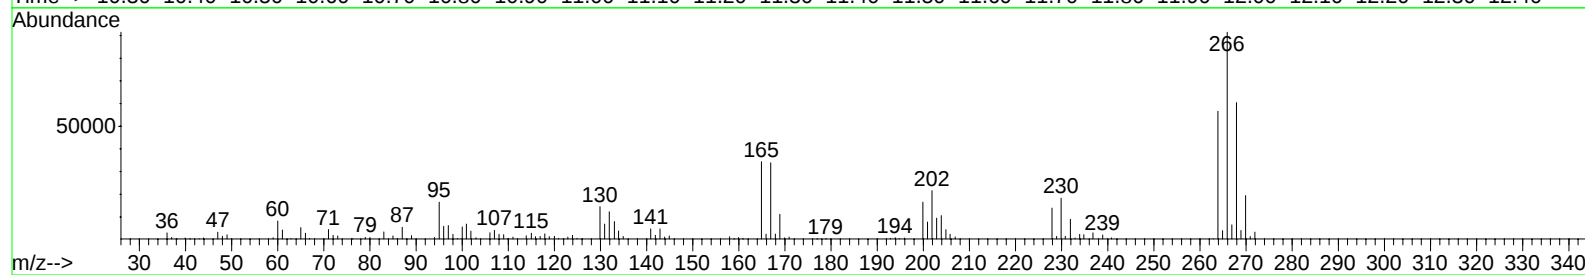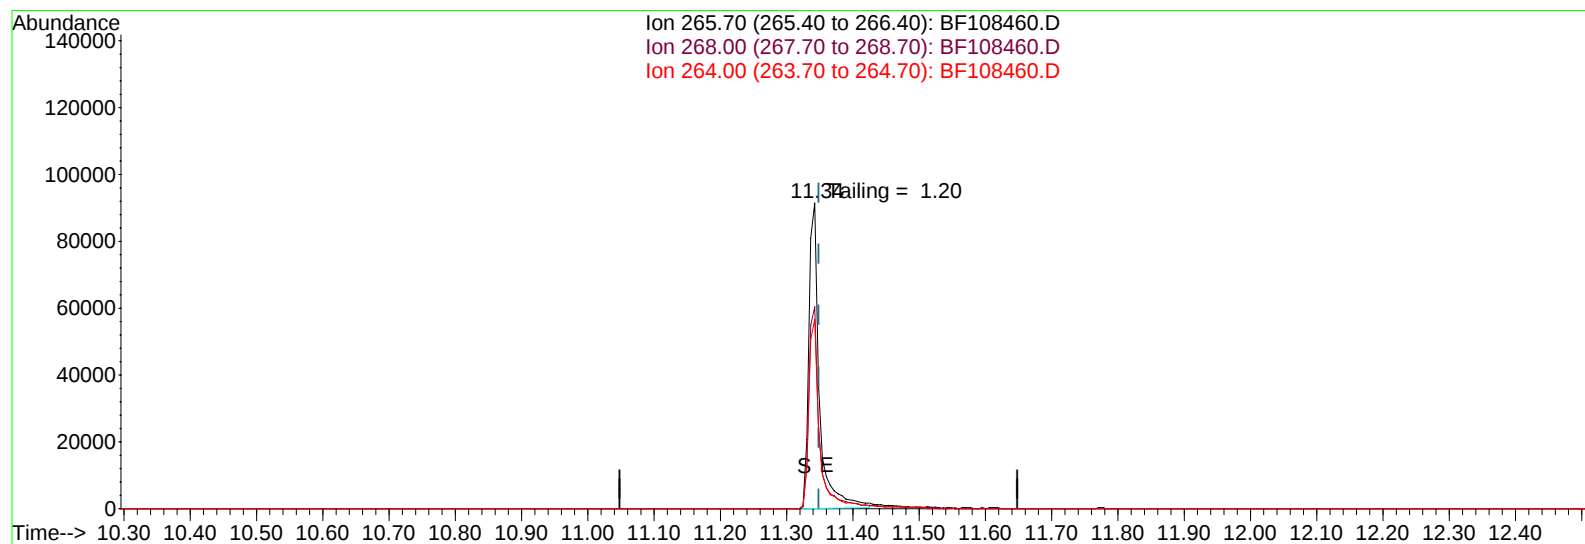

(69) Pentachlorophenol (C)

11.342min (-0.006) 52404.70ng

response 106978

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.05
264.00	61.90	61.91
0.00	0.00	0.00