

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082418\
 Data File : BF108483.D
 Acq On : 25 Aug 2018 00:18
 Operator : JU/SJ
 Sample : J4594-01 5X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 1-3-RO

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.225	489	491	497	rVB	19786	20552	1.86%	0.190%
2	5.619	554	558	570	rBV	611129	563166	50.97%	5.213%
3	6.613	723	727	741	rBV	674496	628606	56.89%	5.819%
4	6.766	749	753	766	rVB	745250	622695	56.36%	5.764%
5	6.995	789	792	796	rBV	869488	774168	70.07%	7.166%
6	7.154	815	819	827	rBV	558372	479448	43.39%	4.438%
7	7.554	884	887	898	rBV	397996	381198	34.50%	3.528%
8	8.283	1006	1011	1014	rBV	1151024	970156	87.81%	8.980%
9	9.354	1189	1193	1202	rBV	801994	709384	64.21%	6.566%
10	9.742	1256	1259	1267	rVB	45524	48011	4.35%	0.444%
11	10.042	1306	1310	1322	rVB2	1188449	1104864	100.00%	10.227%
12	10.595	1400	1404	1408	rVB2	16118	16414	1.49%	0.152%
13	10.672	1413	1417	1422	rVB4	9329	16655	1.51%	0.154%
14	10.836	1441	1445	1455	rBV	264528	292301	26.46%	2.706%
15	10.936	1458	1462	1468	rVB4	14642	19467	1.76%	0.180%
16	11.436	1545	1547	1550	rVB	15418	11965	1.08%	0.111%
17	11.536	1560	1564	1567	rBV	1044350	1019067	92.23%	9.433%
18	11.560	1567	1568	1572	rVV	261094	181839	16.46%	1.683%
19	11.613	1575	1577	1580	rVB	24734	21875	1.98%	0.202%
20	11.772	1599	1604	1608	rBV3	10245	17768	1.61%	0.164%
21	11.871	1618	1621	1625	rVB2	13022	11916	1.08%	0.110%
22	12.036	1647	1649	1652	rBV	37024	36259	3.28%	0.336%
23	12.066	1652	1654	1660	rVB2	43196	46691	4.23%	0.432%
24	12.154	1666	1669	1671	rBV2	35668	43967	3.98%	0.407%
25	12.177	1671	1673	1676	rVB	21048	19055	1.72%	0.176%
26	12.336	1696	1700	1702	rBV	21370	24673	2.23%	0.228%
27	12.366	1702	1705	1708	rVB3	20715	22971	2.08%	0.213%
28	12.483	1723	1725	1729	rBV4	9360	11581	1.05%	0.107%
29	12.589	1740	1743	1747	rBV2	18307	21288	1.93%	0.197%
30	12.683	1756	1759	1762	rBV4	9705	12864	1.16%	0.119%
31	12.754	1768	1771	1776	rBV	150035	144916	13.12%	1.341%
32	12.989	1805	1811	1816	rBV	165933	192714	17.44%	1.784%
33	13.118	1830	1833	1837	rBV	604986	498027	45.08%	4.610%
34	13.201	1845	1847	1854	rVB6	12692	20134	1.82%	0.186%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082418\
Data File : BF108483.D
Acq On : 25 Aug 2018 00:18
Operator : JU/SJ
Sample : J4594-01 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
1-3-RO

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.313	1864	1866	1873	rVB2	22834	34127	3.09%	0.316%
36	13.418	1882	1884	1887	rBV2	17996	16994	1.54%	0.157%
37	13.513	1898	1900	1902	rBV2	14842	12788	1.16%	0.118%
38	13.548	1903	1906	1909	rBV3	17049	25038	2.27%	0.232%
39	14.142	2004	2007	2009	rBV	46598	37452	3.39%	0.347%
40	14.189	2011	2015	2018	rBV	912445	833200	75.41%	7.712%
41	15.742	2274	2279	2292	rVB	568846	837276	75.78%	7.750%


Sum of corrected areas: 10803530

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082418\
Data File : BF108483.D
Acq On : 25 Aug 2018 00:18
Operator : JU/SJ
Sample : J4594-01 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
1-3-RO

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

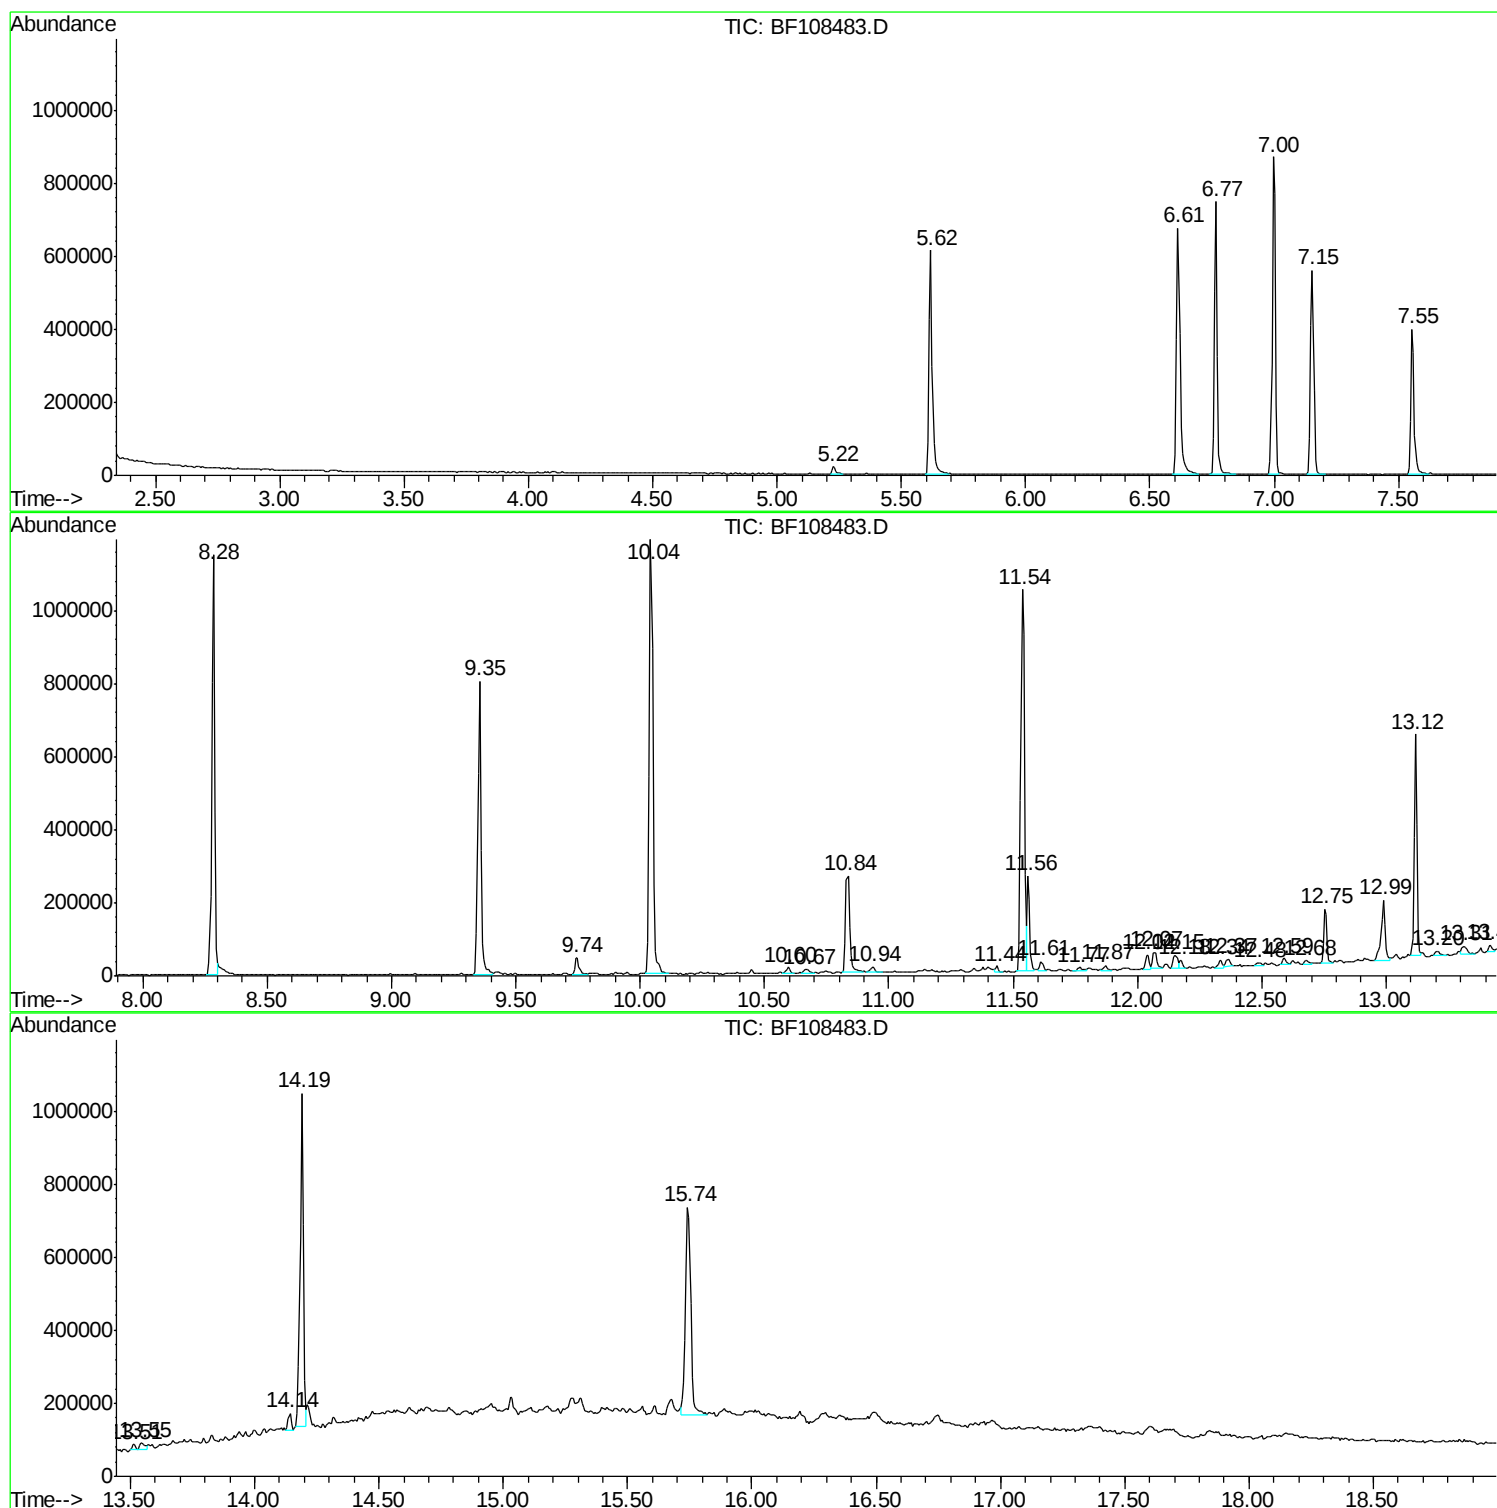

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082418\
Data File : BF108483.D
Acq On : 25 Aug 2018 00:18
Operator : JU/SJ
Sample : J4594-01 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
1-3-RO









Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.77 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.77	16.09 ng	622695	1,4-Dichlorobenzene-d4	7.00

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27	
2	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16	
3	Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	10	
4	Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9	
5	2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9	

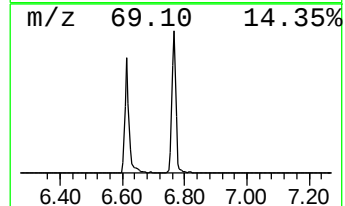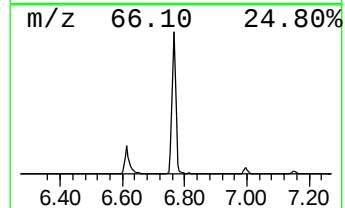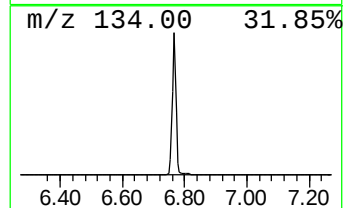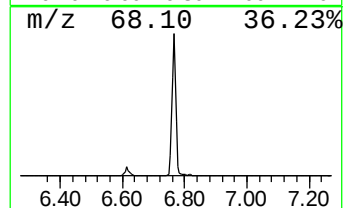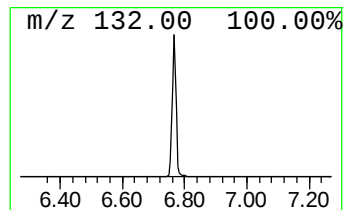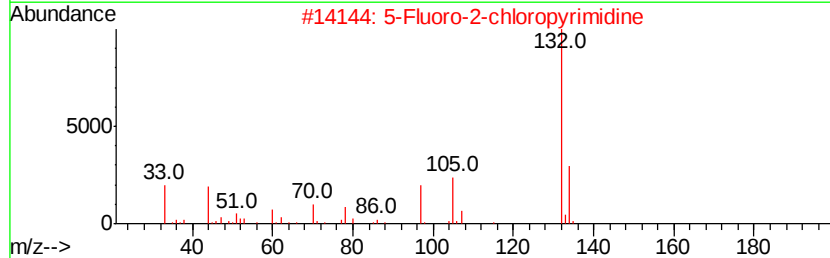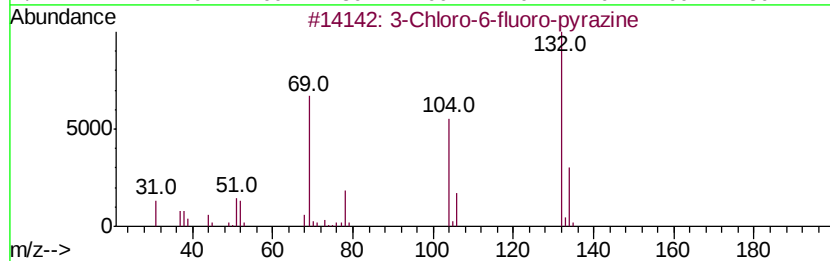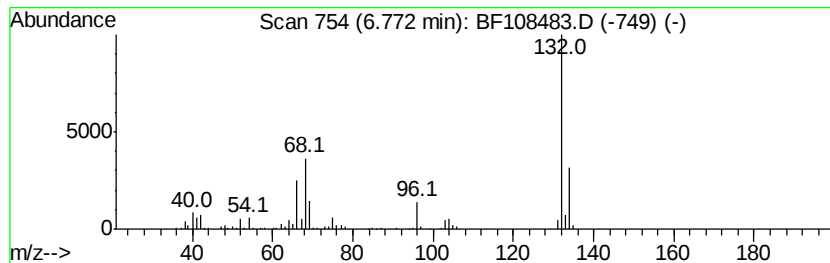

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082418\
Data File : BF108483.D
Acq On : 25 Aug 2018 00:18
Operator : JU/SJ
Sample : J4594-01 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
1-3-RO

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.77	6.77	16.1	ng	622695	1	7.00	774168	20.0