

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082418\
 Data File : BF108489.D
 Acq On : 25 Aug 2018 4:02
 Operator : JU/SJ
 Sample : J4636-01 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BYR-2-E(0-1)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.619	555	558	568	rBV	194204	191098	16.65%	2.518%
2	6.613	724	727	741	rBV	203810	218159	19.01%	2.875%
3	6.766	750	753	764	rVB	263117	220376	19.20%	2.904%
4	6.995	789	792	801	rBV	906161	841395	73.30%	11.087%
5	7.154	815	819	826	rBV	198161	178574	15.56%	2.353%
6	7.554	884	887	898	rBV	122628	133918	11.67%	1.765%
7	8.283	1006	1011	1014	rBV	1249620	1050198	91.49%	13.839%
8	9.354	1189	1193	1203	rBV	250137	232390	20.25%	3.062%
9	9.748	1257	1260	1268	rBV	49613	48840	4.25%	0.644%
10	10.042	1306	1310	1324	rBV2	1184775	1147867	100.00%	15.126%
11	10.836	1442	1445	1456	rBV	77251	83337	7.26%	1.098%
12	11.324	1520	1528	1534	rBV	18333	23245	2.03%	0.306%
13	11.536	1560	1564	1572	rBV	1095785	998366	86.98%	13.156%
14	12.760	1766	1772	1775	rBV	33591	32558	2.84%	0.429%
15	12.989	1809	1811	1815	rVB	34112	28914	2.52%	0.381%
16	13.118	1830	1833	1842	rVB	169989	149930	13.06%	1.976%
17	14.189	2011	2015	2019	rBV	966937	889681	77.51%	11.724%
18	14.948	2142	2144	2148	rVB3	16302	12576	1.10%	0.166%
19	15.277	2196	2200	2203	rBV2	25239	40107	3.49%	0.529%
20	15.306	2203	2205	2212	rVB4	31857	39500	3.44%	0.521%
21	15.606	2253	2256	2261	rVB	15686	18347	1.60%	0.242%
22	15.671	2264	2267	2271	rVV	19436	27294	2.38%	0.360%
23	15.742	2273	2279	2293	rVB	610701	922647	80.38%	12.158%
24	16.189	2352	2355	2361	rVB5	23664	35691	3.11%	0.470%
25	16.748	2445	2450	2455	rVB7	13395	23730	2.07%	0.313%


Sum of corrected areas: 7588738

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082418\
Data File : BF108489.D
Acq On : 25 Aug 2018 4:02
Operator : JU/SJ
Sample : J4636-01 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BYR-2-E(0-1)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

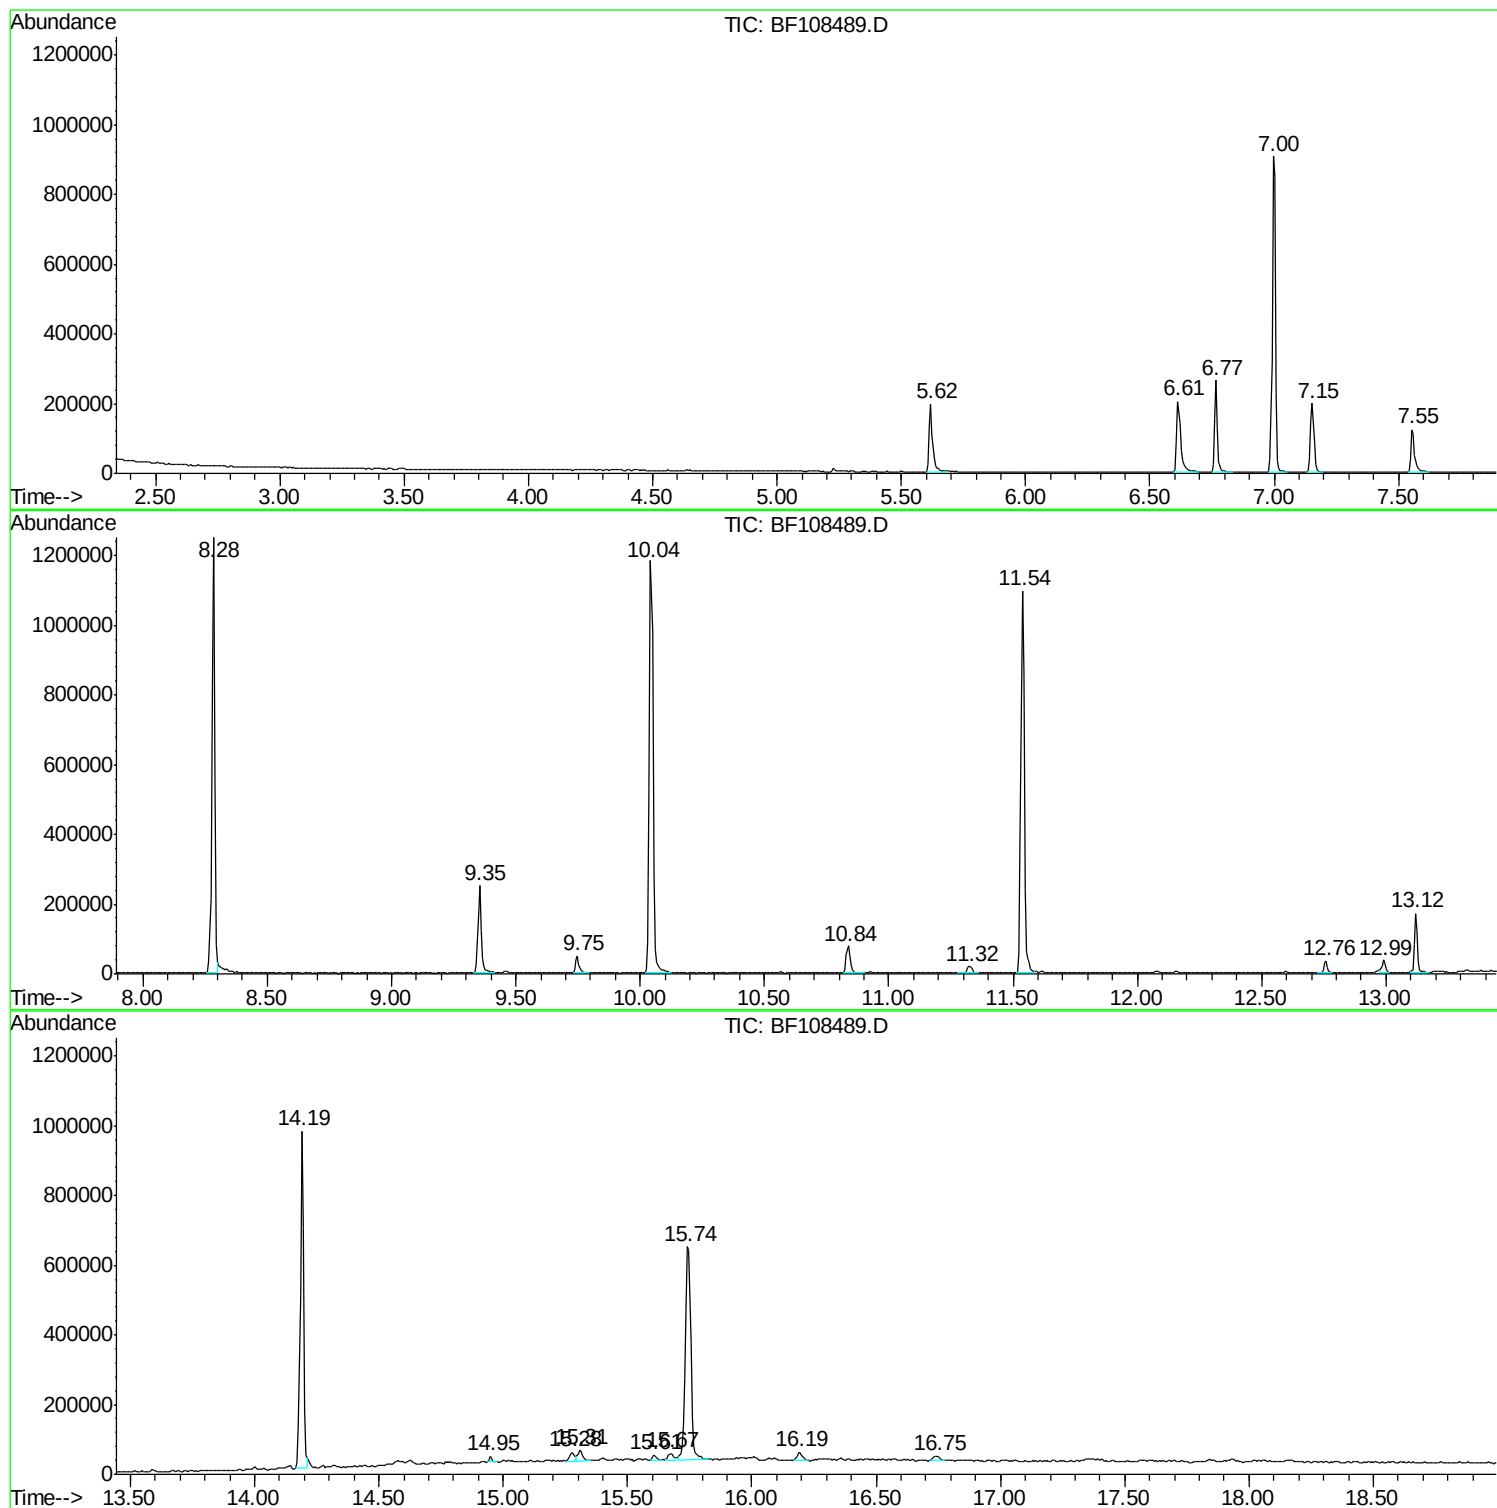

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082418\
Data File : BF108489.D
Acq On : 25 Aug 2018 4:02
Operator : JU/SJ
Sample : J4636-01 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BYR-2-E(0-1)










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.77 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.77	5.24 ng	220376	1,4-Dichlorobenzene-d4	7.00

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3			1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	9
4			Xenon	132	Xe	007440-63-3	9
5			2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

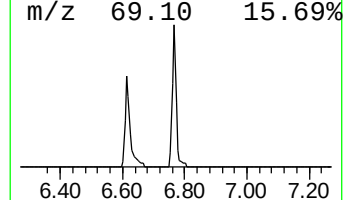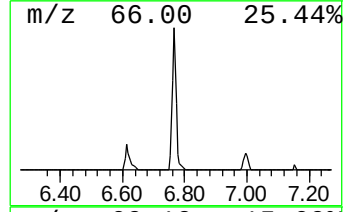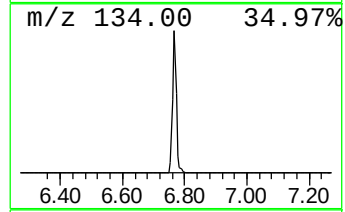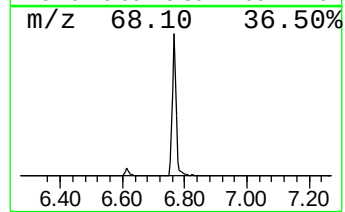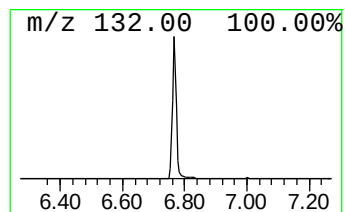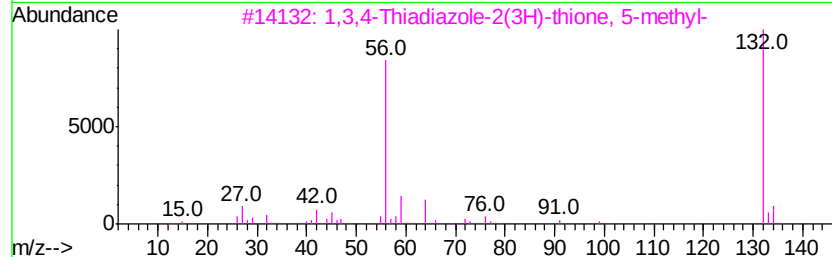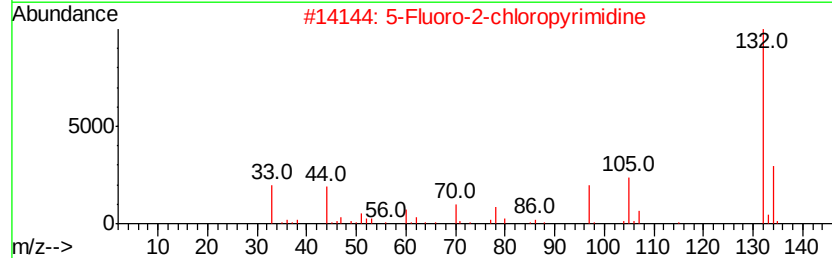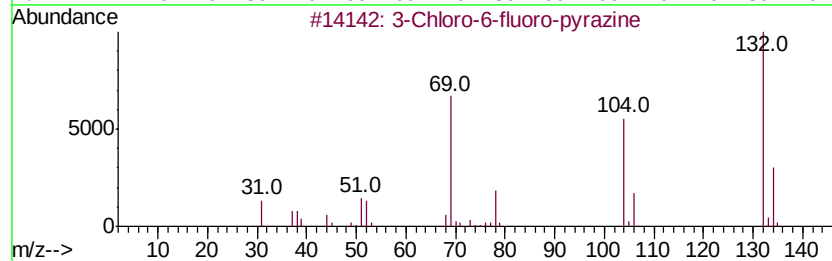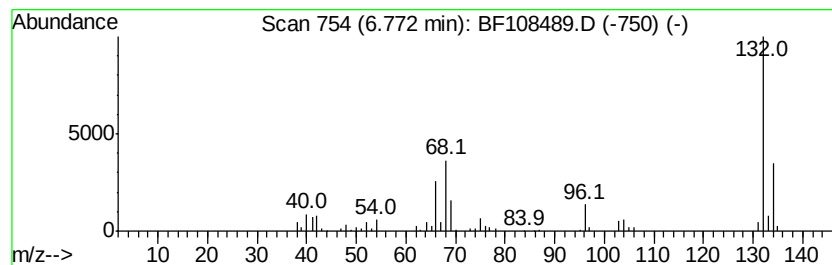

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082418\
Data File : BF108489.D
Acq On : 25 Aug 2018 4:02
Operator : JU/SJ
Sample : J4636-01 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BYR-2-E(0-1)

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.77	6.77	5.2	ng	220376	1	7.00	841395	20.0