


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082418\
 Data File : BF108460.D
 Acq On : 24 Aug 2018 13:43
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 22 11:01:45 2018

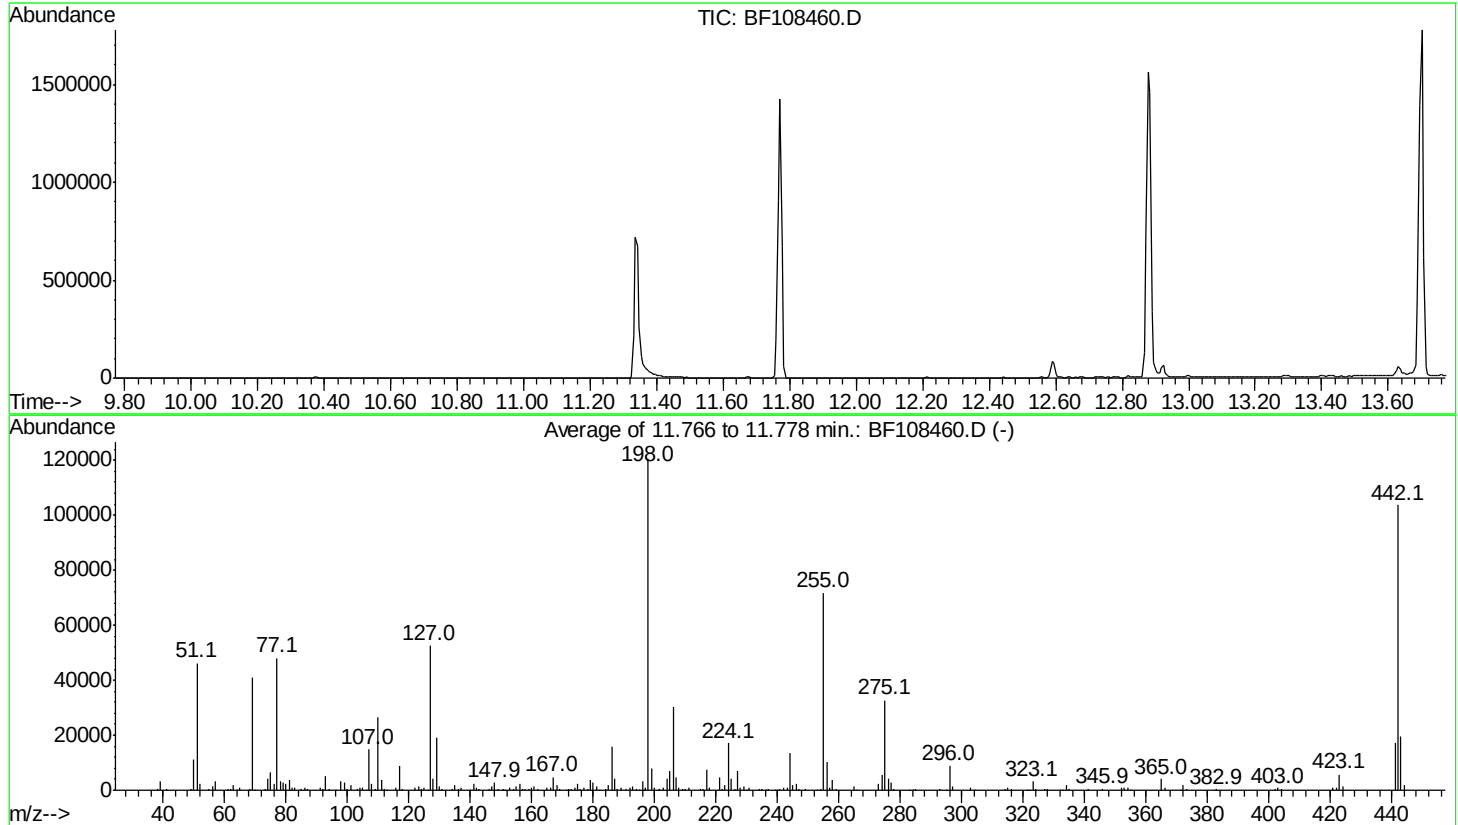

AutoFind: Scans 1603, 1604, 1605; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	46325	PASS
68	69	0.00	2	1.7	688	PASS
69	198	0.00	100	34.0	40952	PASS
70	69	0.00	2	0.6	232	PASS
127	198	10	80	43.5	52466	PASS
197	198	0.00	2	0.6	776	PASS
198	198	100	100	100.0	120602	PASS
199	198	5	9	6.4	7720	PASS
275	198	10	60	27.2	32837	PASS
365	198	1	100	3.4	4120	PASS
441	198	0.01	100	14.2	17081	PASS
442	198	50	100	86.1	103786	PASS
443	442	15	24	18.9	19641	PASS