


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082418\
 Data File : BF108487.D
 Acq On : 25 Aug 2018 3:00
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 22 11:01:45 2018

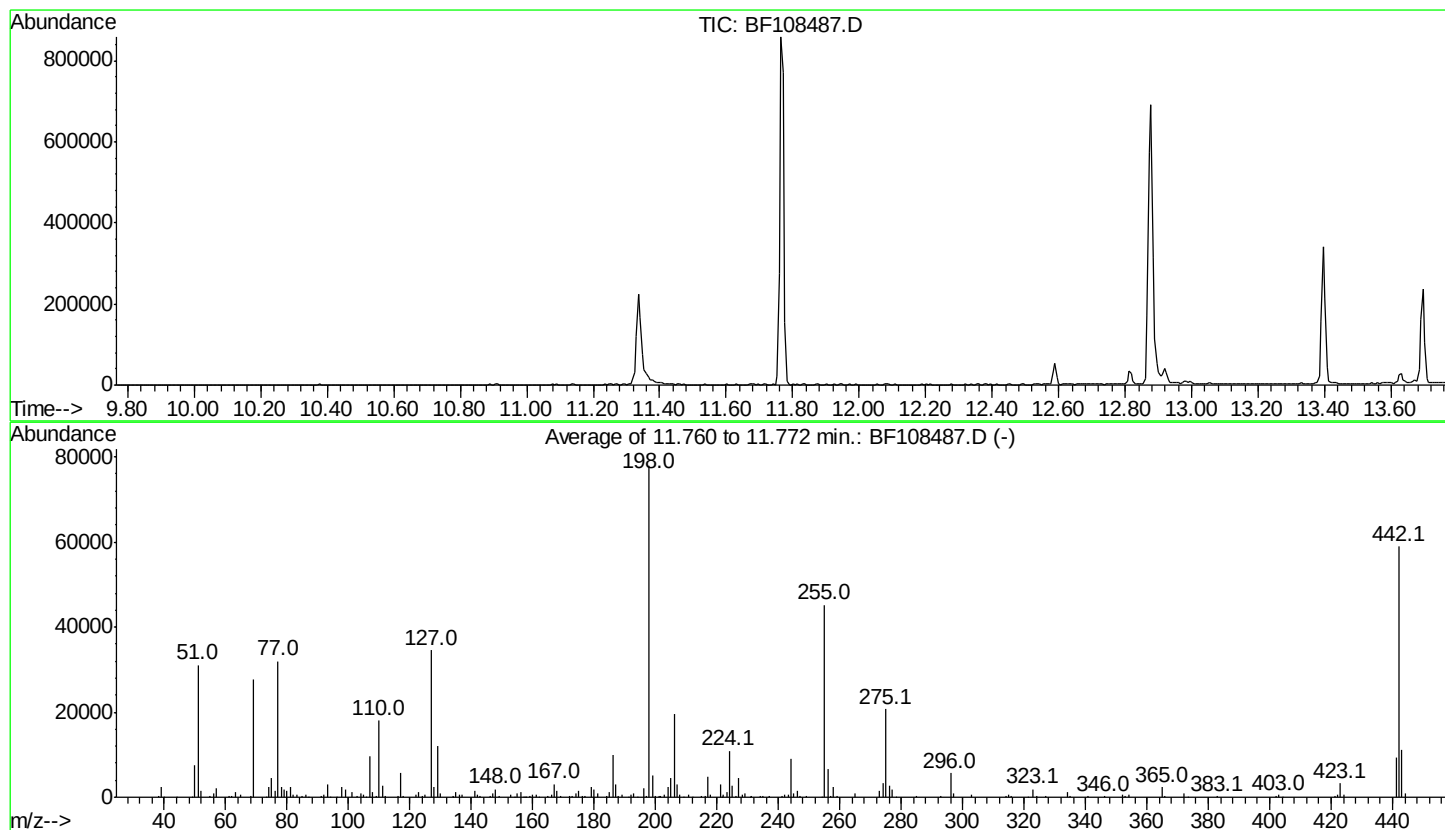

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	31136	PASS
68	69	0.00	2	1.4	398	PASS
69	198	0.00	100	35.4	27616	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.2	34474	PASS
197	198	0.00	2	0.2	190	PASS
198	198	100	100	100.0	77957	PASS
199	198	5	9	6.7	5227	PASS
275	198	10	60	26.5	20676	PASS
365	198	1	100	3.1	2392	PASS
441	198	0.01	100	12.1	9454	PASS
442	198	50	100	75.6	58911	PASS
443	442	15	24	19.1	11239	PASS