
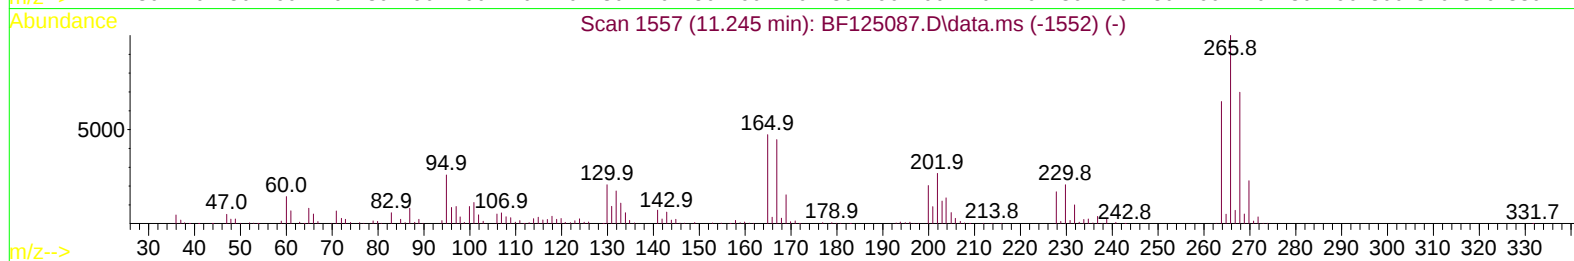
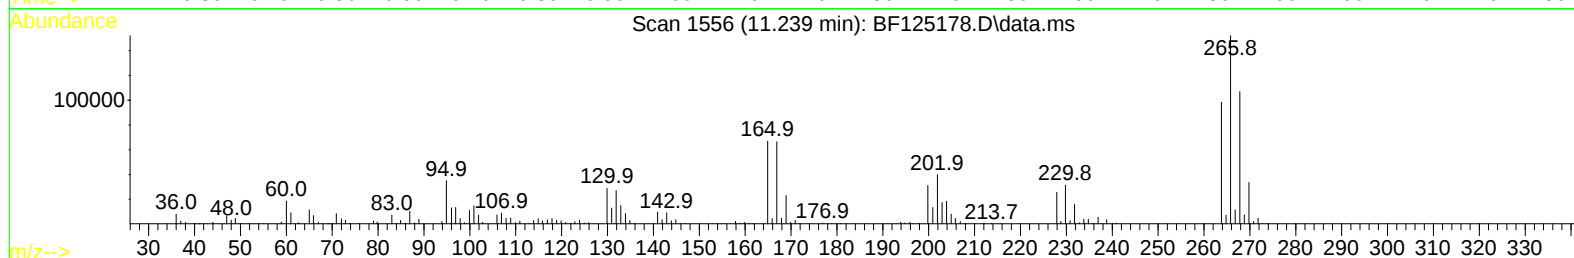


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082421\
Data File : BF125178.D
Acq On : 24 Aug 2021 11:10
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 12:35:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 10:15:49 2021
Response via : Initial Calibration

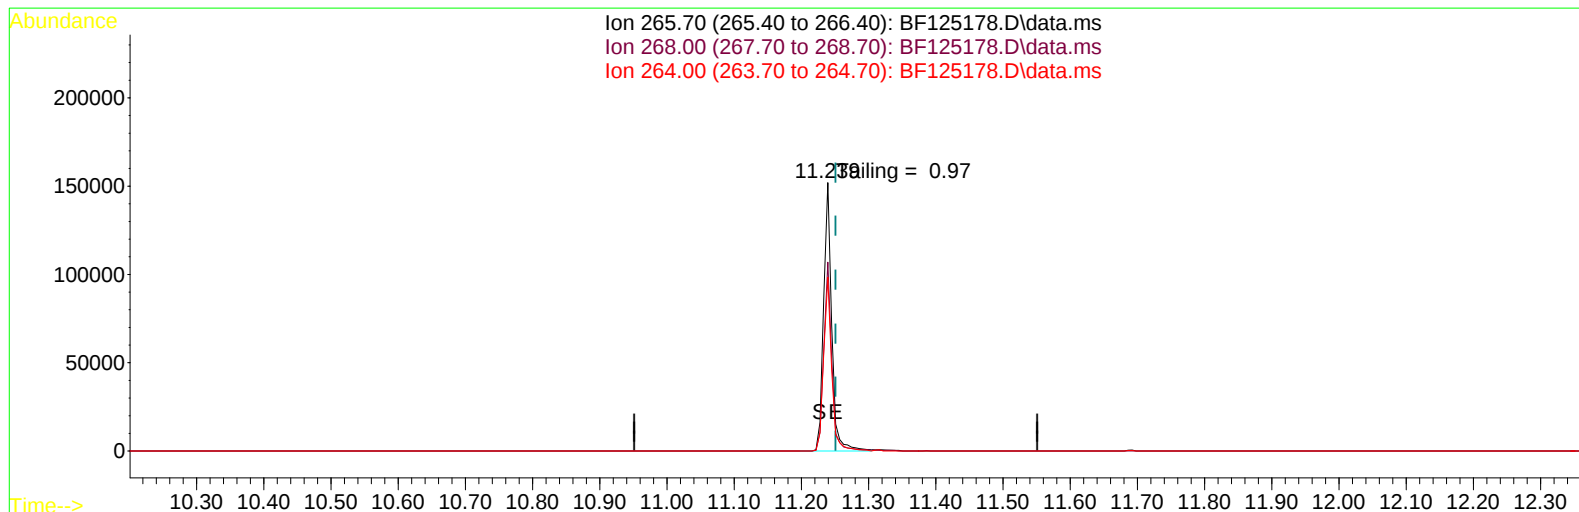

TIC: BF125178.D\data.ms

(70) Pentachlorophenol (C)




11.239min (-0.012) 31055.80 ng

response 130148

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	70.38
264.00	69.90	64.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082421\
Data File : BF125178.D
Acq On : 24 Aug 2021 11:10
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 24 12:35:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 10:15:49 2021
Response via : Initial Calibration

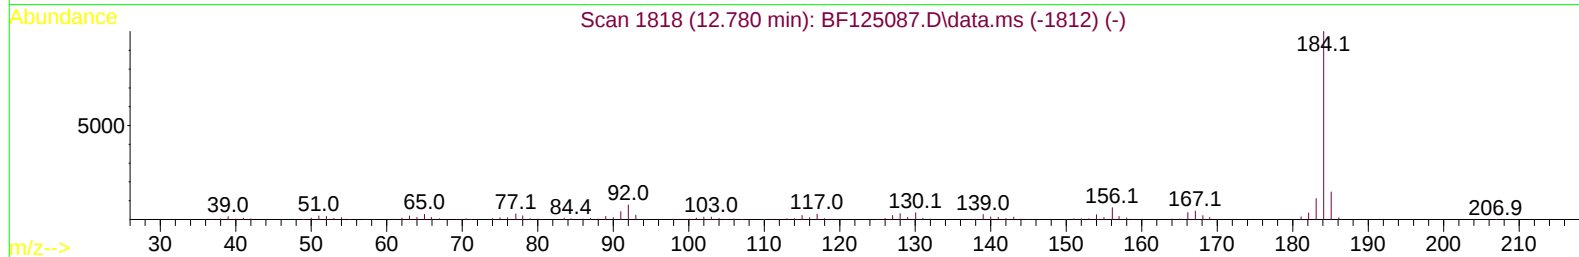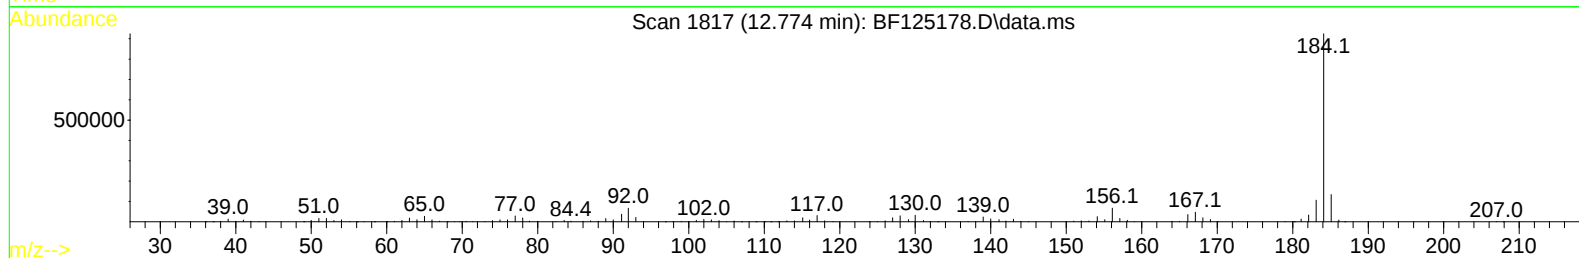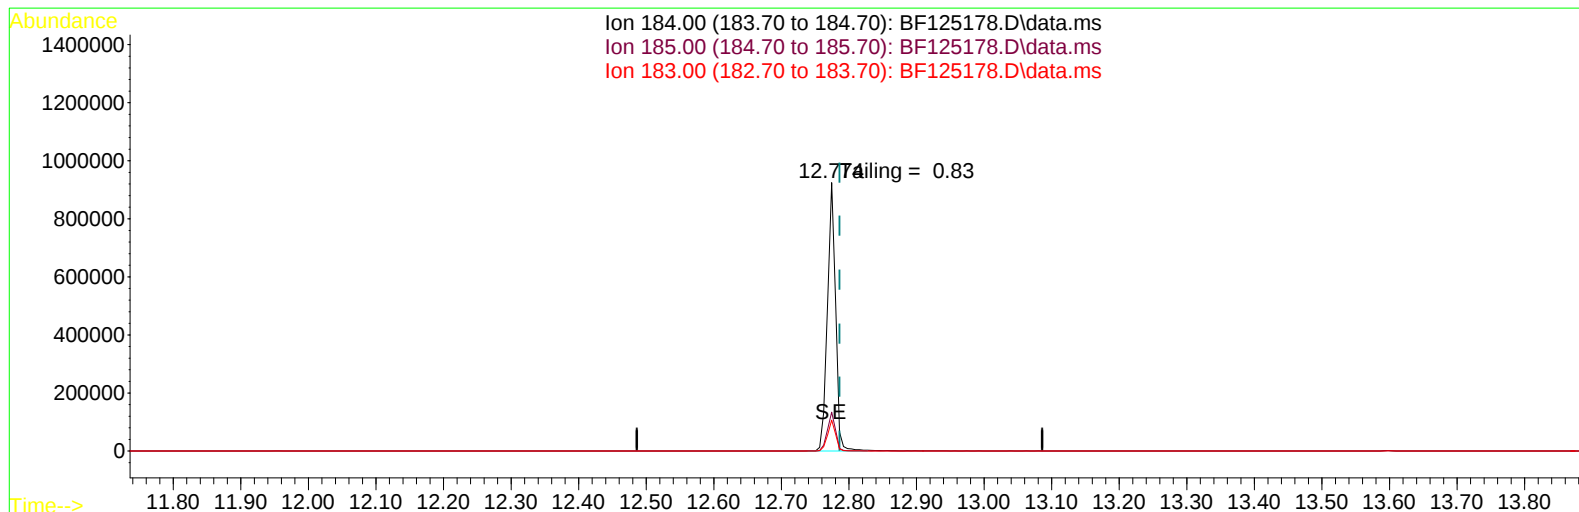

TIC: BF125178.D\data.ms

(77) Benzidine

12.774min (-0.012) 0.00 ng

response 783248

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.50
183.00	10.10	11.51
0.00	0.00	0.00