

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082421\
 Data File : BF125194.D
 Acq On : 24 Aug 2021 20:04
 Operator : JU/CG
 Sample : M3430-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PE-5

Quant Time: Aug 25 04:37:16 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 12:39:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.916	152	139840	20.000	ng	0.00
21) Naphthalene-d8	8.198	136	530316	20.000	ng	# 0.00
39) Acenaphthene-d10	9.951	164	284557	20.000	ng	0.00
64) Phenanthrene-d10	11.439	188	502592	20.000	ng	0.00
76) Chrysene-d12	14.074	240	345788	20.000	ng	# 0.00
86) Perylene-d12	15.574	264	370512	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.528	112	845674	91.534	ng	0.00
7) Phenol-d6	6.534	99	1058222	88.563	ng	0.00
23) Nitrobenzene-d5	7.475	82	701820	66.625	ng	0.00
42) 2,4,6-Tribromophenol	10.739	330	326421	114.916	ng	0.00
45) 2-Fluorobiphenyl	9.269	172	1299390	63.643	ng	0.00
79) Terphenyl-d14	13.021	244	1313448	60.512	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082421\
Data File : BF125194.D
Acq On : 24 Aug 2021 20:04
Operator : JU/CG
Sample : M3430-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PE-5

Quant Time: Aug 25 04:37:16 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 12:39:21 2021
Response via : Initial Calibration



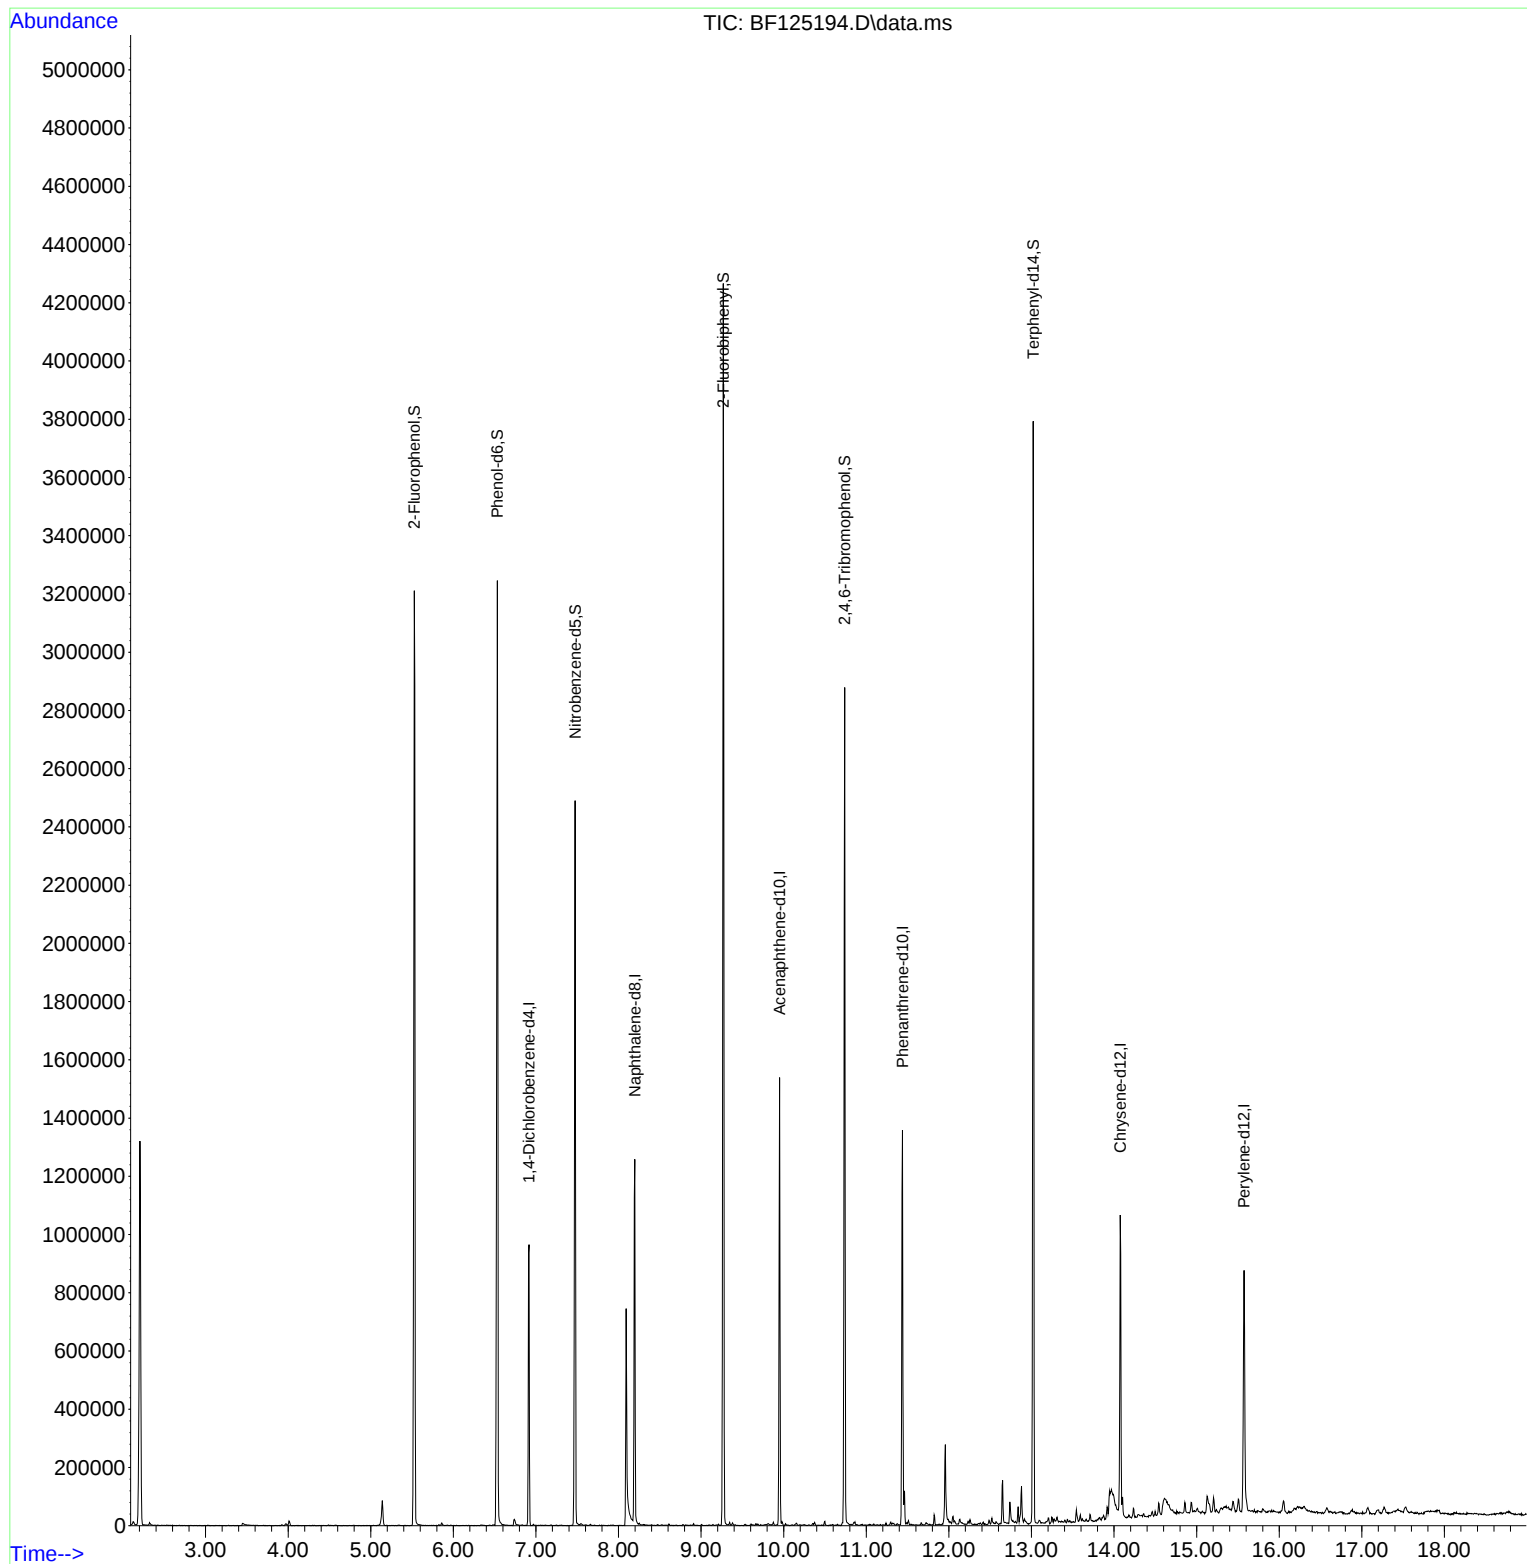


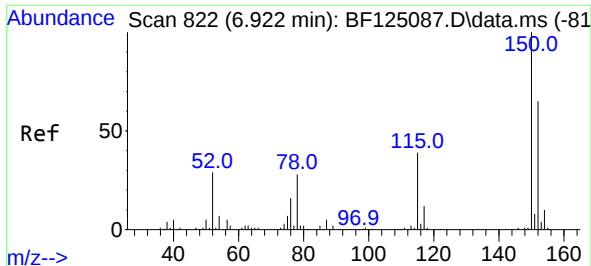

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.916 min Scan# 821
Delta R.T. -0.000 min
Lab File: BF125194.D
Acq: 24 Aug 2021 20:04




Instrument :
BNA_F
ClientSampled :
PE-5

Tgt Ion:152 Resp: 139840
Ion Ratio Lower Upper
152 100
150 156.0 117.6 176.4
115 58.3 47.1 70.7

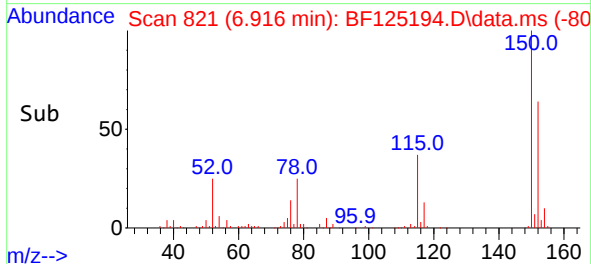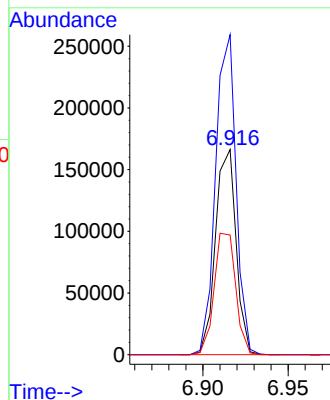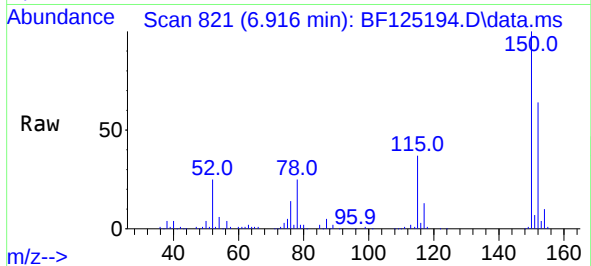

#5
2-Fluorophenol
Concen: 91.534 ng
RT: 5.528 min Scan# 585
Delta R.T. 0.000 min
Lab File: BF125194.D
Acq: 24 Aug 2021 20:04

Tgt Ion:112 Resp: 845674
Ion Ratio Lower Upper
112 100
64 74.3 44.2 66.2#
63 40.0 26.2 39.2#

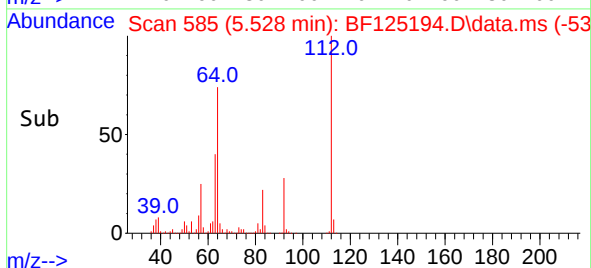
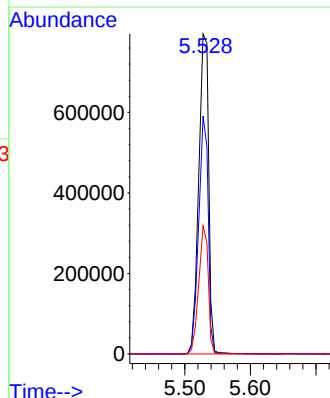
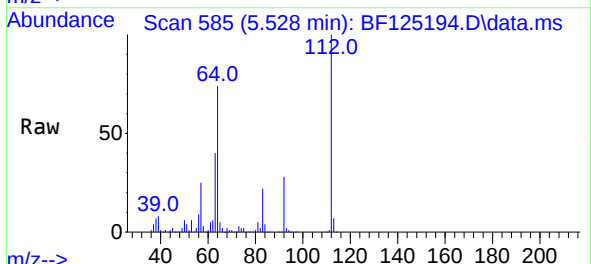




#7
Phenol-d6
Concen: 88.563 ng
RT: 6.534 min Scan# 756
Delta R.T. -0.006 min
Lab File: BF125194.D
Acq: 24 Aug 2021 20:04




Instrument :
BNA_F
ClientSampleId :
PE-5


Tgt Ion: 99 Resp: 1058222
Ion Ratio Lower Upper
99 100
42 23.9 23.5 35.3
71 39.7 25.6 38.4#

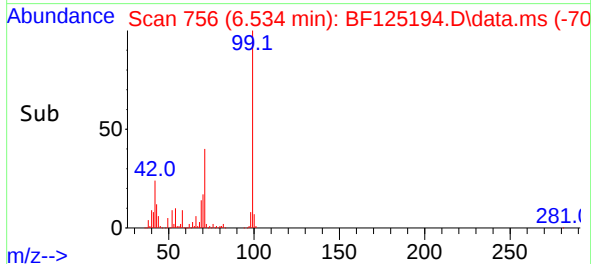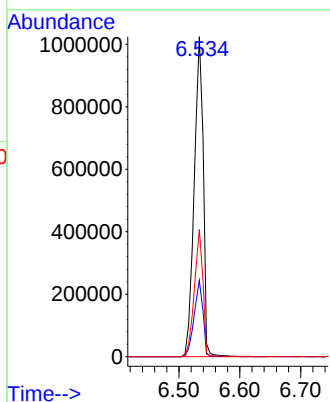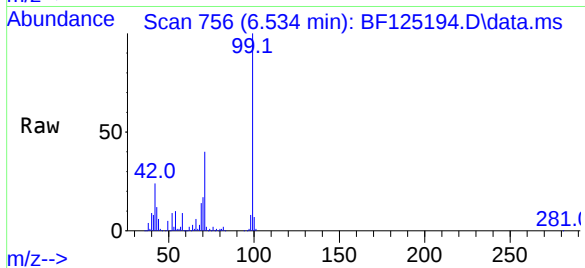

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.198 min Scan# 1039
Delta R.T. 0.000 min
Lab File: BF125194.D
Acq: 24 Aug 2021 20:04

Tgt Ion: 136 Resp: 530316
Ion Ratio Lower Upper
136 100
137 10.3 9.8 14.6
54 9.5 6.4 9.6
68 5.6 3.3 4.9#


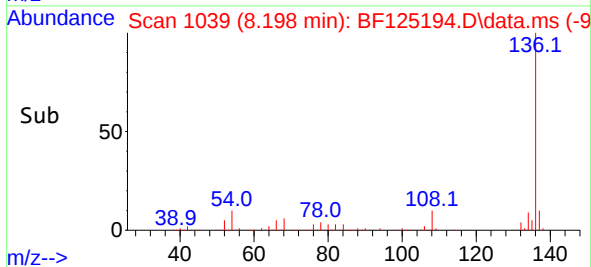
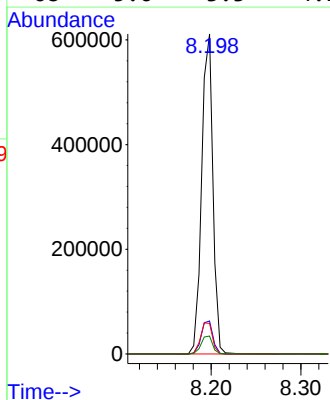
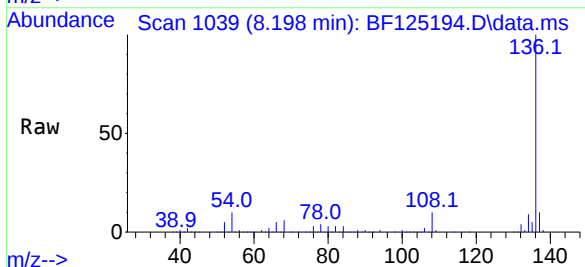


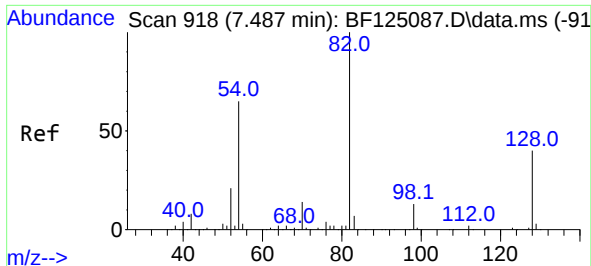

#23
Nitrobenzene-d5
Concen: 66.625 ng
RT: 7.475 min Scan# 916
Delta R.T. -0.006 min
Lab File: BF125194.D
Acq: 24 Aug 2021 20:04




Instrument :
BNA_F
ClientSampled :
PE-5

Tgt Ion: 82 Resp: 701820
Ion Ratio Lower Upper
82 100
128 39.3 40.6 60.8#
54 65.4 49.6 74.4

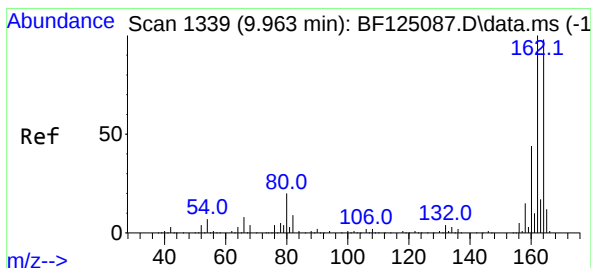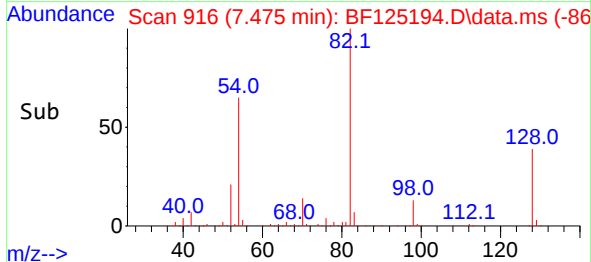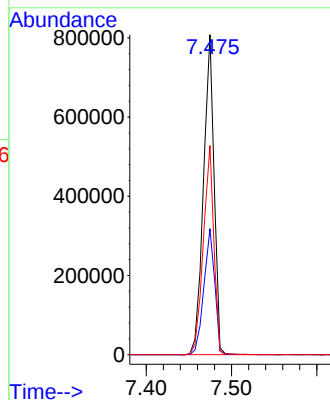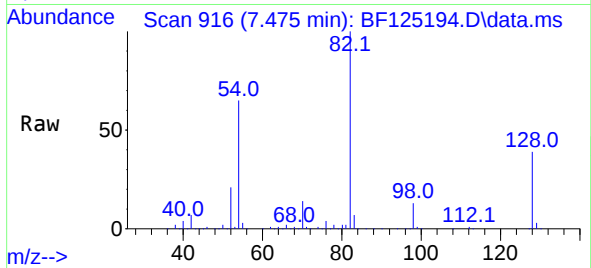

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.951 min Scan# 1337
Delta R.T. 0.000 min
Lab File: BF125194.D
Acq: 24 Aug 2021 20:04

Tgt Ion:164 Resp: 284557
Ion Ratio Lower Upper
164 100
162 104.3 81.3 121.9
160 45.9 38.0 57.0


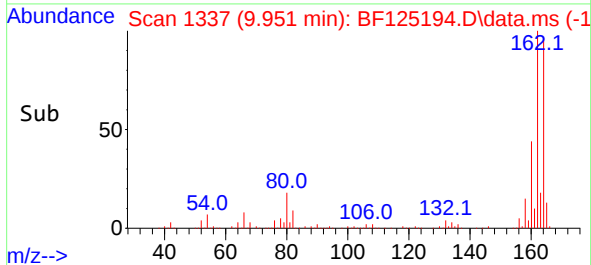
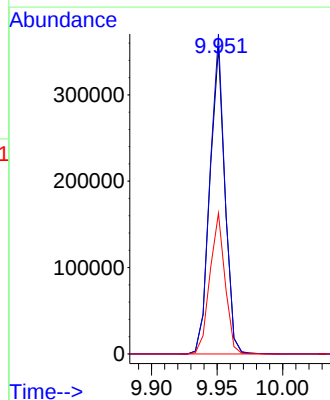
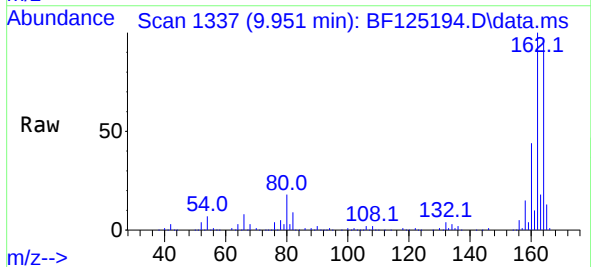




#42
2,4,6-Tribromophenol
Concen: 114.916 ng
RT: 10.739 min Scan# 1471
Delta R.T. 0.000 min
Lab File: BF125194.D
Acq: 24 Aug 2021 20:04




Instrument :
BNA_F
ClientSampleID :
PE-5


Tgt Ion: 330 Resp: 326421
Ion Ratio Lower Upper
330 100
332 95.9 76.2 114.4
141 31.3 44.6 66.8#

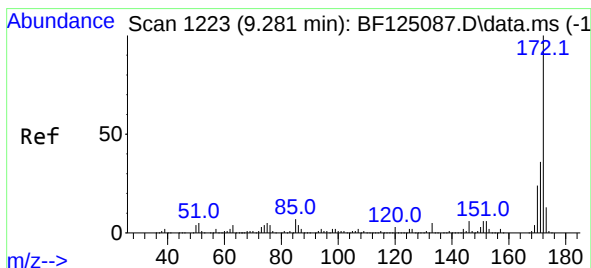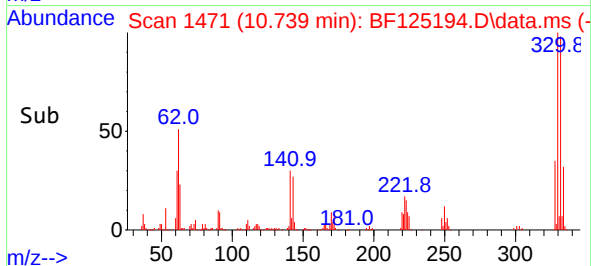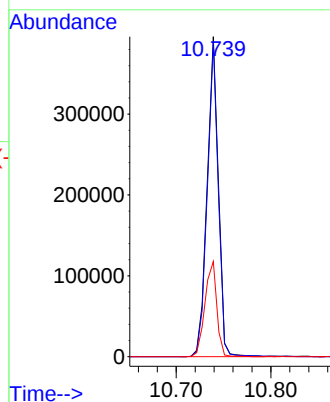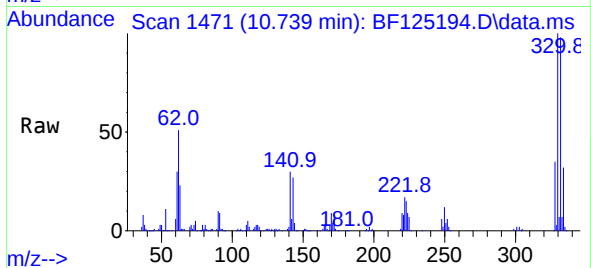

#45
2-Fluorobiphenyl
Concen: 63.643 ng
RT: 9.269 min Scan# 1221
Delta R.T. -0.006 min
Lab File: BF125194.D
Acq: 24 Aug 2021 20:04

Tgt Ion: 172 Resp: 1299390
Ion Ratio Lower Upper
172 100
171 35.4 26.5 39.7
170 24.0 18.8 28.2


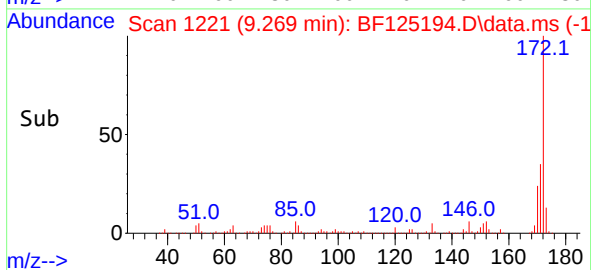
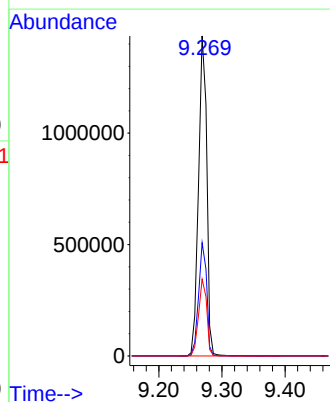
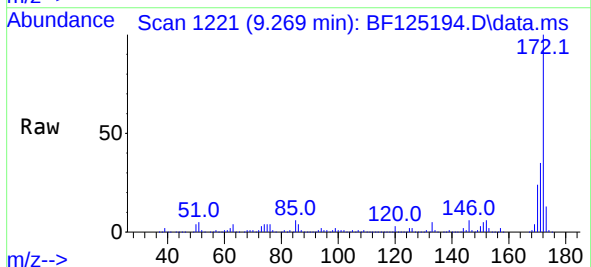


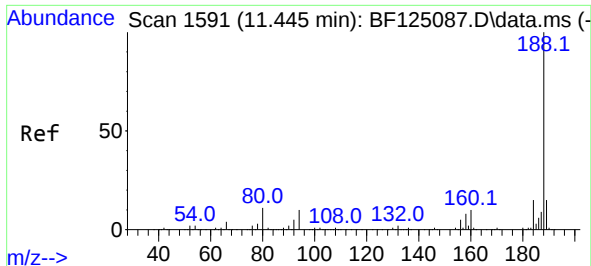

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.439 min Scan# 1590
Delta R.T. 0.000 min
Lab File: BF125194.D
Acq: 24 Aug 2021 20:04




Instrument :
BNA_F
ClientSampled :
PE-5


Tgt Ion:188 Resp: 502592
Ion Ratio Lower Upper
188 100
94 7.8 6.7 10.1
80 8.8 7.5 11.3

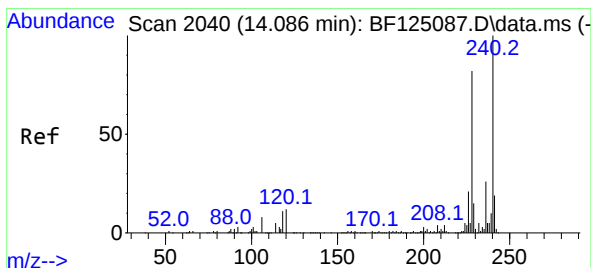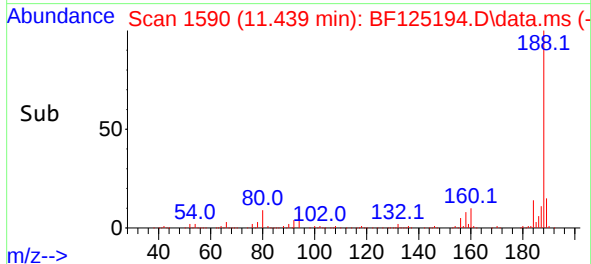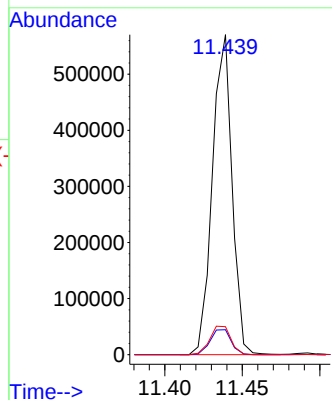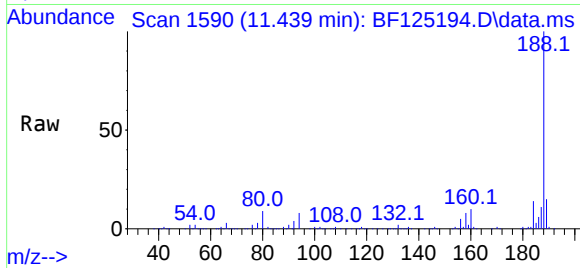

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.074 min Scan# 2038
Delta R.T. -0.006 min
Lab File: BF125194.D
Acq: 24 Aug 2021 20:04


Tgt Ion:240 Resp: 345788
Ion Ratio Lower Upper
240 100
120 9.9 10.8 16.2#
236 25.5 21.6 32.4

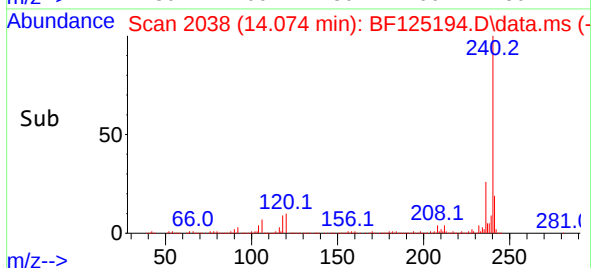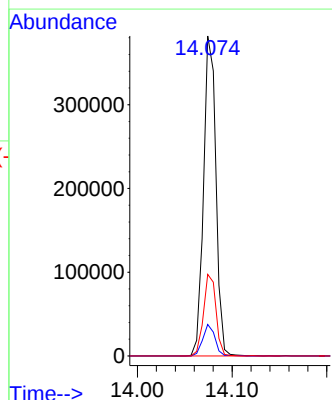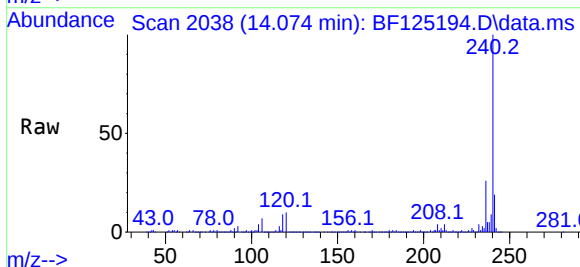



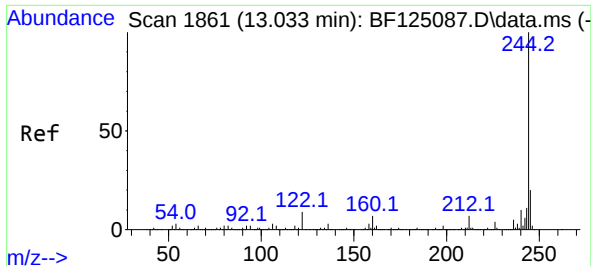


#79
Terphenyl-d14
Concen: 60.512 ng
RT: 13.021 min Scan# 1859
Delta R.T. 0.000 min
Lab File: BF125194.D
Acq: 24 Aug 2021 20:04

Instrument :
BNA_F
ClientSampled :
PE-5

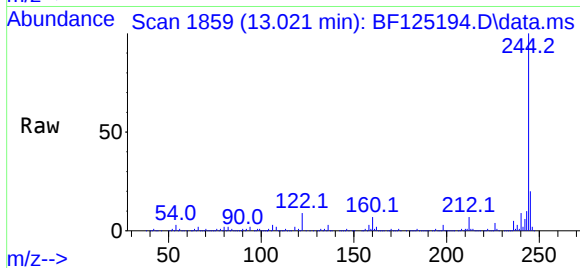

Tgt Ion:244 Resp: 1313448
Ion Ratio Lower Upper
244 100
212 7.1 5.9 8.9
122 9.1 9.0 13.4

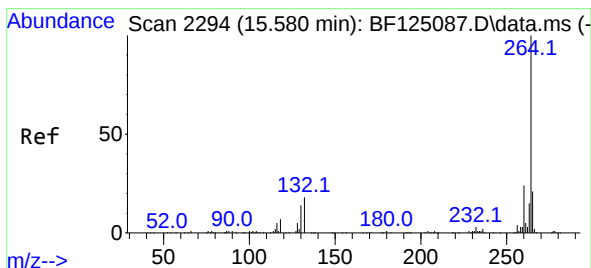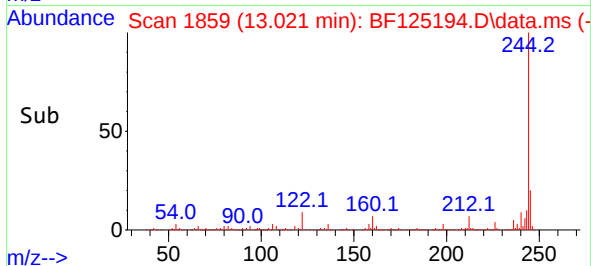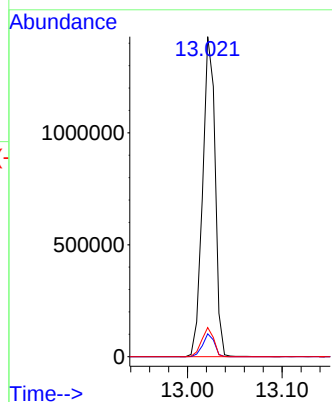

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.574 min Scan# 2293
Delta R.T. 0.000 min
Lab File: BF125194.D
Acq: 24 Aug 2021 20:04

Tgt Ion:264 Resp: 370512
Ion Ratio Lower Upper
264 100
260 23.9 19.6 29.4
265 21.6 17.2 25.8

