
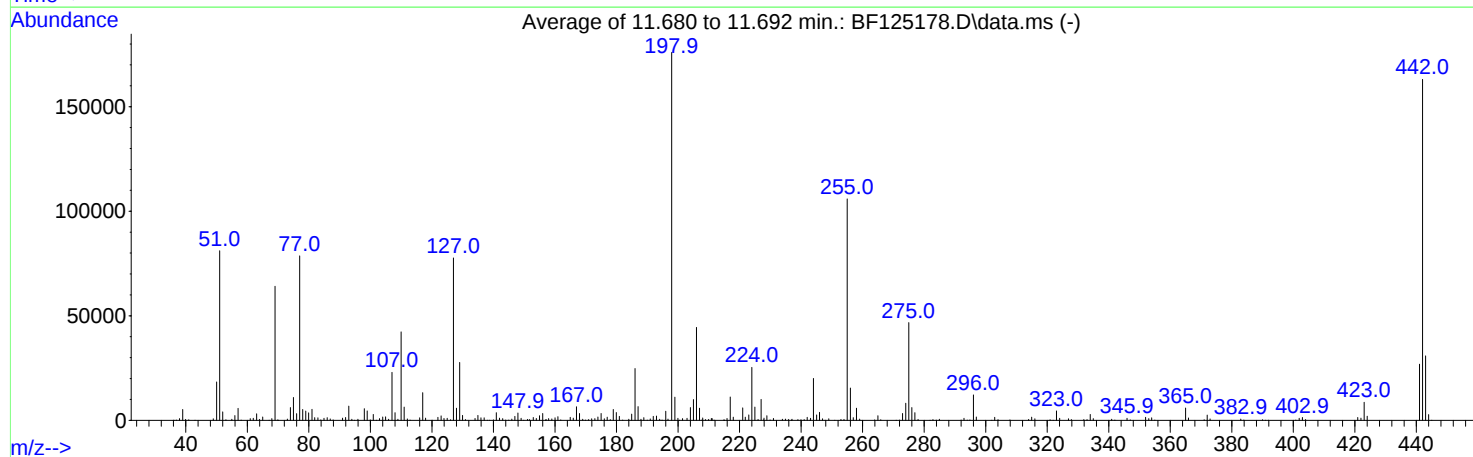


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082421\
 Data File : BF125178.D
 Acq On : 24 Aug 2021 11:10
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 24 12:39:21 2021

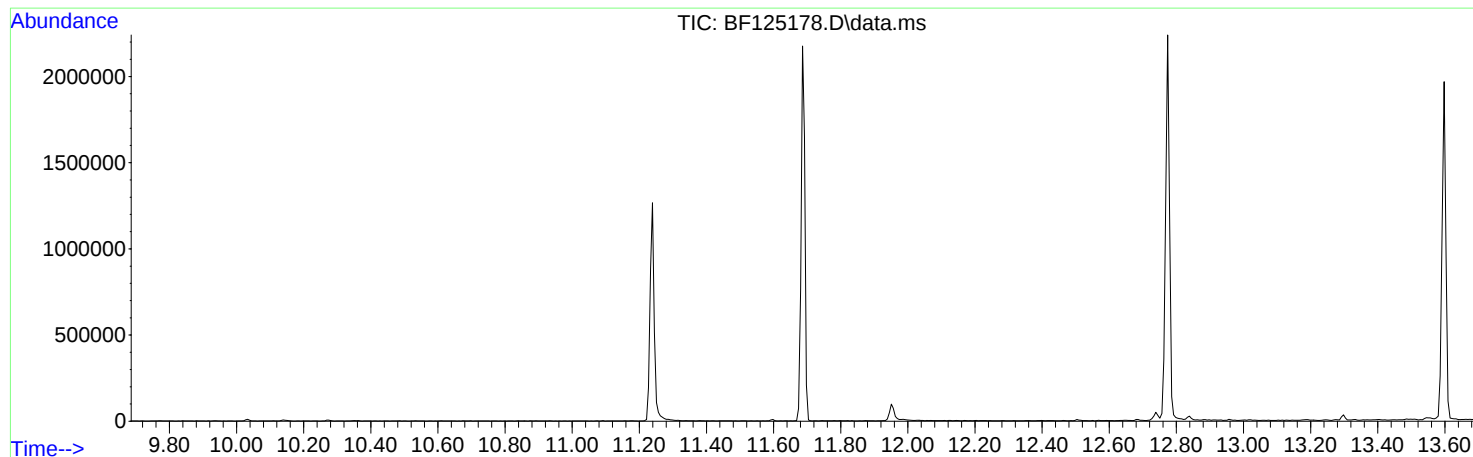




AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	81077	PASS
68	69	0.00	2	1.3	810	PASS
69	198	0.00	100	36.4	64115	PASS
70	69	0.00	2	0.4	234	PASS
127	198	10	80	44.2	77696	PASS
197	198	0.00	2	0.4	627	PASS
198	198	100	100	100.0	175912	PASS
199	198	5	9	6.3	11088	PASS
275	198	10	60	26.6	46741	PASS
365	198	1	100	3.3	5856	PASS
441	198	0.01	100	15.3	26837	PASS
442	442	50	100	100.0	163075	PASS
443	442	15	24	18.9	30837	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082421\
 Data File : BF125178.D
 Acq On : 24 Aug 2021 11:10
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 24 12:35:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 23 10:15:49 2021
 Response via : Initial Calibration

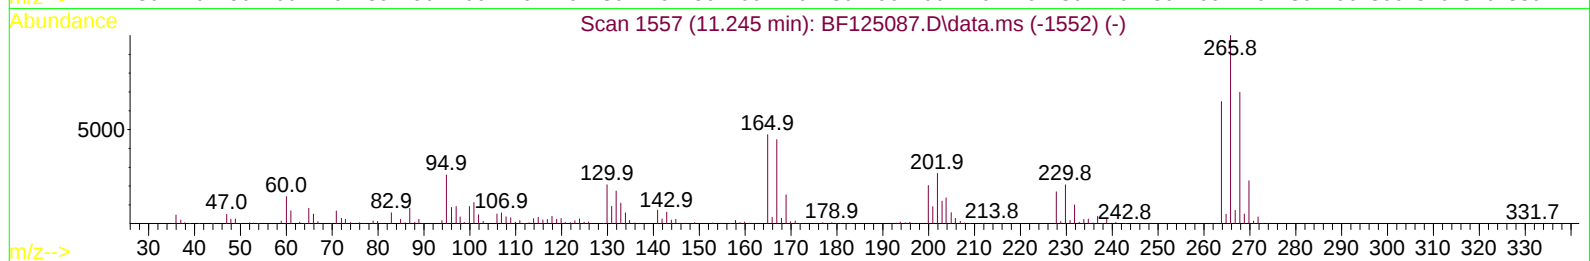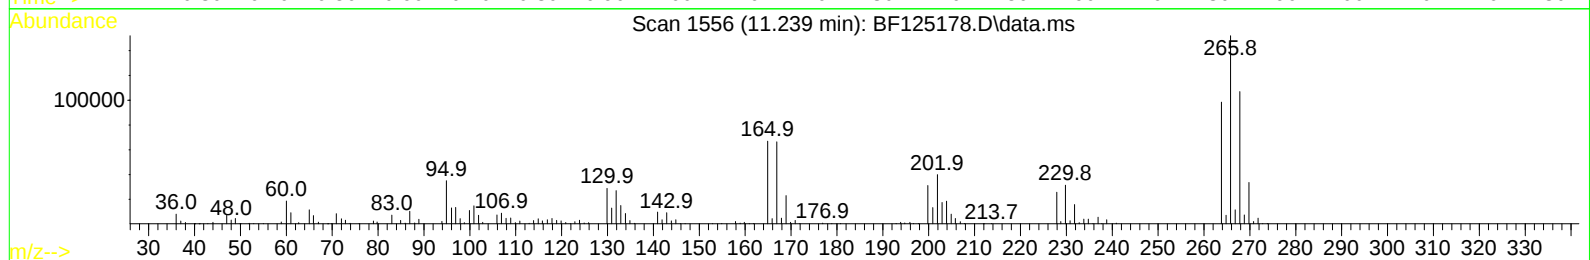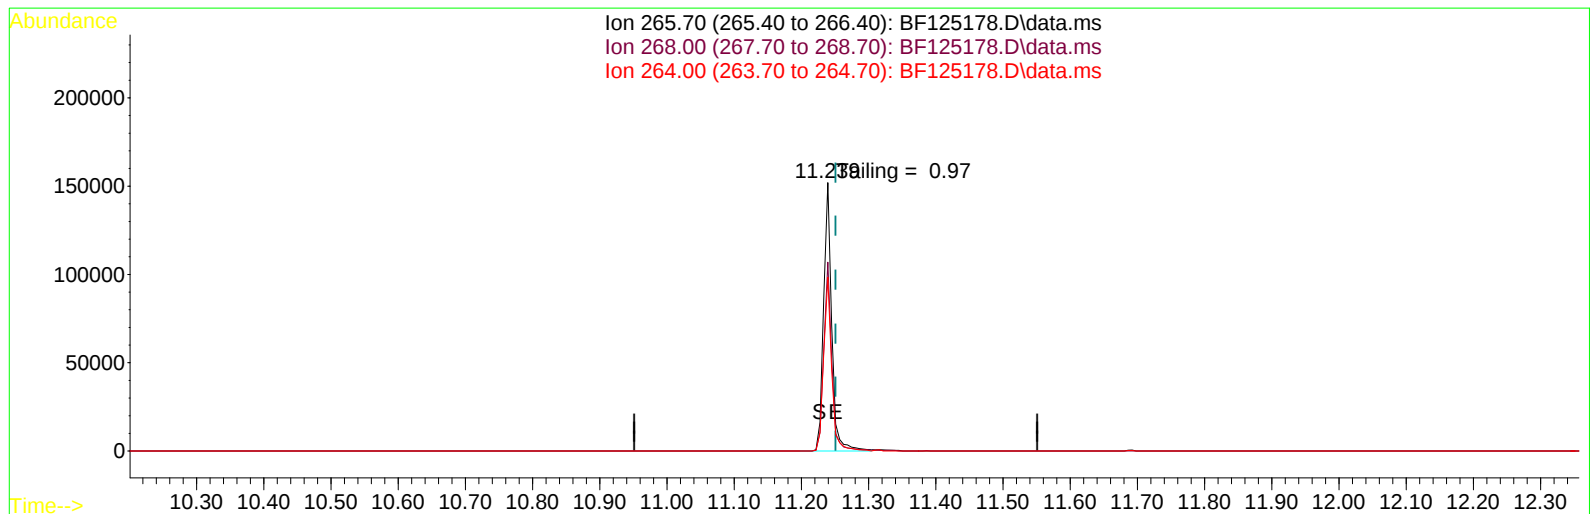

TIC: BF125178.D\data.ms

(70) Pentachlorophenol (C)

11.239min (-0.012) 31055.80 ng




response 130148

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	70.38
264.00	69.90	64.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082421\
Data File : BF125178.D
Acq On : 24 Aug 2021 11:10
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 24 12:35:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 23 10:15:49 2021
Response via : Initial Calibration

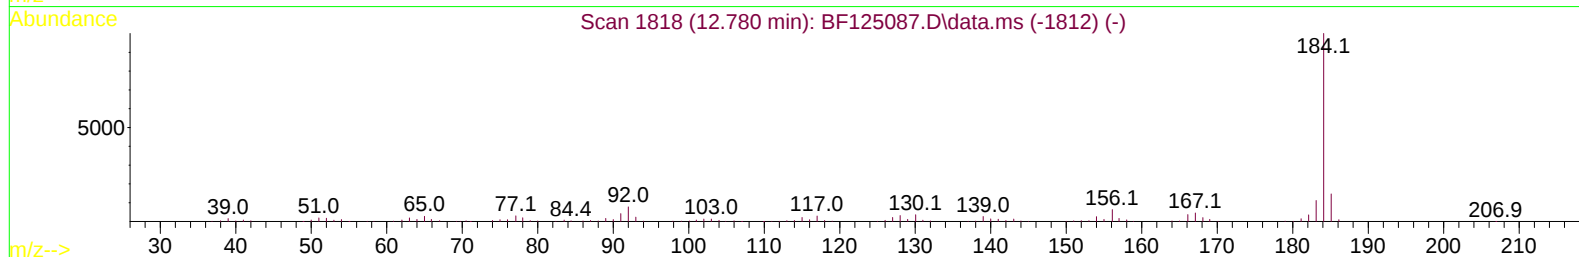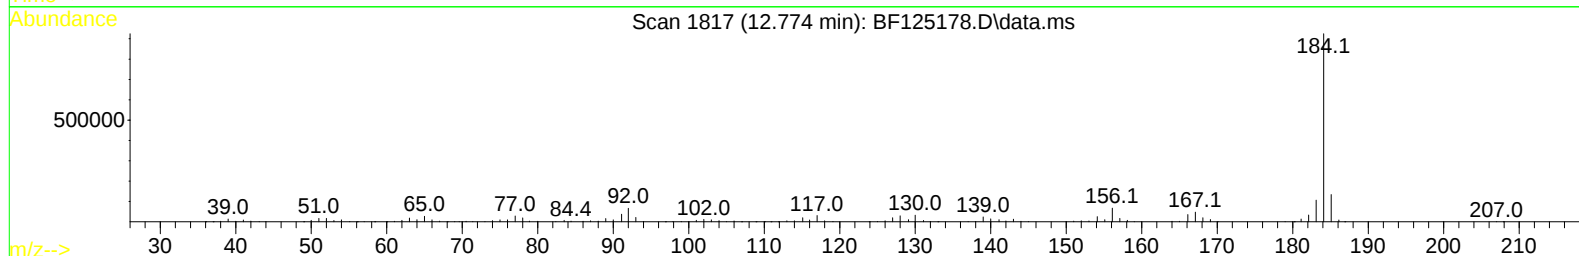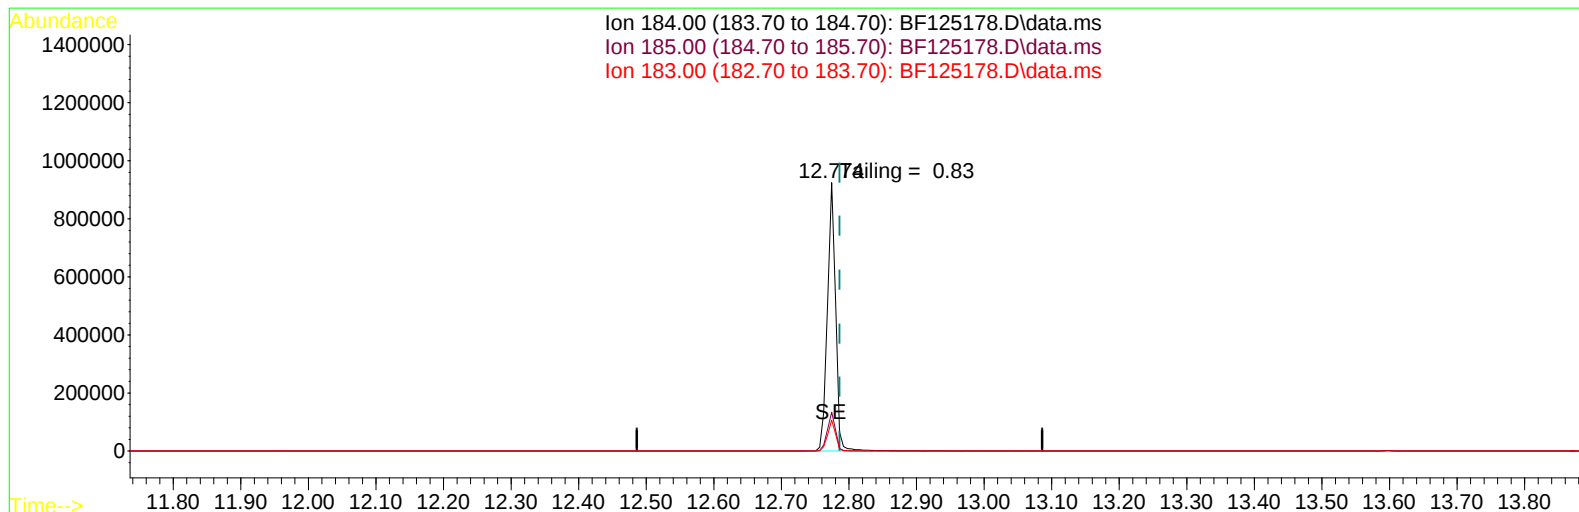

TIC: BF125178.D\data.ms

(77) Benzidine

12.774min (-0.012) 0.00 ng

response 783248

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.50
183.00	10.10	11.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/24/2021	BNA_F	<u>BF125178.D</u>
Compound Name	Response	Retention Time
DDT	296102	13.59
DDD	5780	13.29
DDE	747	12.95
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6527	302629	2.16

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP