
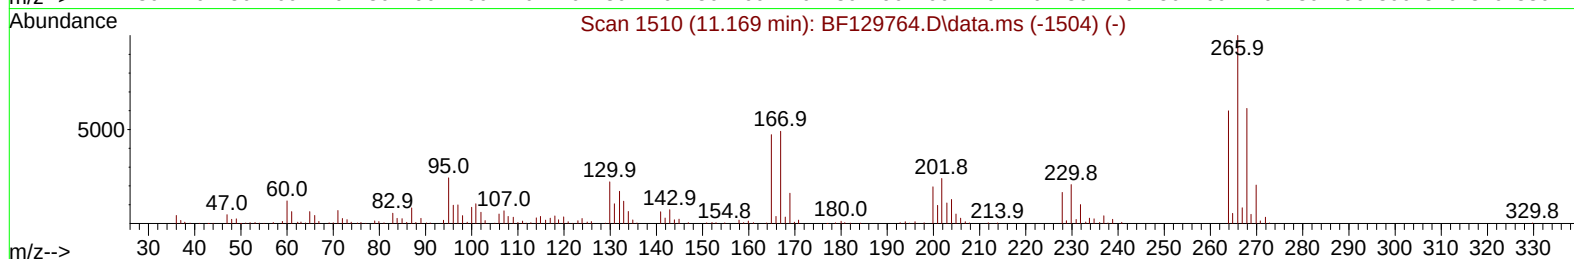
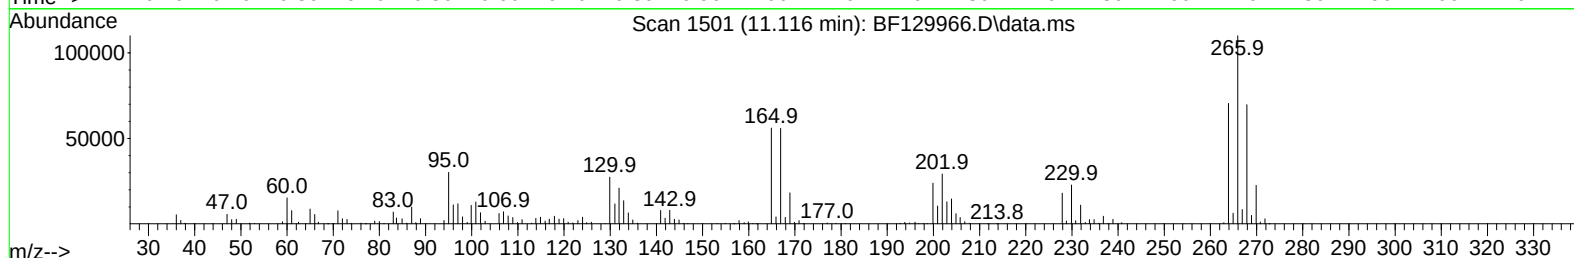


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
Data File : BF129966.D
Acq On : 24 Aug 2022 09:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 07:45:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 04:08:38 2022
Response via : Initial Calibration

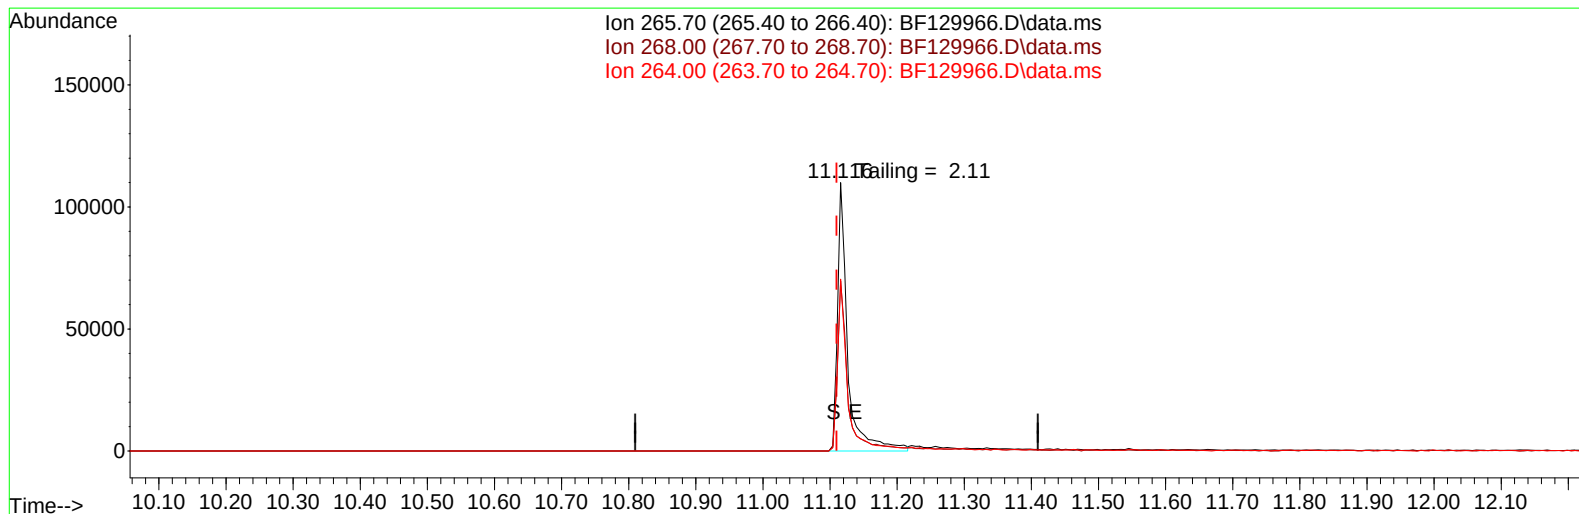

TIC: BF129966.D\data.ms

(70) Pentachlorophenol (C)




11.116min (+ 0.006) 102363.52 ng

response **116547**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.34
264.00	59.90	64.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
Data File : BF129966.D
Acq On : 24 Aug 2022 09:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 07:45:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 04:08:38 2022
Response via : Initial Calibration

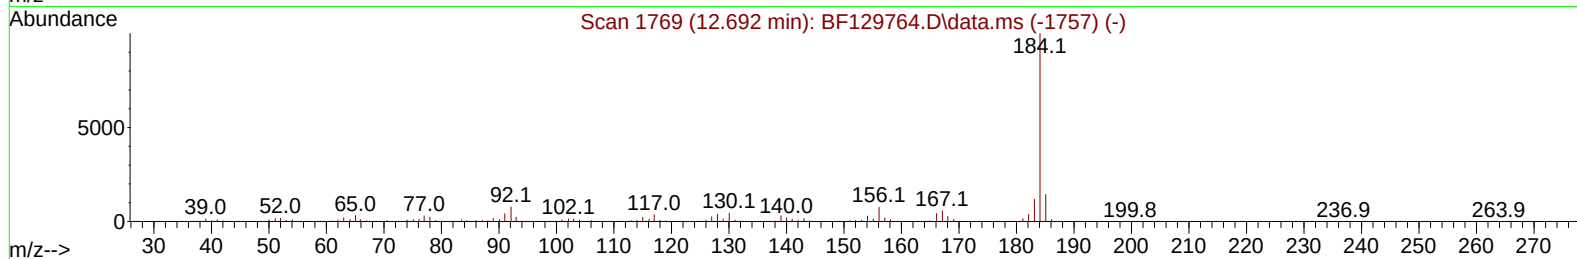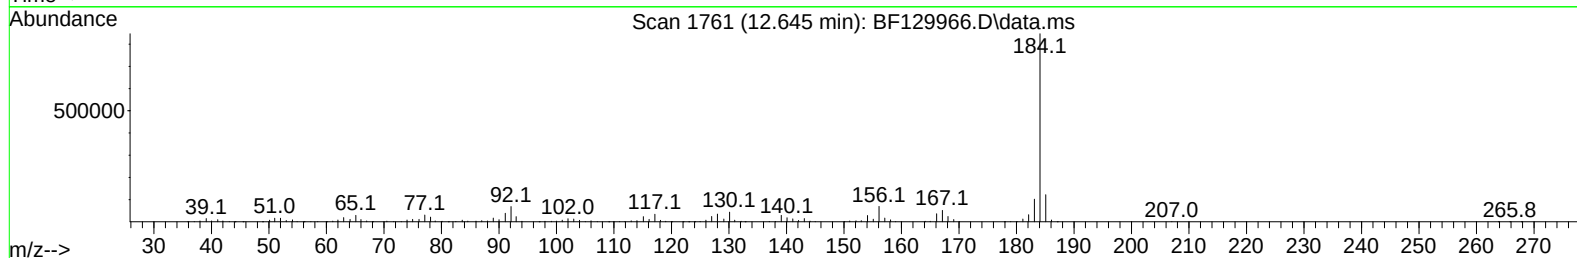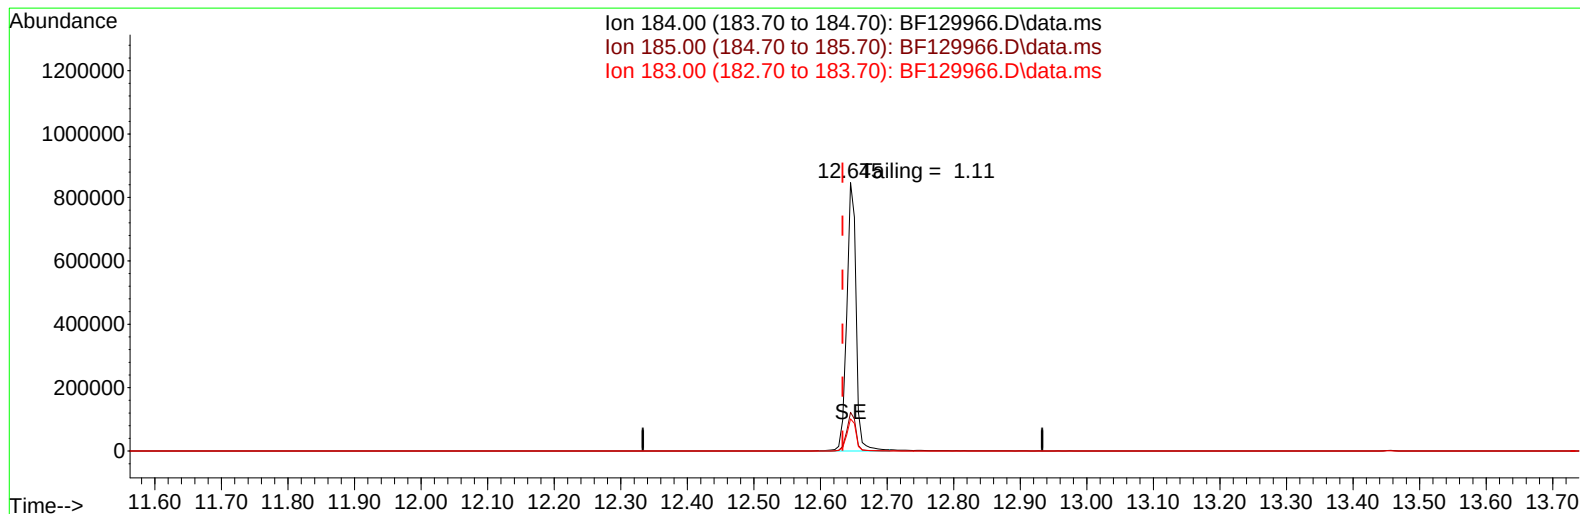

TIC: BF129966.D\data.ms

(77) Benzidine

12.645min (+ 0.012) 255976.21 ng

response 833564

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.43
183.00	11.80	12.00
0.00	0.00	0.00