
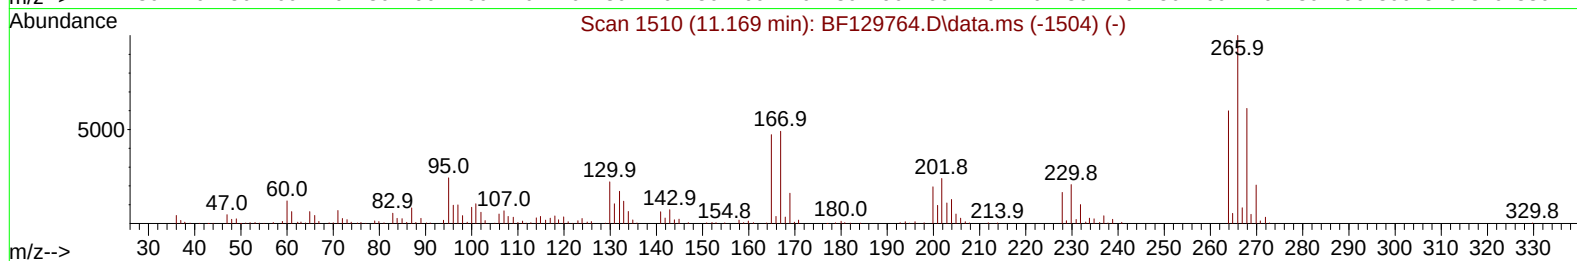
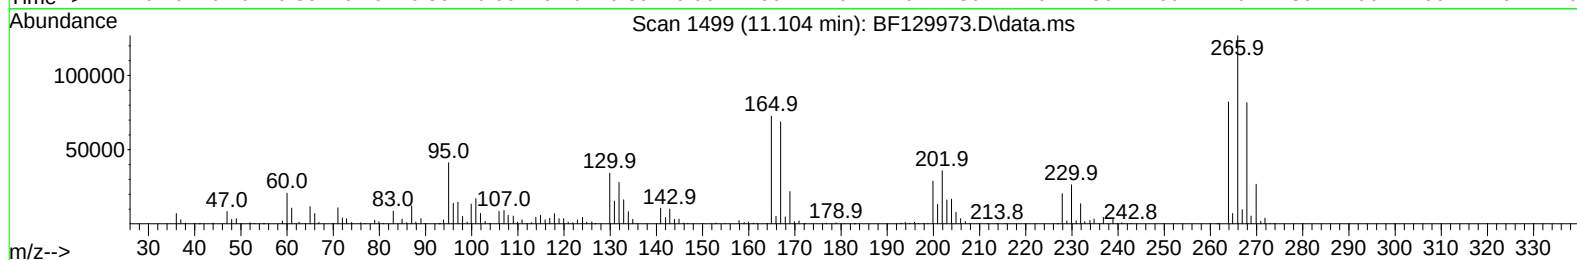


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
 Data File : BF129973.D
 Acq On : 24 Aug 2022 15:32
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 07:50:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 25 04:08:38 2022
 Response via : Initial Calibration

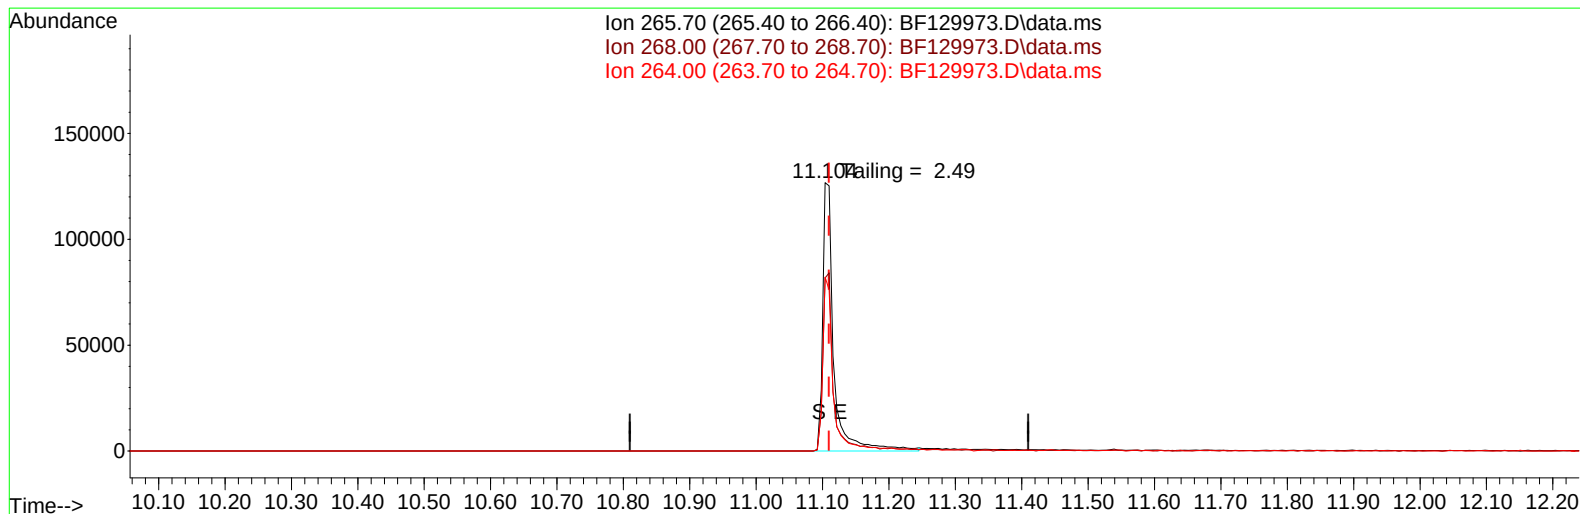

TIC: BF129973.D\data.ms

(70) Pentachlorophenol (C)




11.104min (-0.006) 181199.26 ng

response 146628

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.47
264.00	59.90	64.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
Data File : BF129973.D
Acq On : 24 Aug 2022 15:32
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 25 07:50:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 04:08:38 2022
Response via : Initial Calibration

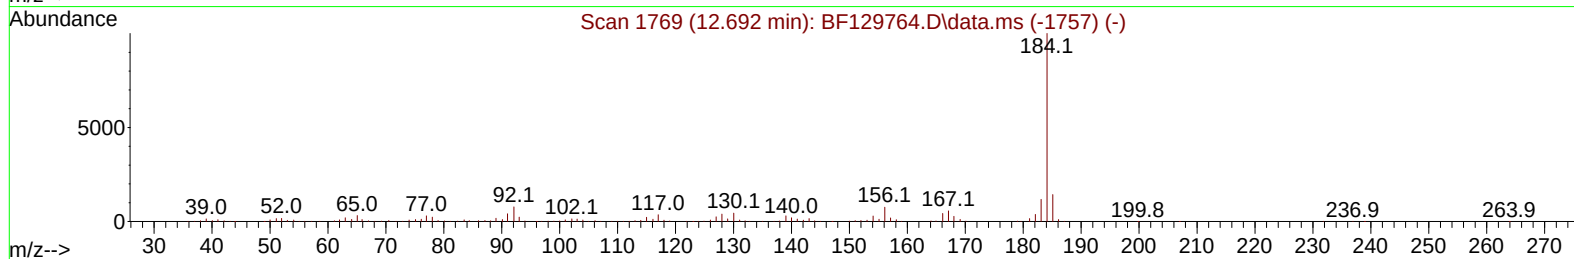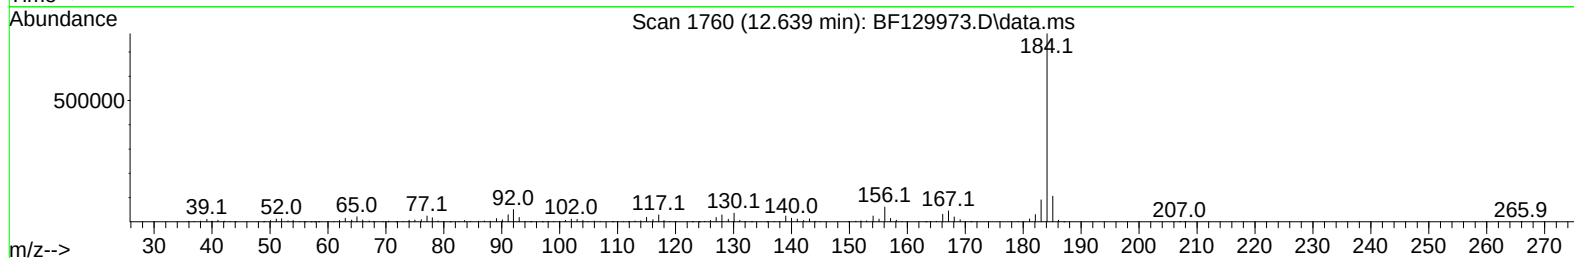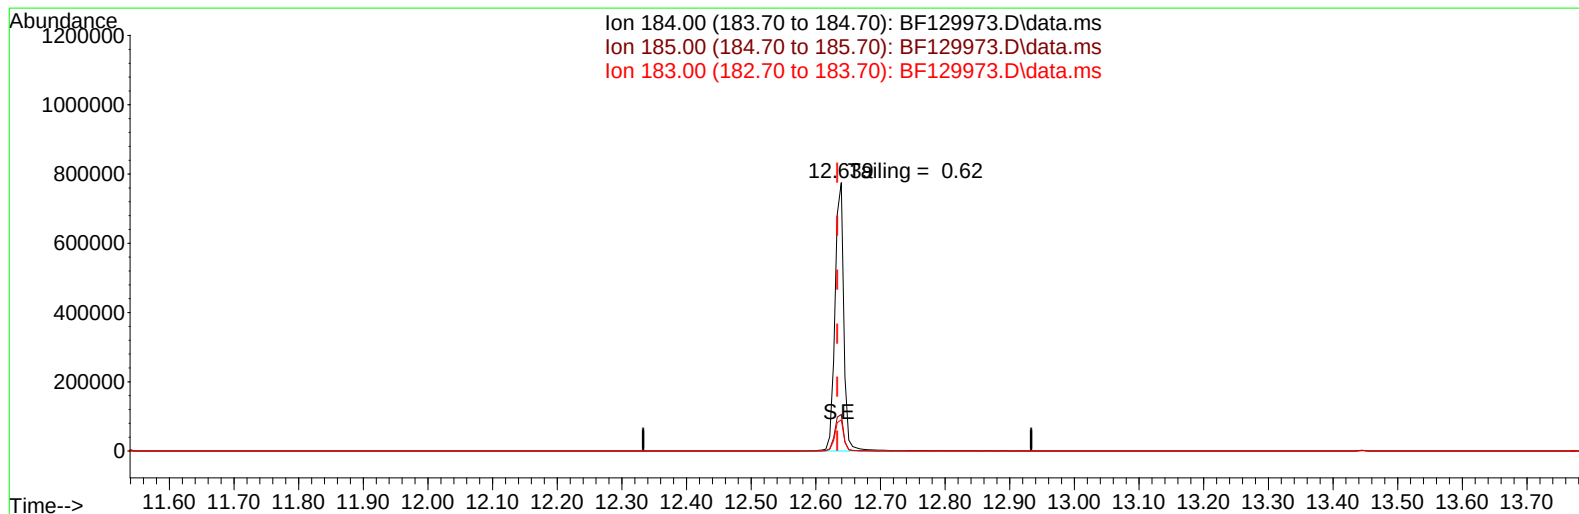

TIC: BF129973.D\data.ms

(77) Benzidine**12.639min (+ 0.006) 132098.78 ng****response 734654**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.62
183.00	11.80	11.66
0.00	0.00	0.00