

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
 Data File : BF129982.D
 Acq On : 24 Aug 2022 20:57
 Operator : CG\JU
 Sample : N4262-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-102D

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129982.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.987	457	459	474	rVB	39674	56266	1.44%	0.304%
2	5.404	527	530	559	rBV	1331673	1518897	38.96%	8.205%
3	6.428	701	704	720	rBV	836952	924945	23.72%	4.997%
4	6.763	758	761	771	rBV	801744	685238	17.57%	3.702%
5	7.340	854	859	875	rBV	2187908	2175411	55.79%	11.752%
6	8.045	976	979	989	rBV	1058423	906410	23.25%	4.897%
7	9.122	1157	1162	1165	rBV	4812283	3899055	100.00%	21.064%
8	9.798	1273	1277	1281	rBV	1206557	980352	25.14%	5.296%
9	10.598	1409	1413	1416	rBV	2299251	2174834	55.78%	11.749%
10	11.286	1527	1530	1534	rBV	980859	882260	22.63%	4.766%
11	12.875	1795	1800	1803	rBV	3406829	2856317	73.26%	15.431%
12	13.933	1977	1980	1985	rBV	647080	615275	15.78%	3.324%
13	14.022	1990	1995	2000	rBV	185757	182712	4.69%	0.987%
14	14.992	2154	2160	2165	rVB2	34358	48930	1.25%	0.264%
15	15.386	2223	2227	2237	rVB	484891	603913	15.49%	3.262%




Sum of corrected areas: 18510815

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
Data File : BF129982.D
Acq On : 24 Aug 2022 20:57
Operator : CG\JU
Sample : N4262-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-102D

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

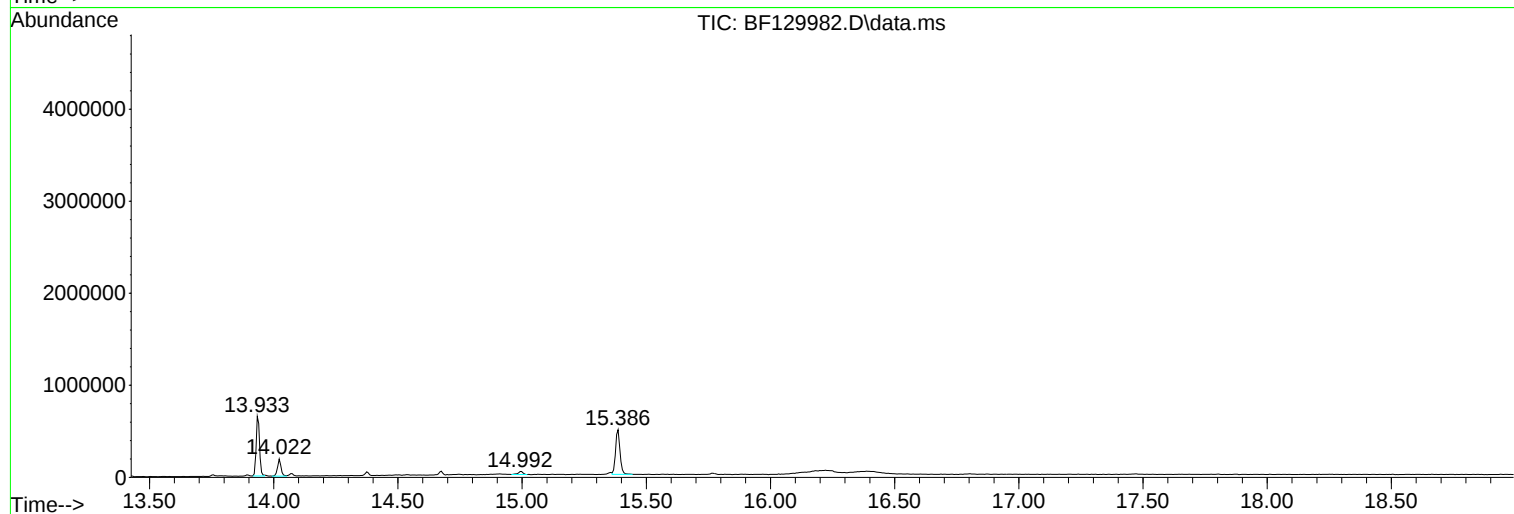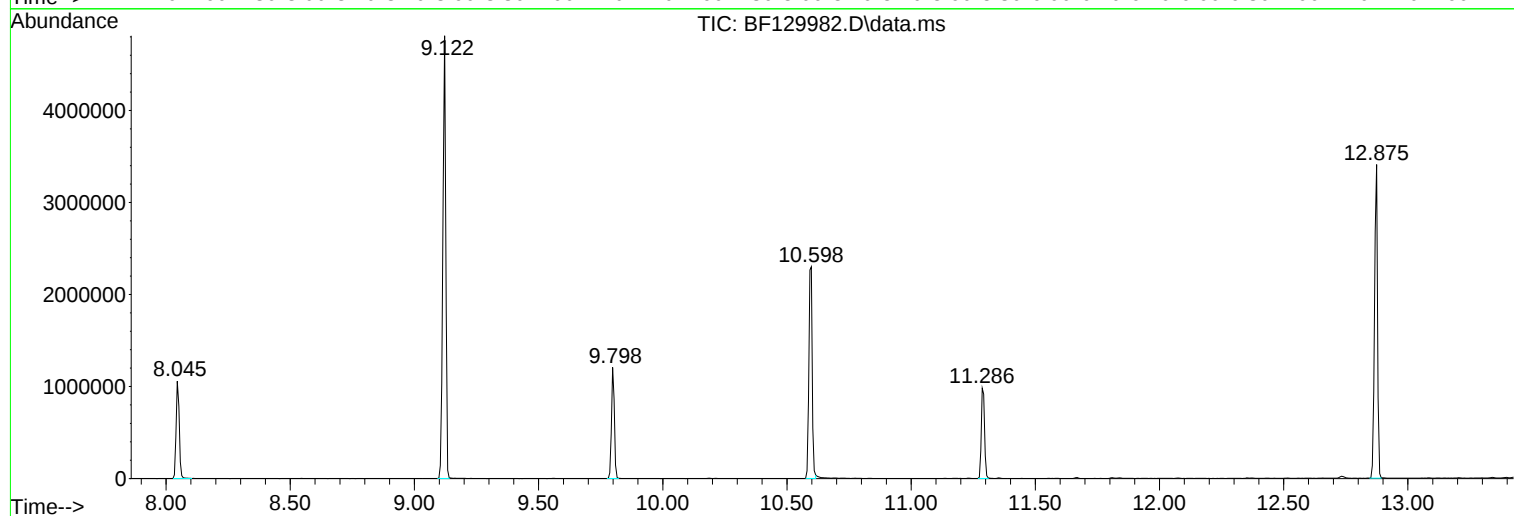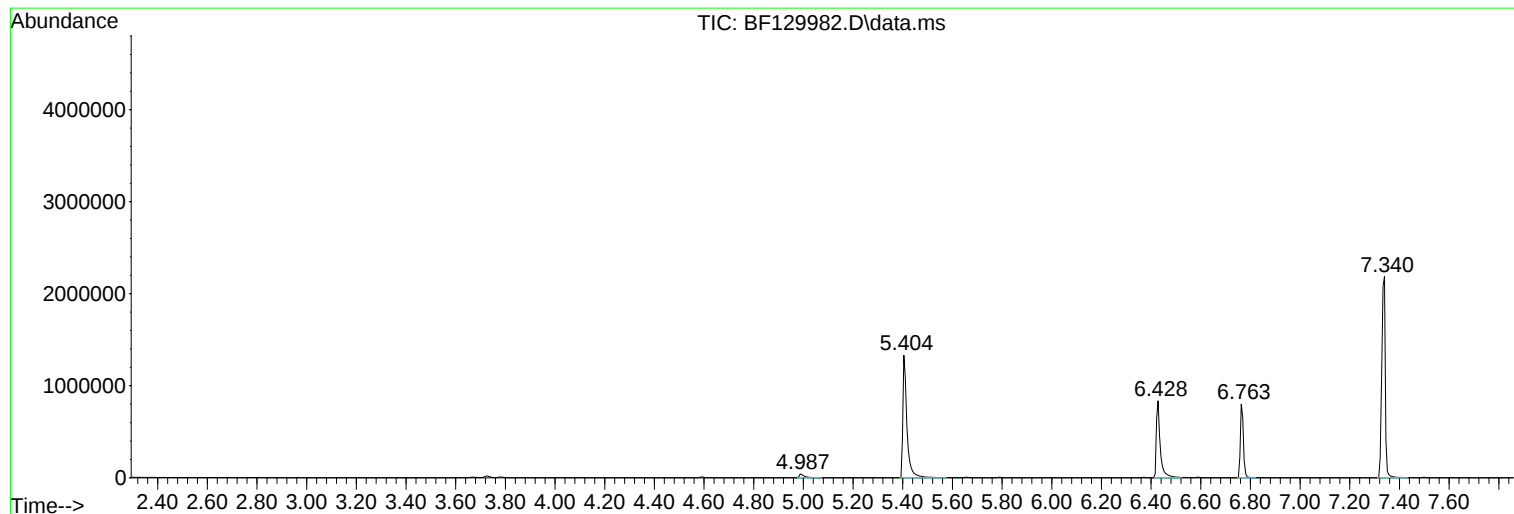

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
Data File : BF129982.D
Acq On : 24 Aug 2022 20:57
Operator : CG\JU
Sample : N4262-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-102D










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.022	5.94 ng	182712	Chrysene-d12	13.933

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	97
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	76
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	50
4			1H-Indole-3-acetic acid, 5-[(tri...]	277	C14H19N03Si	072101-35-0	17
5			5-quinolinol, 8-[2-(3,5-dimethyl...]	277	C17H15N3O	1000397-10-2	9

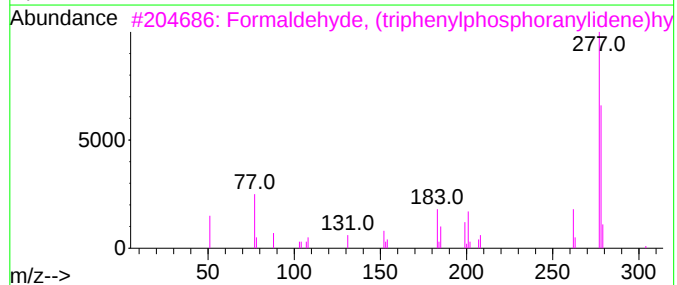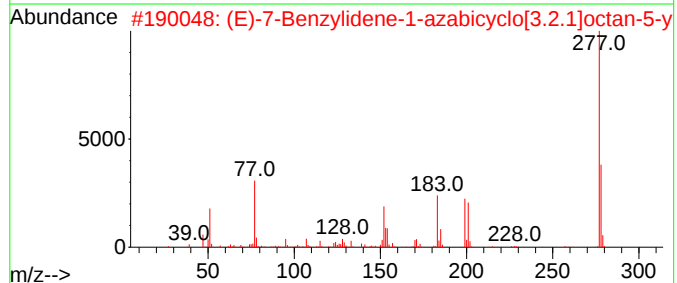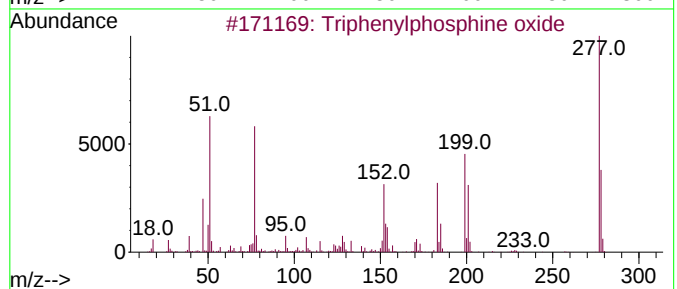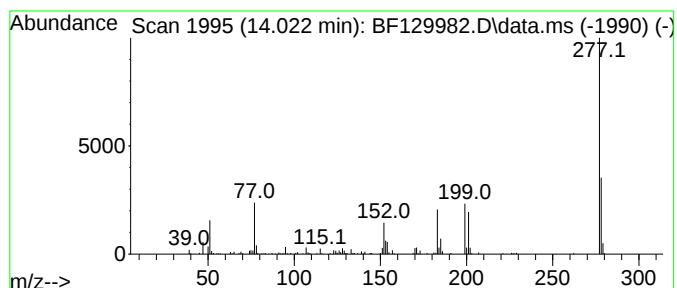

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
Data File : BF129982.D
Acq On : 24 Aug 2022 20:57
Operator : CG\JU
Sample : N4262-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-102D

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.022	5.9	ng	182712	5	13.933	615275	20.0