

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
 Data File : BF129984.D
 Acq On : 24 Aug 2022 22:07
 Operator : CG\JU
 Sample : N4262-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-1021

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129984.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.346	3	10	22	rVB	47359	75120	1.86%	0.387%
2	4.457	364	369	379	rBV	350093	418530	10.38%	2.155%
3	4.987	457	459	475	rBV	44259	63855	1.58%	0.329%
4	5.404	527	530	558	rBV	1494362	1613345	40.01%	8.308%
5	6.428	701	704	722	rBV	847567	987026	24.48%	5.083%
6	6.763	758	761	771	rBV	786038	665768	16.51%	3.429%
7	7.333	854	858	872	rBV	2229057	2218584	55.03%	11.425%
8	8.045	976	979	989	rBV	1040084	885084	21.95%	4.558%
9	9.122	1157	1162	1165	rBV	4908758	4031920	100.00%	20.763%
10	9.798	1274	1277	1281	rBV	1253308	966313	23.97%	4.976%
11	10.598	1409	1413	1416	rBV	2633485	2328367	57.75%	11.990%
12	11.286	1527	1530	1534	rBV	1023508	876185	21.73%	4.512%
13	12.874	1795	1800	1803	rBV	3064657	2910102	72.18%	14.986%
14	13.933	1977	1980	1989	rBV	641687	604905	15.00%	3.115%
15	14.021	1991	1995	2000	rBV	235497	219849	5.45%	1.132%
16	15.386	2223	2227	2233	rVB2	435304	553534	13.73%	2.851%




Sum of corrected areas: 19418487

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
Data File : BF129984.D
Acq On : 24 Aug 2022 22:07
Operator : CG\JU
Sample : N4262-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-102I

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

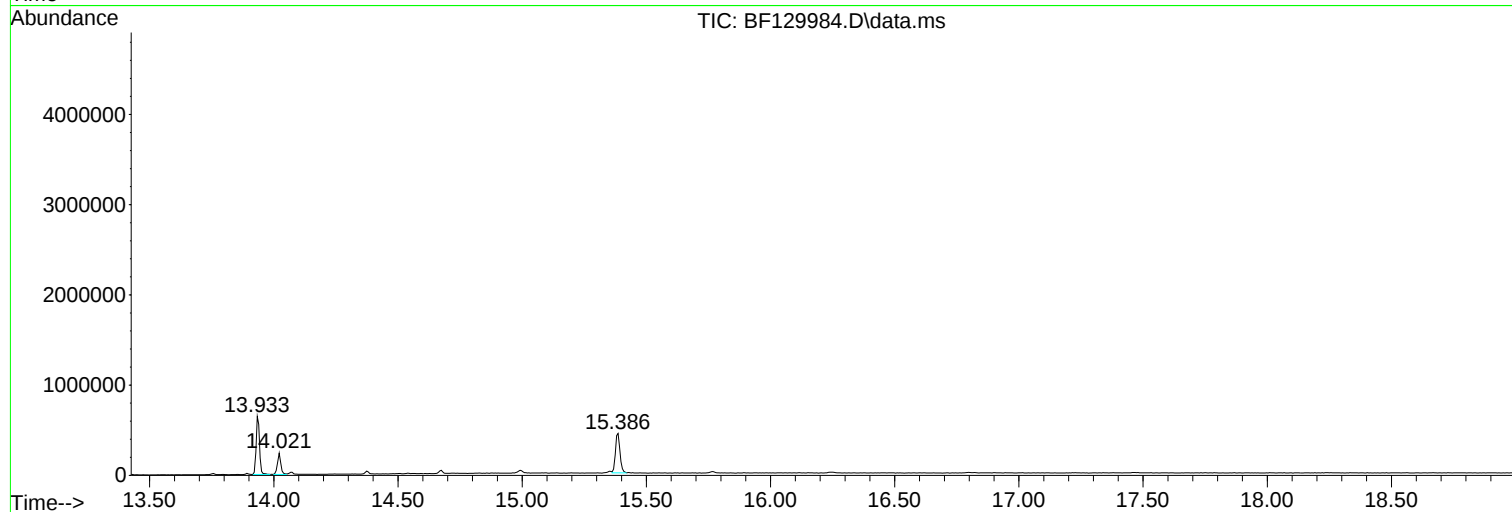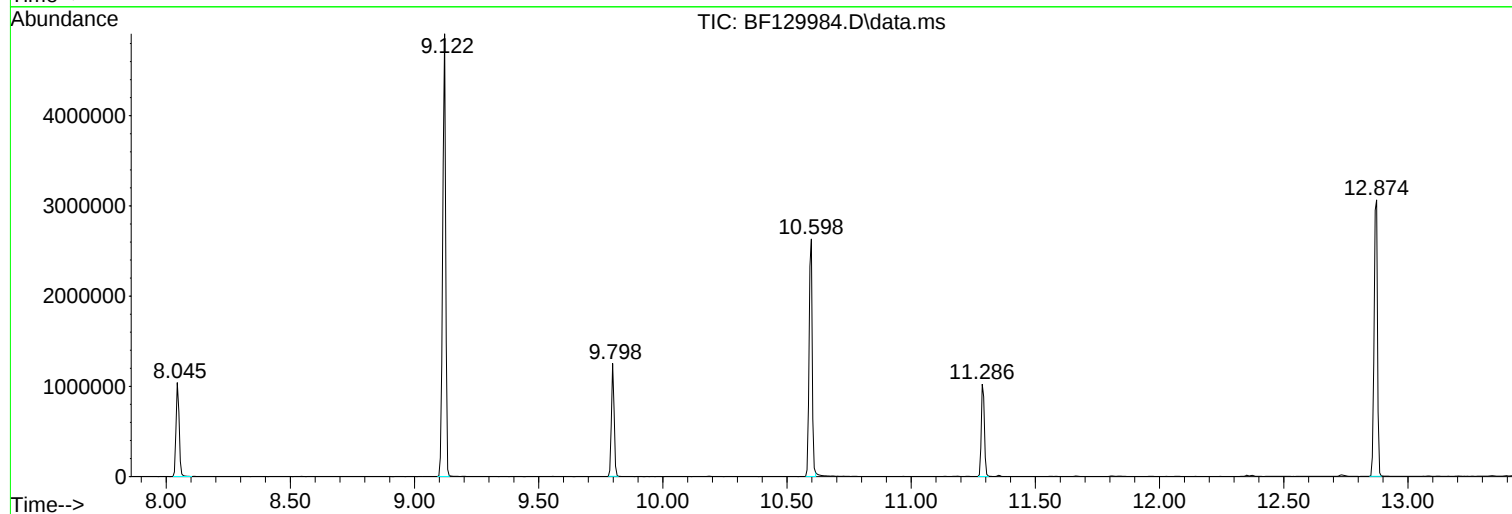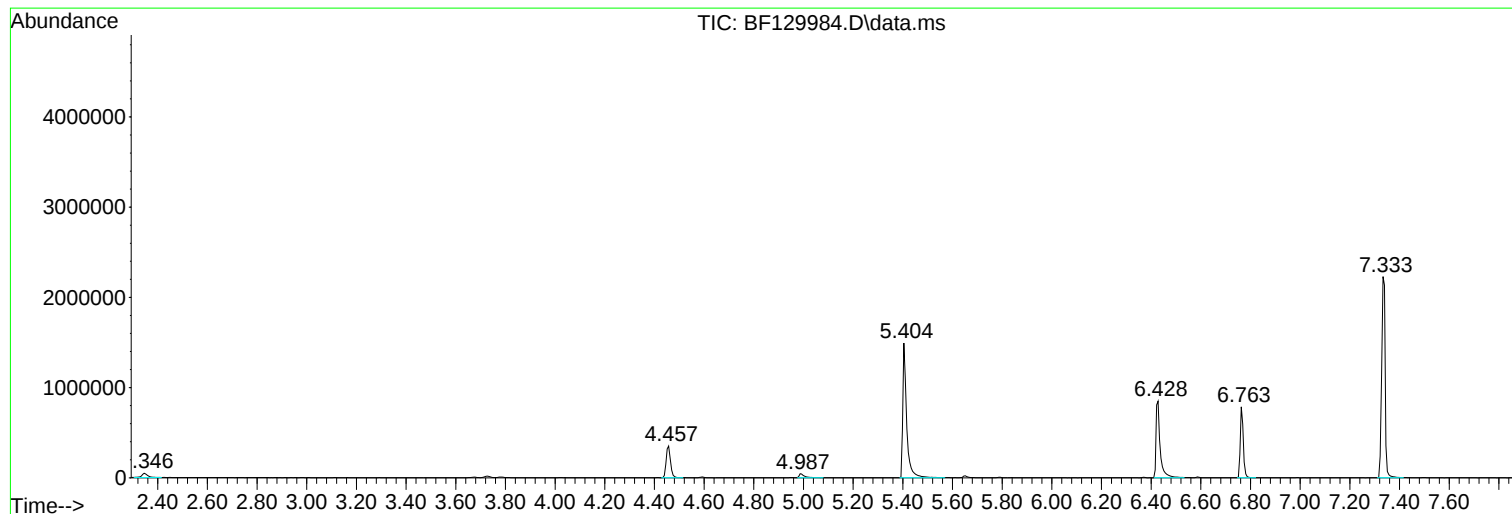

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
Data File : BF129984.D
Acq On : 24 Aug 2022 22:07
Operator : CG\JU
Sample : N4262-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-102I










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Triphenylphosphine oxide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.021	7.27 ng	219849	Chrysene-d12	13.933

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	97
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	50
4			Vanadium, cycloheptatrienyl-(pen...]	277	C17H22V	1000155-20-5	25
5			1H-Indole-3-acetic acid, 5-[(tri...]	277	C14H19N03Si	072101-35-0	17

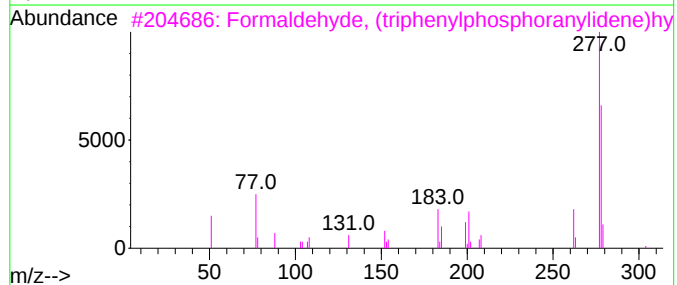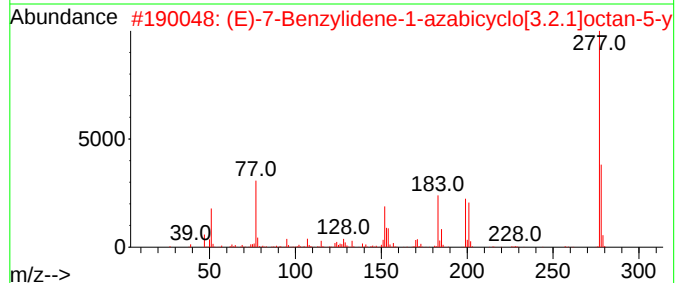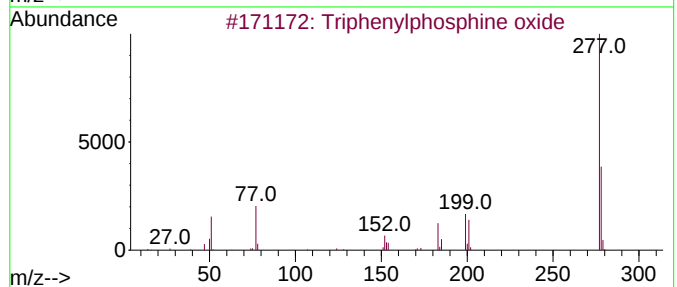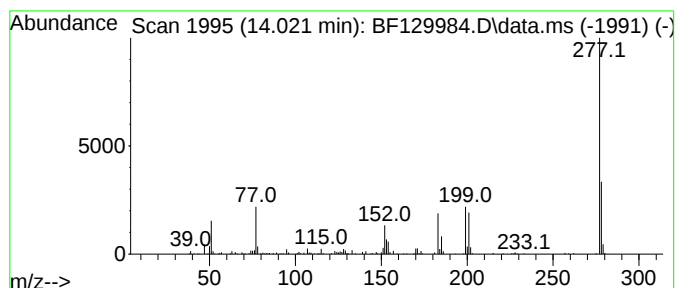

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
Data File : BF129984.D
Acq On : 24 Aug 2022 22:07
Operator : CG\JU
Sample : N4262-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-102I

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.021	7.3	ng	219849	5	13.933	604905	20.0