

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
 Data File : BF129985.D
 Acq On : 24 Aug 2022 22:43
 Operator : CG\JU
 Sample : N4262-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-101S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129985.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.340	3	9	18	rVB	101394	152273	4.21%	0.904%
2	2.481	31	33	42	rBV	38219	58993	1.63%	0.350%
3	4.457	365	369	380	rVB	71212	87188	2.41%	0.518%
4	4.987	456	459	472	rBV	41172	57365	1.58%	0.341%
5	5.404	528	530	553	rBV	1115313	1347978	37.24%	8.003%
6	6.428	701	704	719	rBV	726416	791403	21.86%	4.699%
7	6.763	758	761	770	rBV	708257	606989	16.77%	3.604%
8	7.334	854	858	869	rBV	2066499	2036889	56.28%	12.094%
9	8.045	976	979	985	rBV	980989	795102	21.97%	4.721%
10	9.122	1157	1162	1165	rBV	4467285	3619511	100.00%	21.490%
11	9.798	1274	1277	1281	rBV	1078951	835261	23.08%	4.959%
12	10.592	1409	1412	1422	rBV	2186654	1956225	54.05%	11.615%
13	11.286	1527	1530	1536	rBV	886942	737548	20.38%	4.379%
14	12.875	1795	1800	1803	rBV	2549192	2404578	66.43%	14.277%
15	13.933	1977	1980	1990	rVB	594875	535393	14.79%	3.179%
16	14.022	1990	1995	1999	rBV	255391	252254	6.97%	1.498%
17	14.992	2154	2160	2165	rBV3	32952	48499	1.34%	0.288%
18	15.386	2223	2227	2233	rVB	410046	519230	14.35%	3.083%




Sum of corrected areas: 16842679

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
Data File : BF129985.D
Acq On : 24 Aug 2022 22:43
Operator : CG\JU
Sample : N4262-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-101S

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

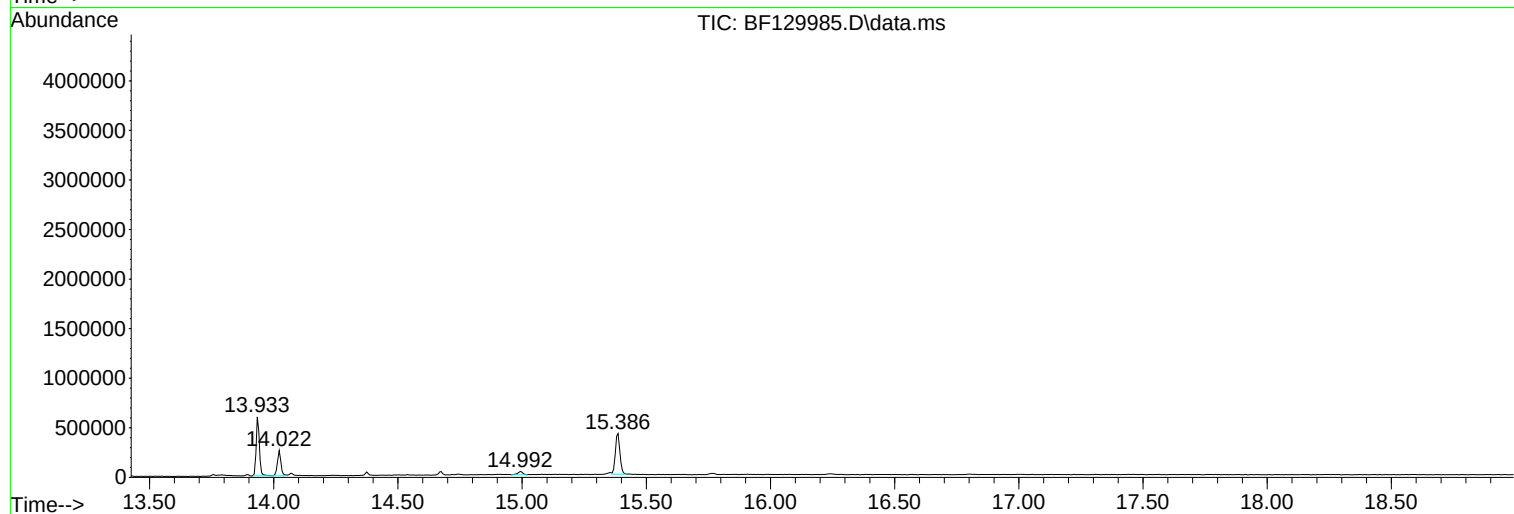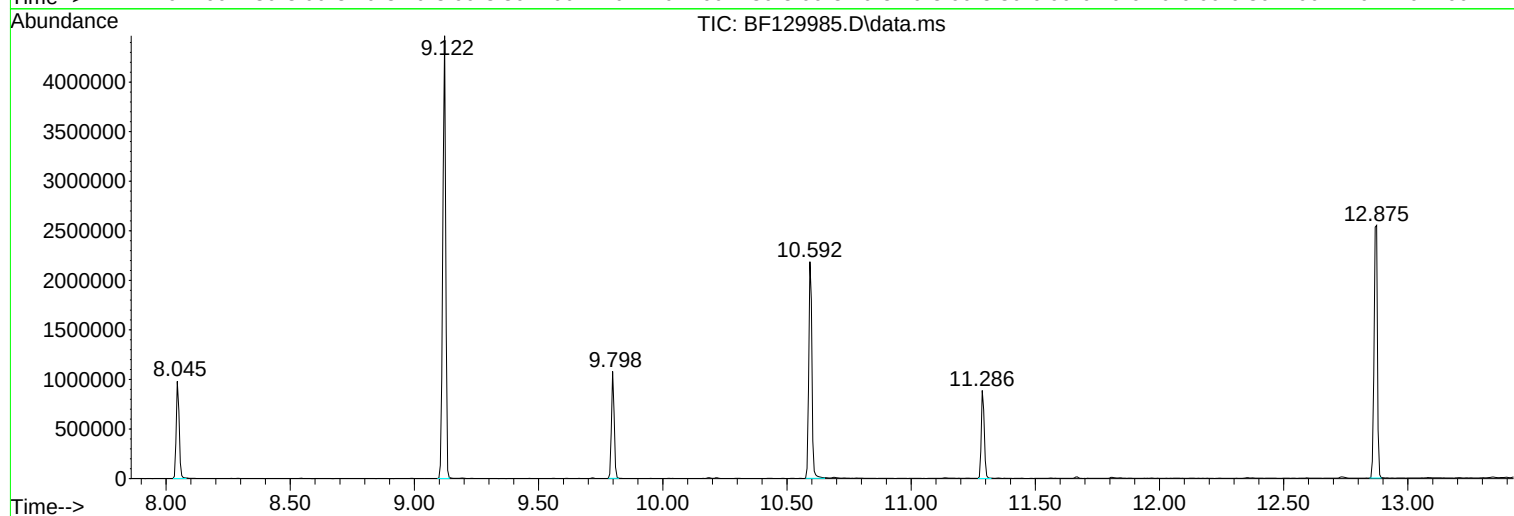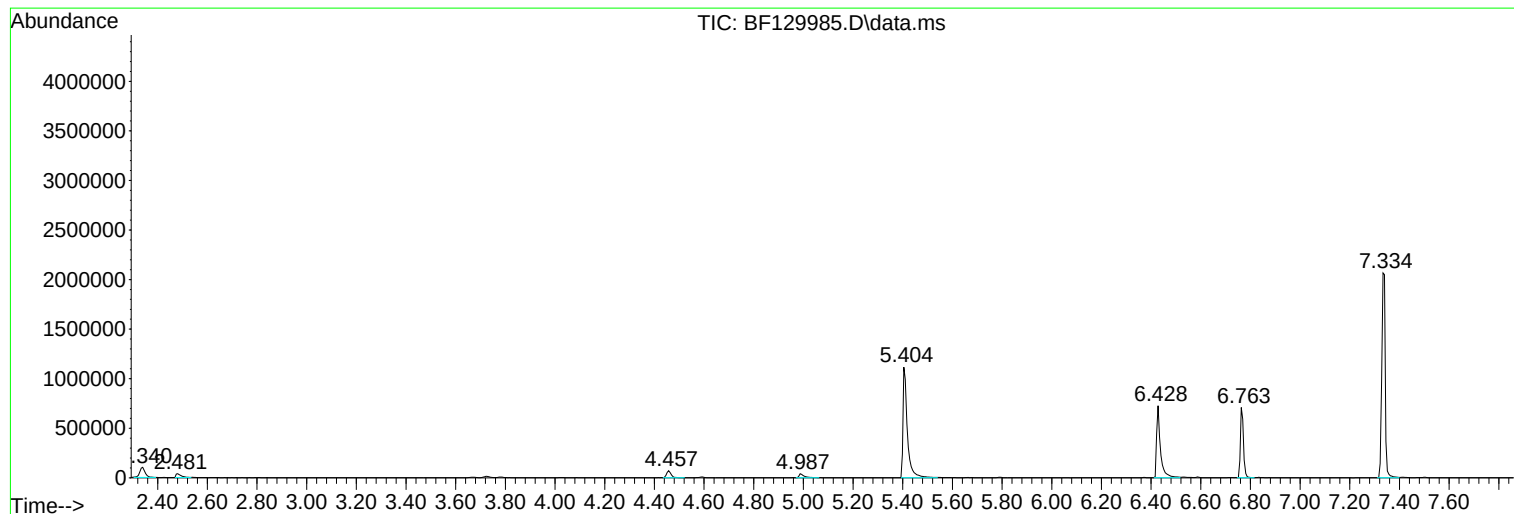

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
Data File : BF129985.D
Acq On : 24 Aug 2022 22:43
Operator : CG\JU
Sample : N4262-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-101S










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.022	9.42 ng	252254	Chrysene-d12	13.933

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	95
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	95
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	50
4			3-(3,4-Dichlorophenyl)-2-thioxo-...	277	C9H5Cl2NOS2	017046-34-3	25
5			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	23

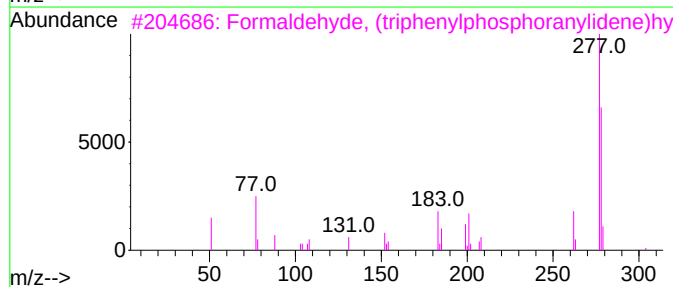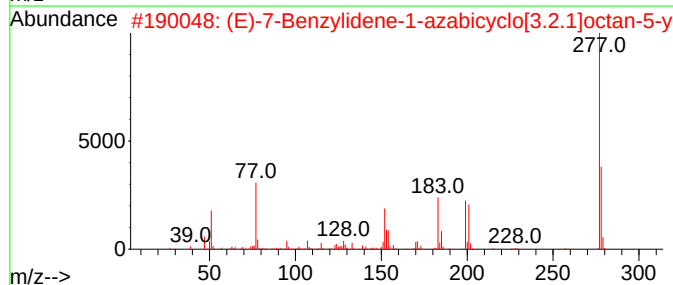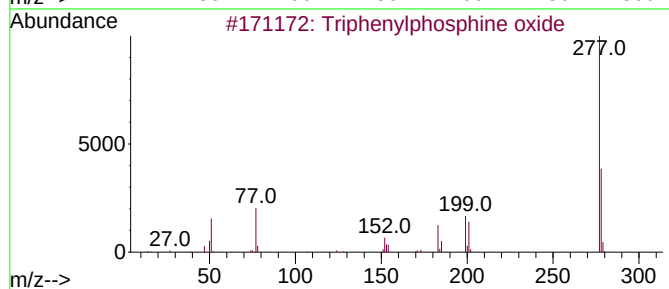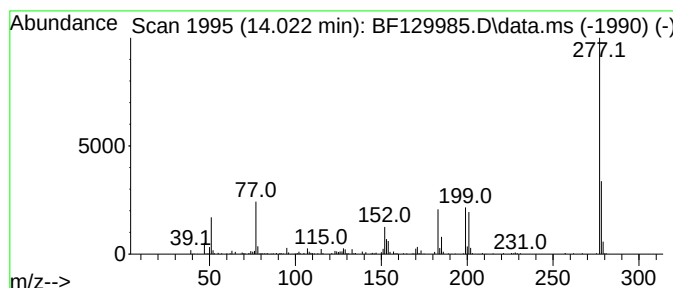

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
Data File : BF129985.D
Acq On : 24 Aug 2022 22:43
Operator : CG\JU
Sample : N4262-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-101S

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.022	9.4	ng	252254	5	13.933	535393	20.0