

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
 Data File : BF129986.D
 Acq On : 24 Aug 2022 23:18
 Operator : CG\JU
 Sample : N4262-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-101I

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129986.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.340	4	9	16	rVB	59050	87731	2.27%	0.470%
2	2.469	28	31	45	rBV	107960	159806	4.13%	0.856%
3	4.457	364	369	376	rVB	83537	105420	2.73%	0.564%
4	4.987	457	459	470	rBV	36634	54602	1.41%	0.292%
5	5.404	527	530	554	rBV	1406186	1537803	39.76%	8.233%
6	6.428	701	704	720	rBV	851892	990825	25.62%	5.304%
7	6.763	758	761	771	rBV	763160	651502	16.85%	3.488%
8	7.334	854	858	870	rBV	2163730	2144309	55.45%	11.480%
9	8.045	976	979	989	rBV	1047112	859851	22.23%	4.603%
10	9.122	1157	1162	1165	rBV	4688402	3867249	100.00%	20.704%
11	9.798	1274	1277	1281	rBV	1130347	900462	23.28%	4.821%
12	10.592	1409	1412	1426	rBV	2203840	2026920	52.41%	10.851%
13	11.286	1527	1530	1539	rBV	951785	799600	20.68%	4.281%
14	12.874	1795	1800	1803	rBV	3246617	2985894	77.21%	15.985%
15	13.786	1951	1955	1968	rVB6	24817	67010	1.73%	0.359%
16	13.933	1977	1980	1988	rBV	615982	569366	14.72%	3.048%
17	14.021	1990	1995	2001	rBV	247304	254042	6.57%	1.360%
18	14.992	2157	2160	2168	rVB	31721	47541	1.23%	0.255%
19	15.386	2223	2227	2236	rVB	466443	569125	14.72%	3.047%




Sum of corrected areas: 18679058

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
Data File : BF129986.D
Acq On : 24 Aug 2022 23:18
Operator : CG\JU
Sample : N4262-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-101I

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

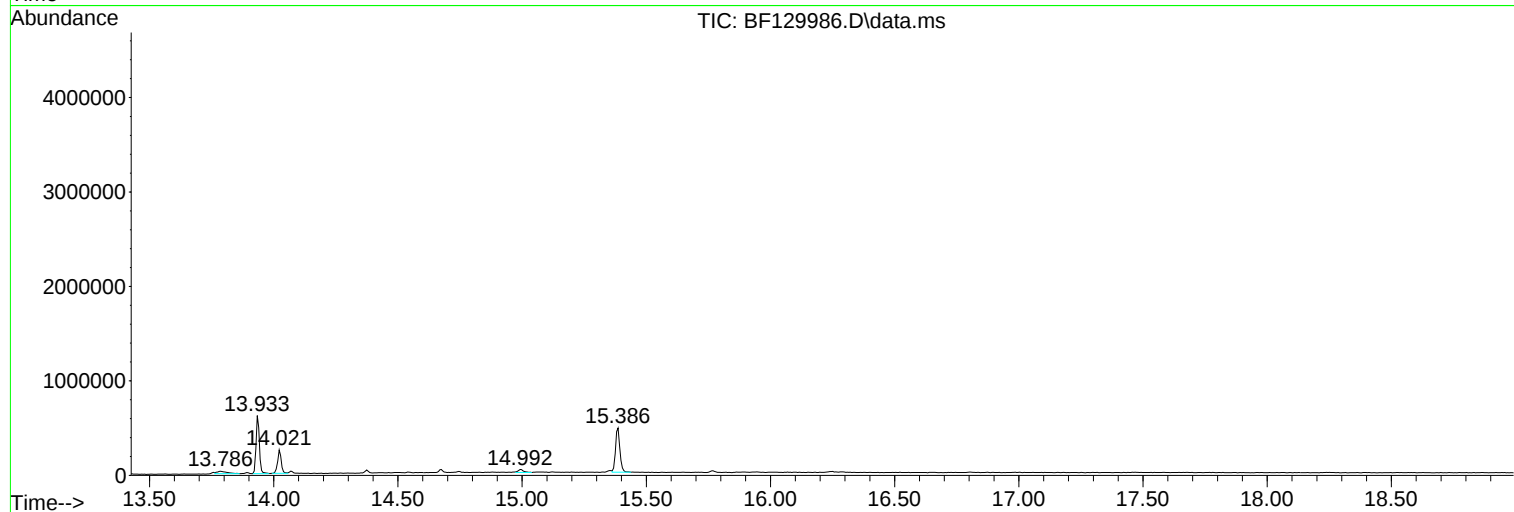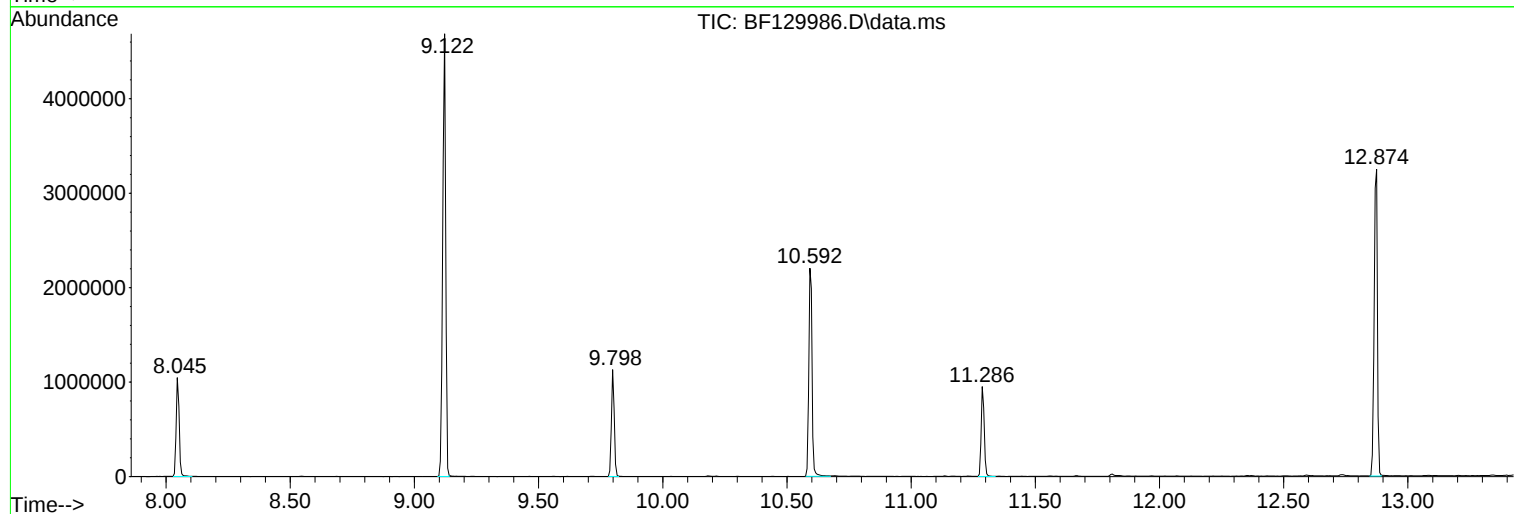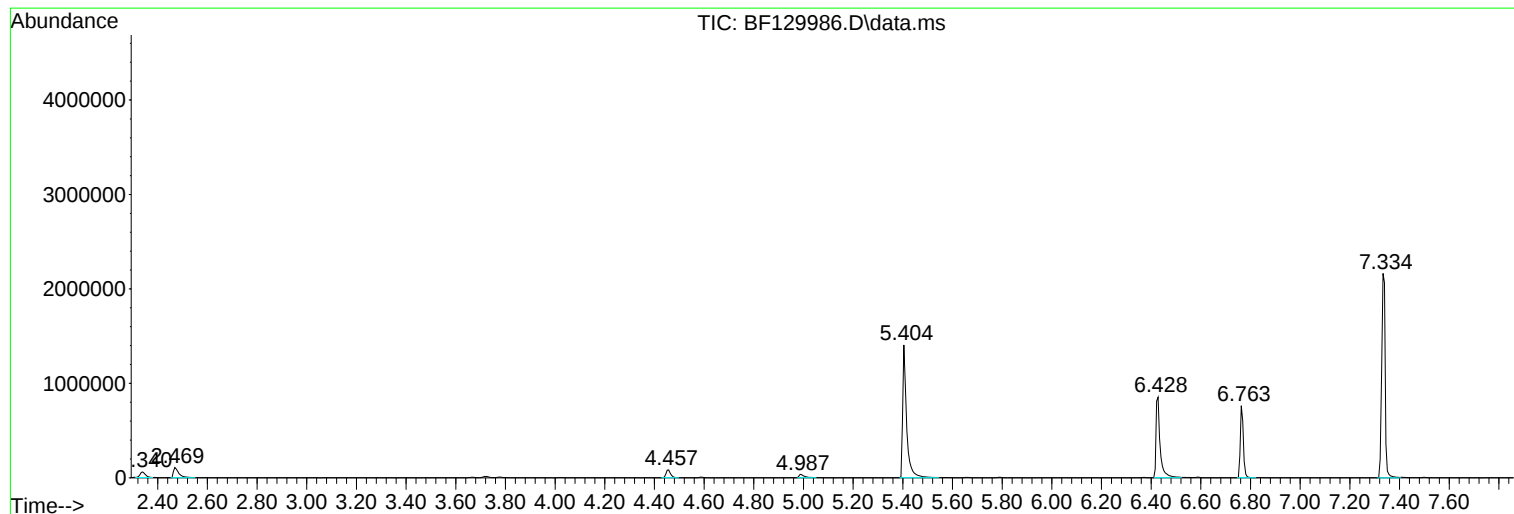

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
Data File : BF129986.D
Acq On : 24 Aug 2022 23:18
Operator : CG\JU
Sample : N4262-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-101I










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 unknown13.786 Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.786	2.35 ng	67010	Chrysene-d12	13.933

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Decene	140	C10H20	000872-05-9	49
2			Nonadecyl pentafluoropropionate	430	C22H39F5O2	1000351-88-8	49
3			Cyclopentane, 1,1,3-trimethyl-	112	C8H16	004516-69-2	41
4			Cyclodecane	140	C10H20	000293-96-9	38
5			Cyclohexanone, 3-ethyl-	126	C8H14O	022461-89-8	38

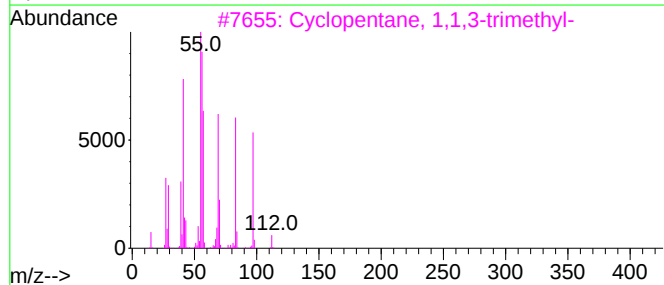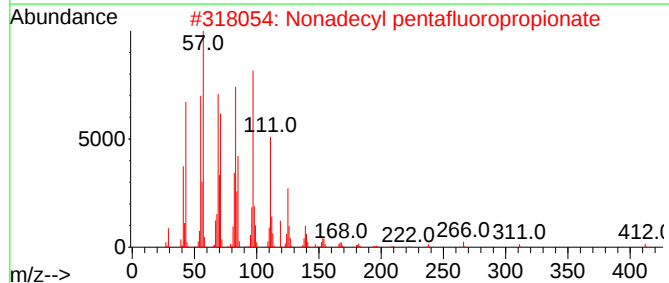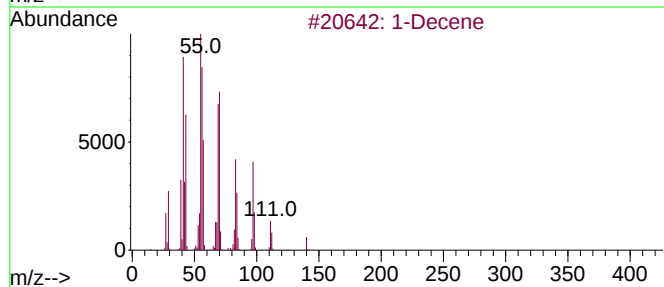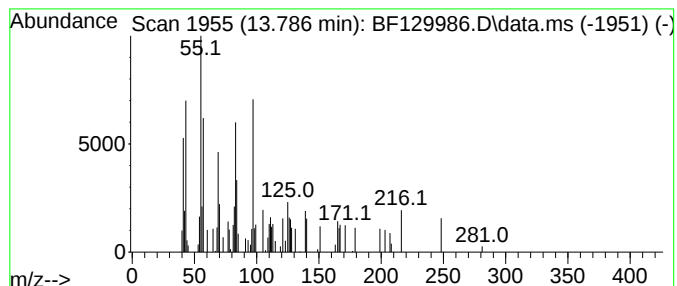

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
Data File : BF129986.D
Acq On : 24 Aug 2022 23:18
Operator : CG\JU
Sample : N4262-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-101I










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.022	8.92 ng	254042	Chrysene-d12	13.933

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	96
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	64
4			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15N02	299962-12-2	37
5			2-Phenyl-6-(trifluoromethyl)-1H-...	277	C15H10F3NO	1000387-59-3	25

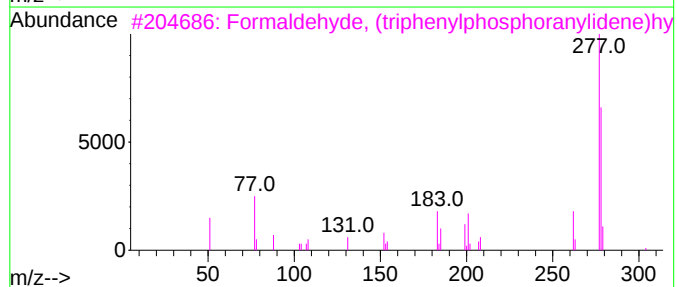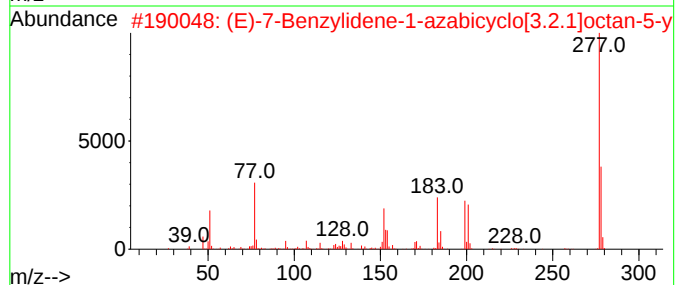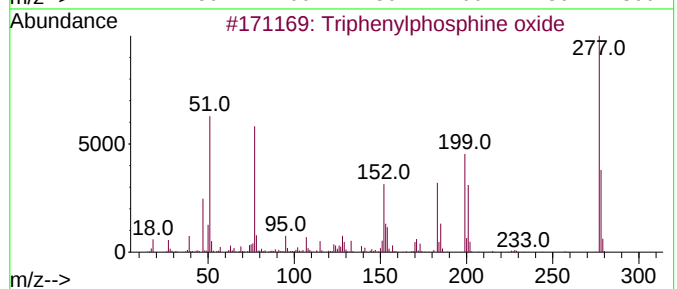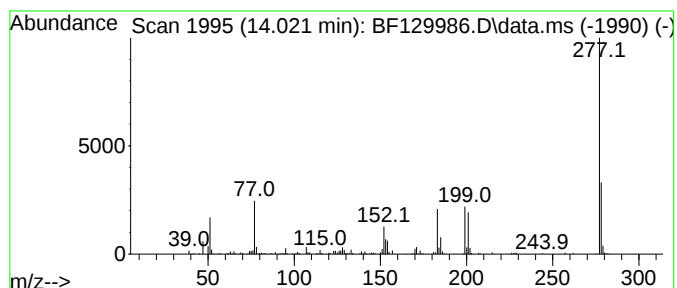

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
Data File : BF129986.D
Acq On : 24 Aug 2022 23:18
Operator : CG\JU
Sample : N4262-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-101I

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown13.786	13.786	2.4	ng	67010	5	13.933	569366	20.0
Triphenylphosph...	14.022	8.9	ng	254042	5	13.933	569366	20.0