


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
 Data File : BF129966.D
 Acq On : 24 Aug 2022 09:21
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 25 04:08:38 2022

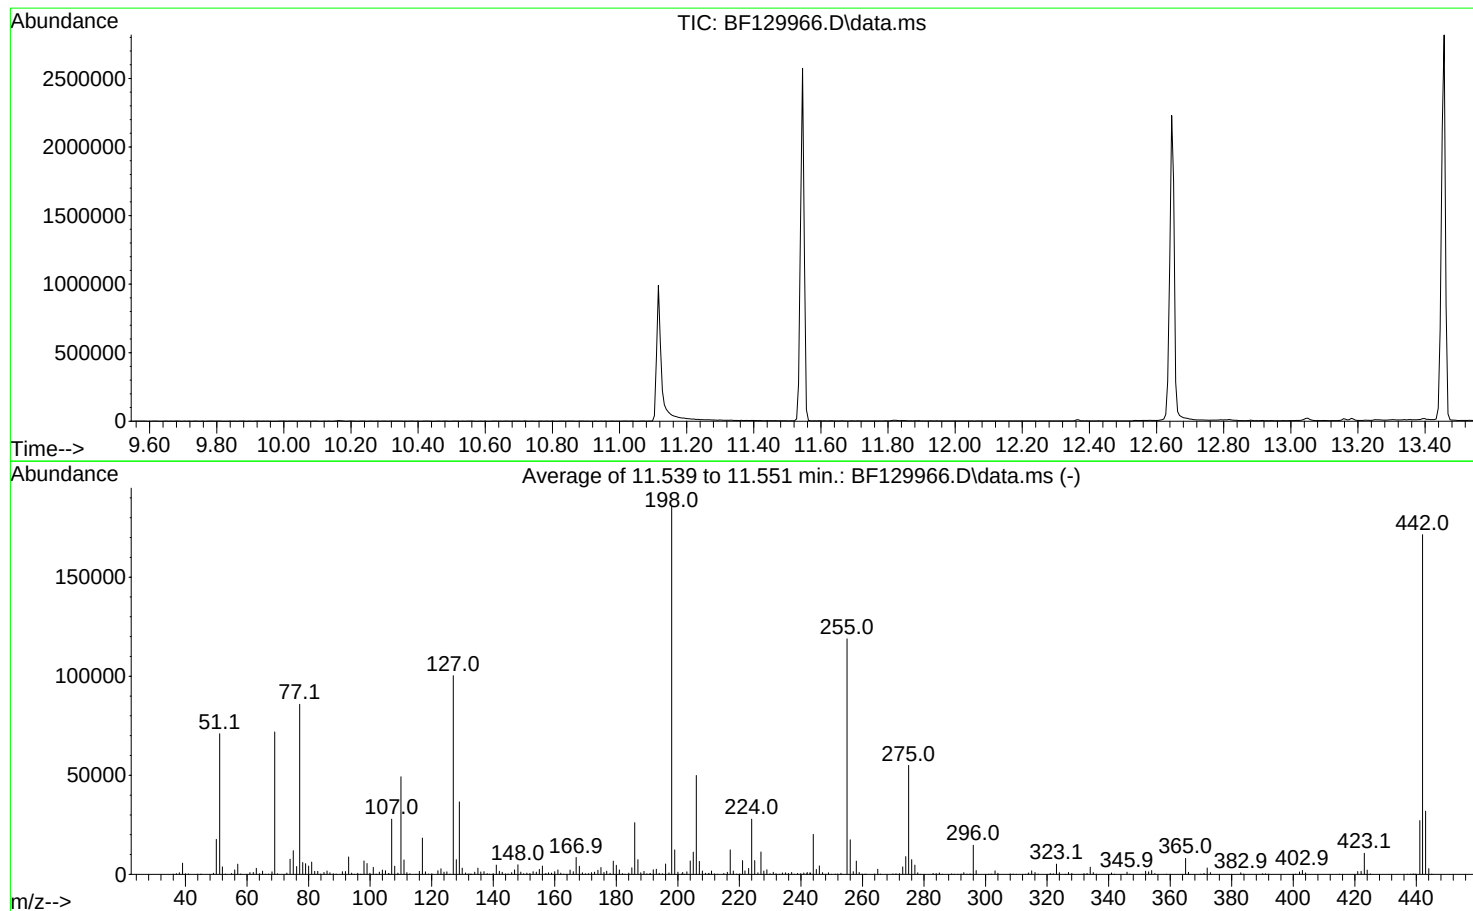




AutoFind: Scans 1573, 1574, 1575; Background Corrected with Scan 1568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.2	70989	PASS
68	69	0.00	2	1.8	1281	PASS
69	198	0.00	100	38.7	71885	PASS
70	69	0.00	2	0.4	300	PASS
127	198	10	80	54.0	100312	PASS
197	198	0.00	2	0.4	696	PASS
198	198	100	100	100.0	185675	PASS
199	198	5	9	6.6	12321	PASS
275	198	10	60	29.6	54971	PASS
365	198	1	100	4.4	8118	PASS
441	198	0.01	100	14.6	27163	PASS
442	442	50	100	100.0	171456	PASS
443	442	15	24	18.6	31900	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
Data File : BF129966.D
Acq On : 24 Aug 2022 09:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 25 07:45:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 04:08:38 2022
Response via : Initial Calibration

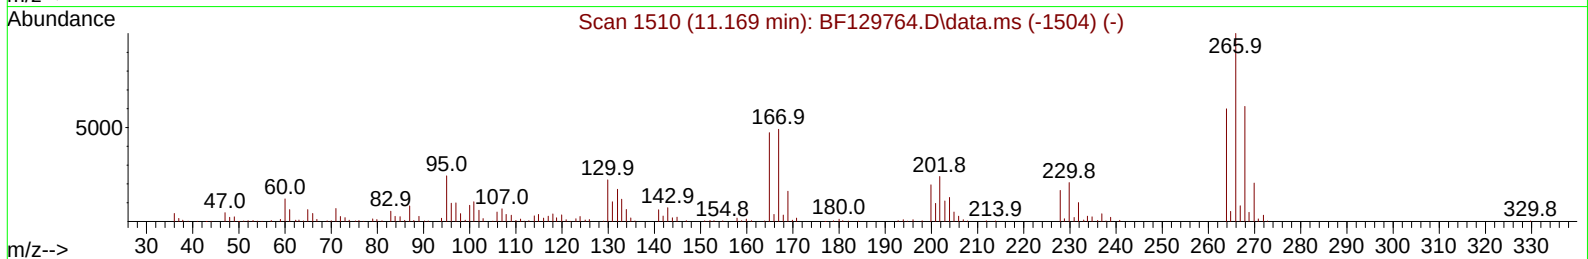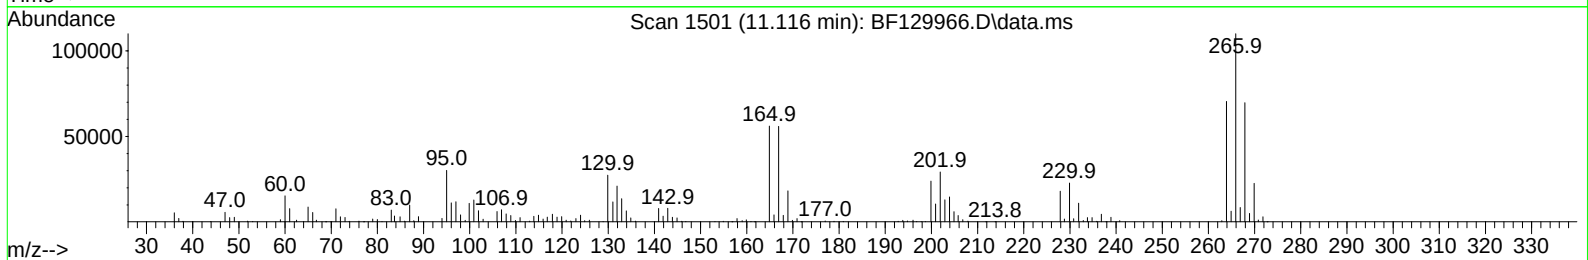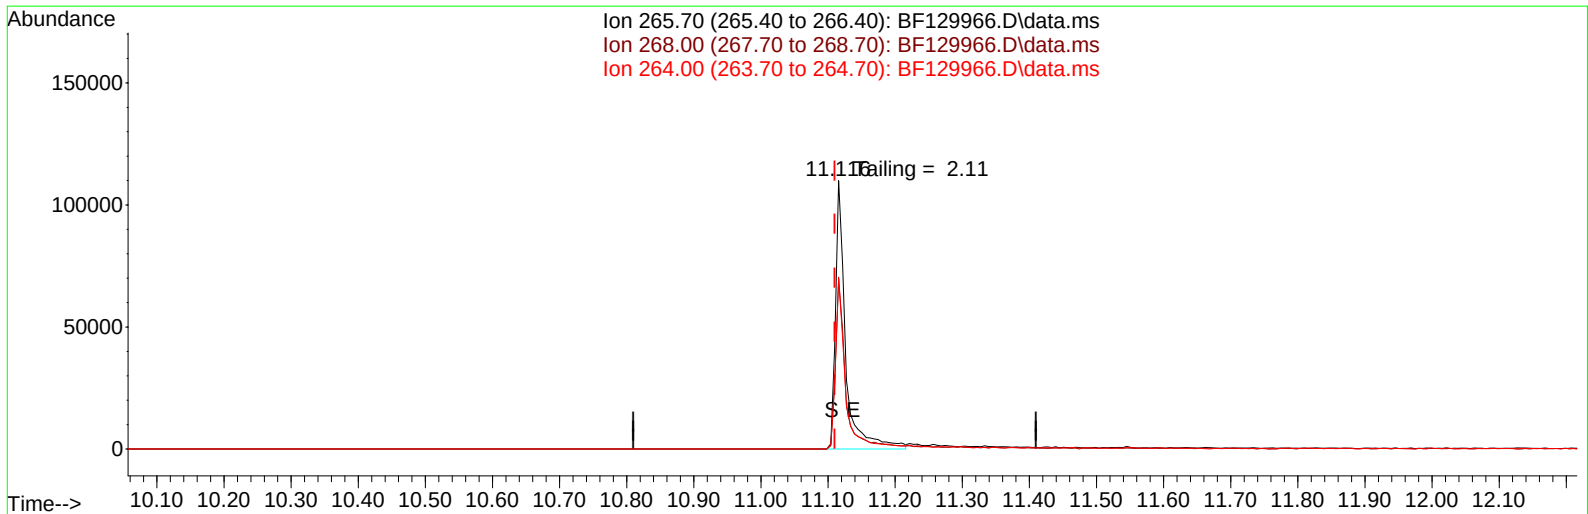

TIC: BF129966.D\data.ms

(70) Pentachlorophenol (C)

11.116min (+ 0.006) 102363.52 ng




response 116547

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	63.34
264.00	59.90	64.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
Data File : BF129966.D
Acq On : 24 Aug 2022 09:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 25 07:45:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 25 04:08:38 2022
Response via : Initial Calibration

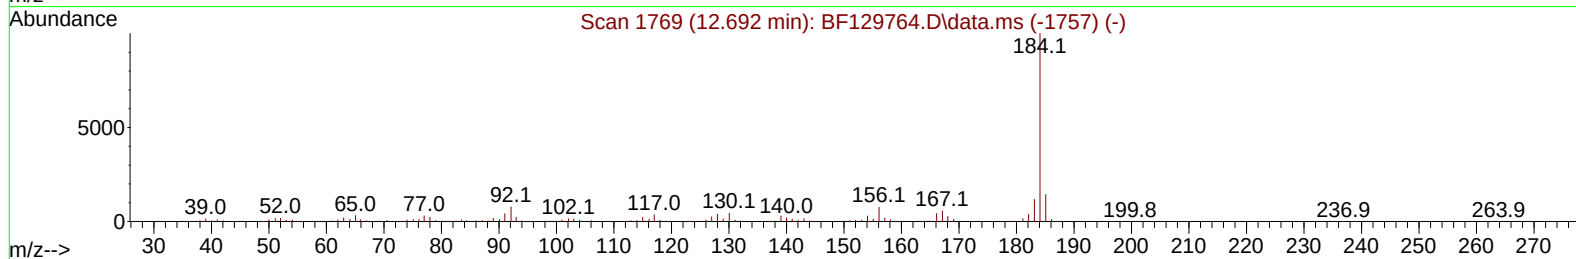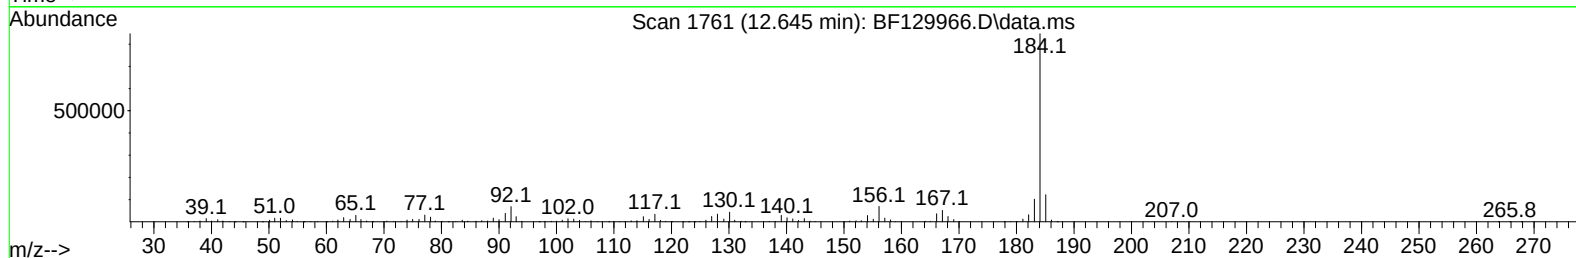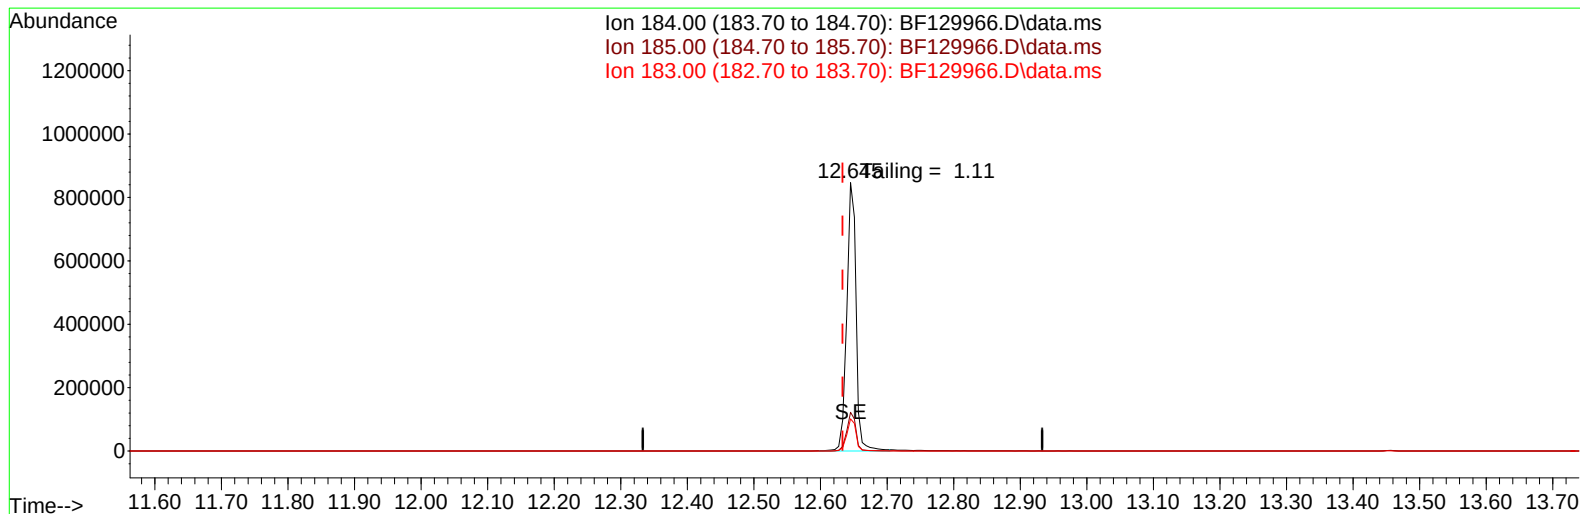

TIC: BF129966.D\data.ms

(77) Benzidine

12.645min (+ 0.012) 255976.21 ng

response 833564

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.43
183.00	11.80	12.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/24/2022	BNA_F	<u>BF129966.D</u>
Compound Name	Response	Retention Time
DDT	437847	13.457
DDD	5249	13.157
DDE	1354	12.822
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6603	444450	1.49

Instrument :
BNA_F
ClientSampleId :
DFTPP