


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
Data File : BF129973.D
Acq On : 24 Aug 2022 15:32
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 25 04:08:38 2022

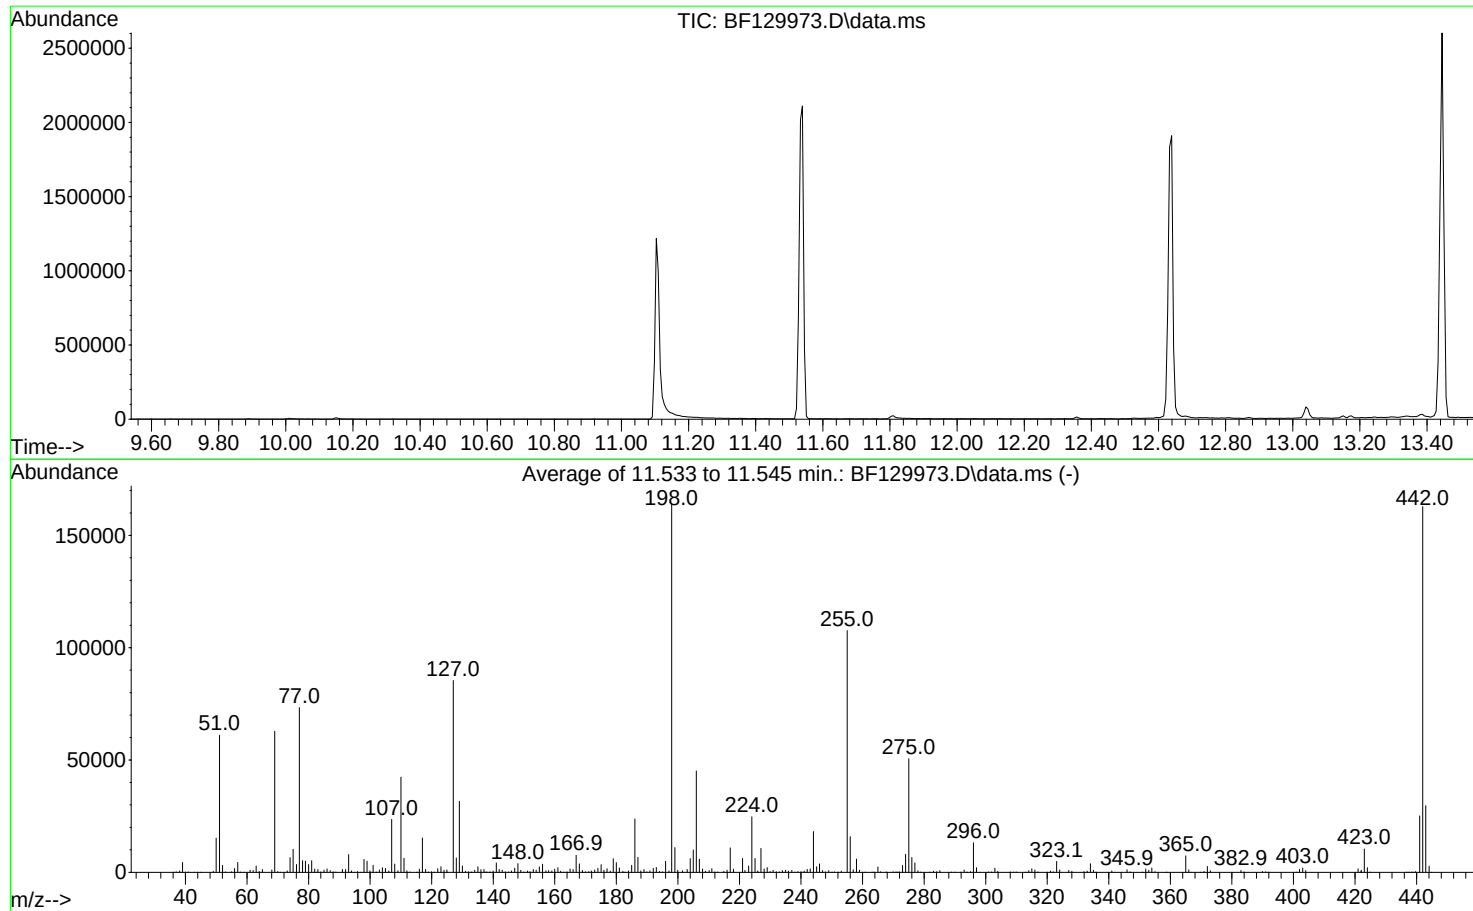




AutoFind: Scans 1572, 1573, 1574; Background Corrected with Scan 1566

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	61024	PASS
68	69	0.00	2	1.6	1023	PASS
69	198	0.00	100	38.4	62835	PASS
70	69	0.00	2	0.5	314	PASS
127	198	10	80	52.1	85411	PASS
197	198	0.00	2	0.4	600	PASS
198	198	100	100	100.0	163800	PASS
199	198	5	9	6.7	11000	PASS
275	198	10	60	30.9	50547	PASS
365	198	1	100	4.5	7338	PASS
441	198	0.01	100	15.3	25117	PASS
442	442	50	100	100.0	162845	PASS
443	442	15	24	18.2	29643	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\
 Data File : BF129973.D
 Acq On : 24 Aug 2022 15:32
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 25 07:50:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Aug 25 04:08:38 2022
 Response via : Initial Calibration

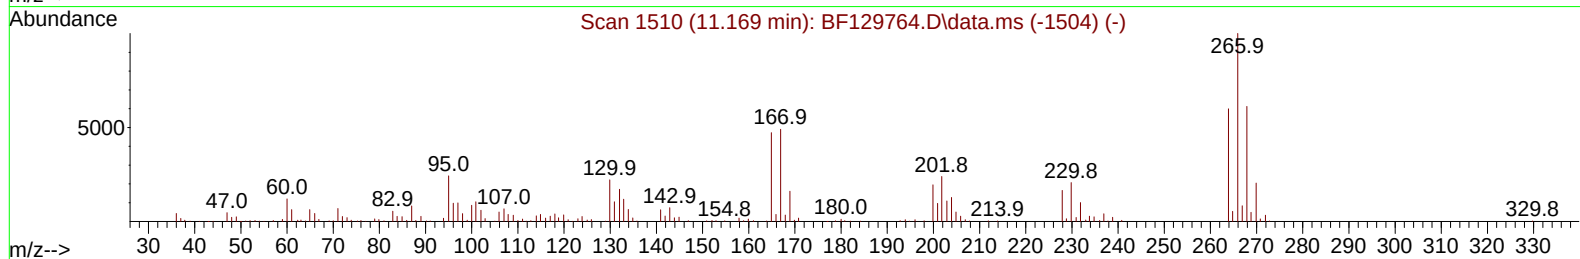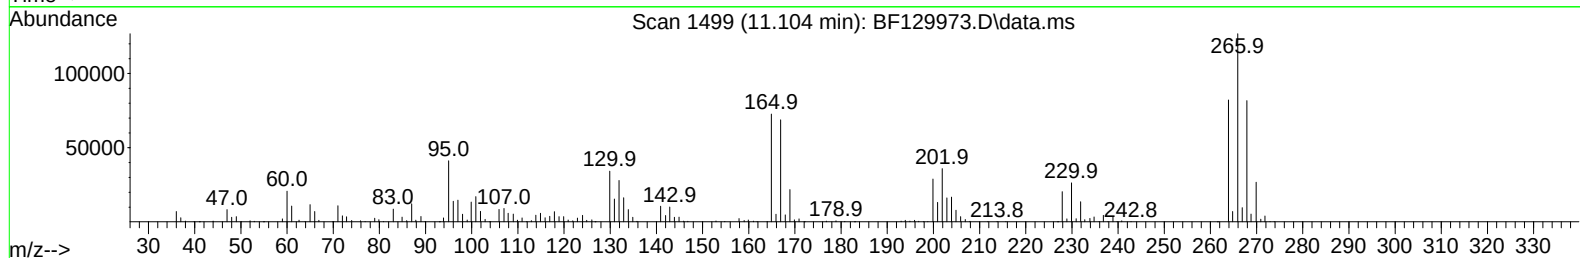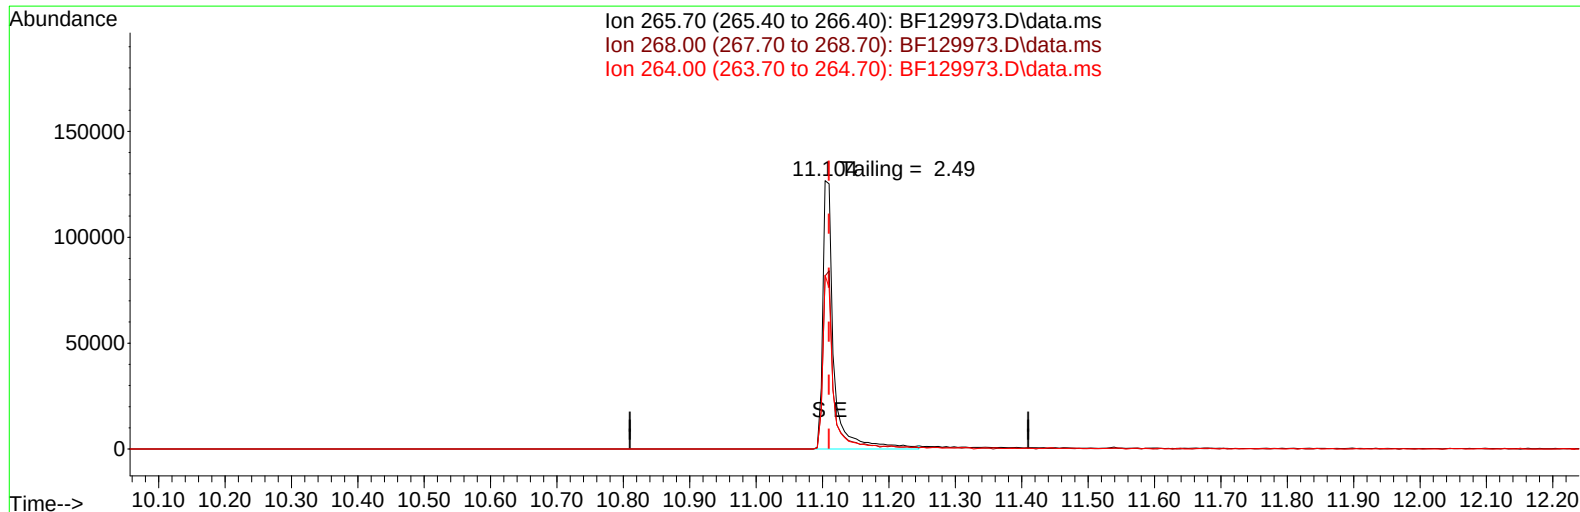

TIC: BF129973.D\data.ms

(70) Pentachlorophenol (C)

11.104min (-0.006) 181199.26 ng




response 146628

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.47
264.00	59.90	64.84
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082422\  
Data File : BF129973.D  
Acq On    : 24 Aug 2022  15:32  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 25 07:50:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Thu Aug 25 04:08:38 2022
Response via : Initial Calibration

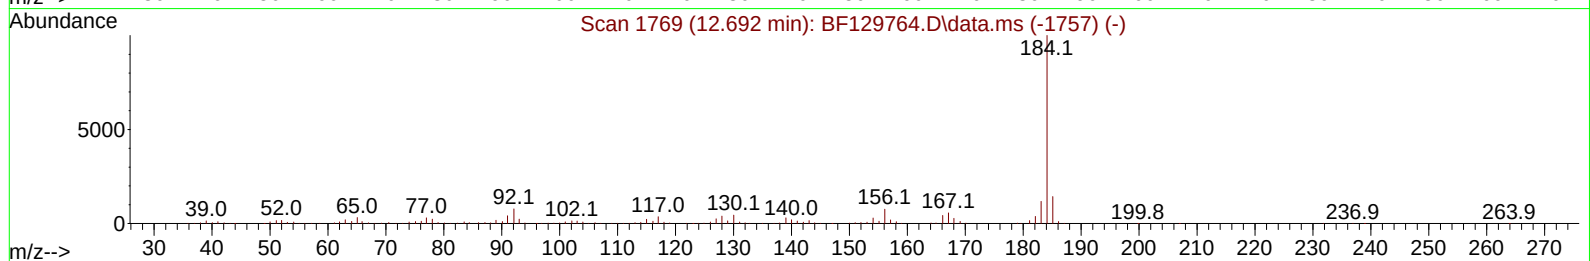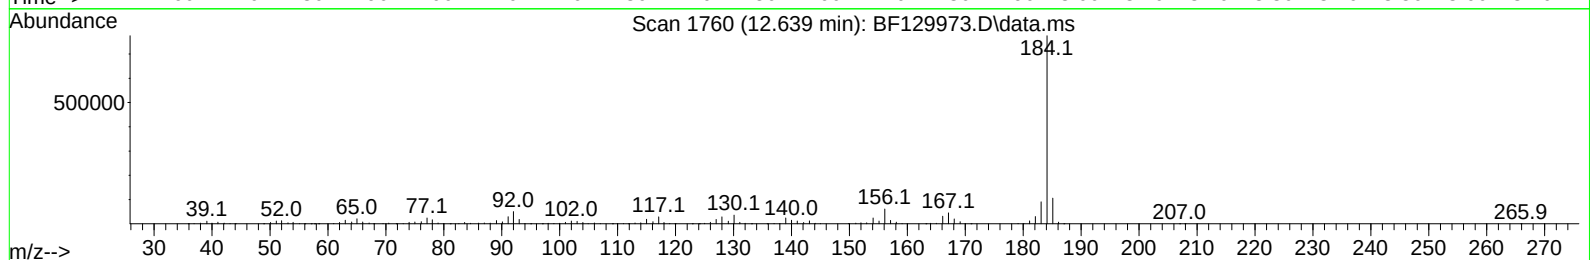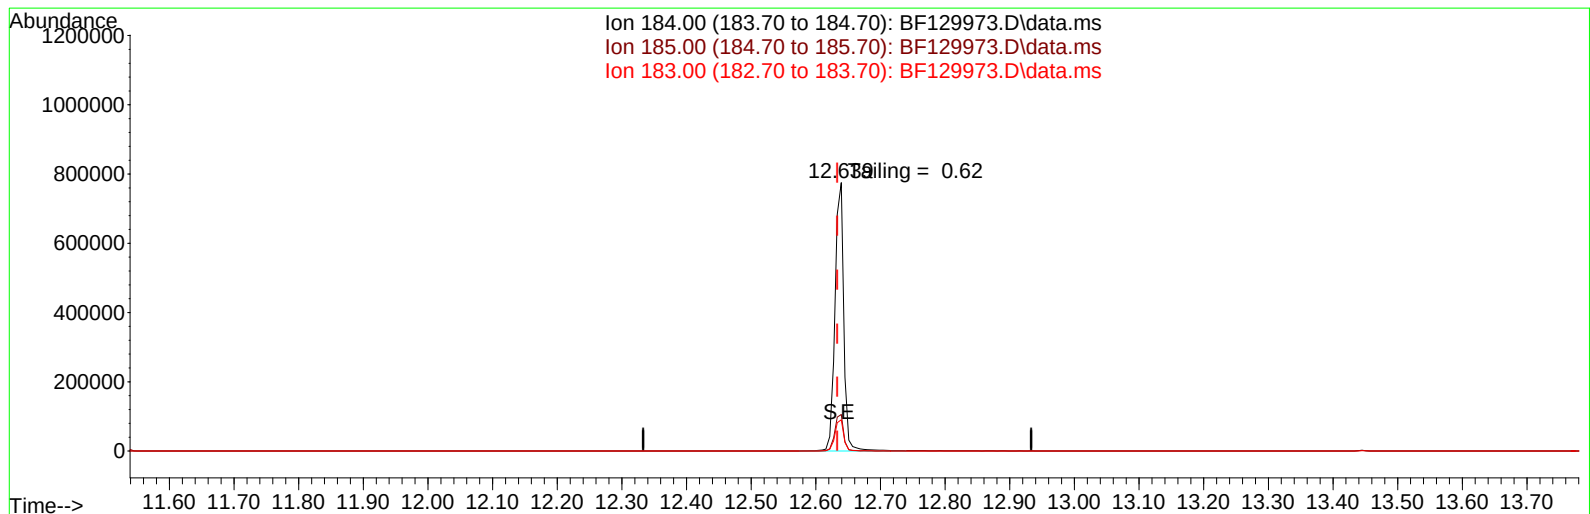

TIC: BF129973.D\data.ms

(77) Benzidine

12.639min (+ 0.006) 132098.78 ng

response 734654

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.62
183.00	11.80	11.66
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/24/2022	BNA_F	<u>BF129973.D</u>
Compound Name	Response	Retention Time
DDT	393757	13.445
DDD	4724	13.151
DDE	1245	12.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5969	399726	1.49

Instrument :
BNA_F
ClientSampleId :
DFTPP