


Data Path : Z:\HPCHEM1\BNA_F\Data\BF082516\
 Data File : BF089908.D
 Acq On : 25 Aug 2016 11:01
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 19 14:02:57 2016

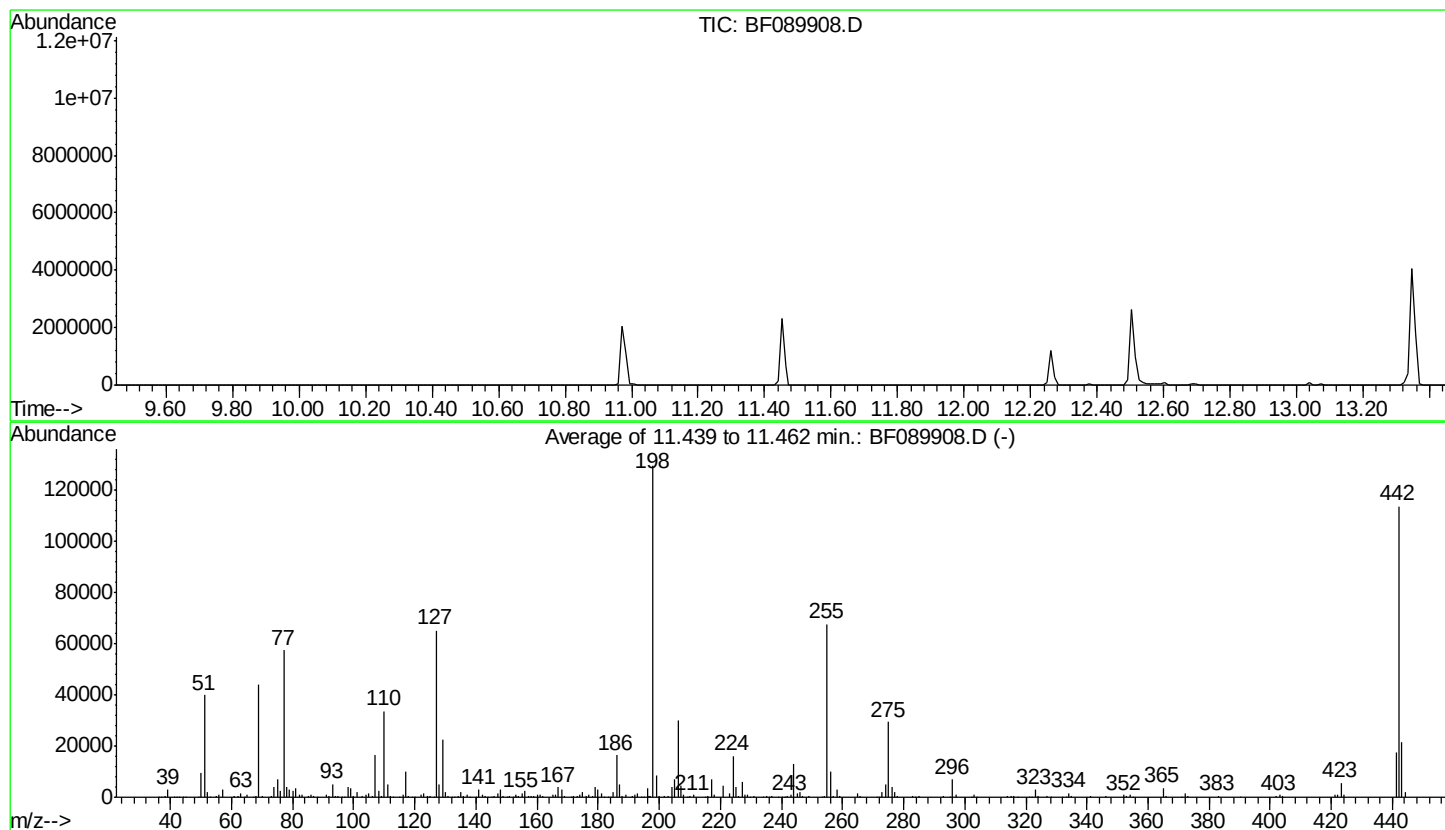

AutoFind: Scans 862, 863, 864; Background Corrected with Scan 859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.8	39768	PASS
68	69	0.00	2	1.3	585	PASS
69	198	0.00	100	34.0	43933	PASS
70	69	0.00	2	0.7	325	PASS
127	198	10	80	50.2	64980	PASS
197	198	0.00	2	0.5	590	PASS
198	198	100	100	100.0	129314	PASS
199	198	5	9	6.6	8593	PASS
275	198	10	60	22.7	29409	PASS
365	198	1	100	2.8	3596	PASS
441	442	0.01	24	15.4	17421	PASS
442	198	50	100	87.6	113341	PASS
443	442	15	24	19.1	21645	PASS