


Data Path : Z:\HPCHEM1\BNA F\Data\BF082517\  
 Data File : BF098031.D  
 Acq On : 25 Aug 2017 15:31  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF081517.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Aug 21 15:59:04 2017

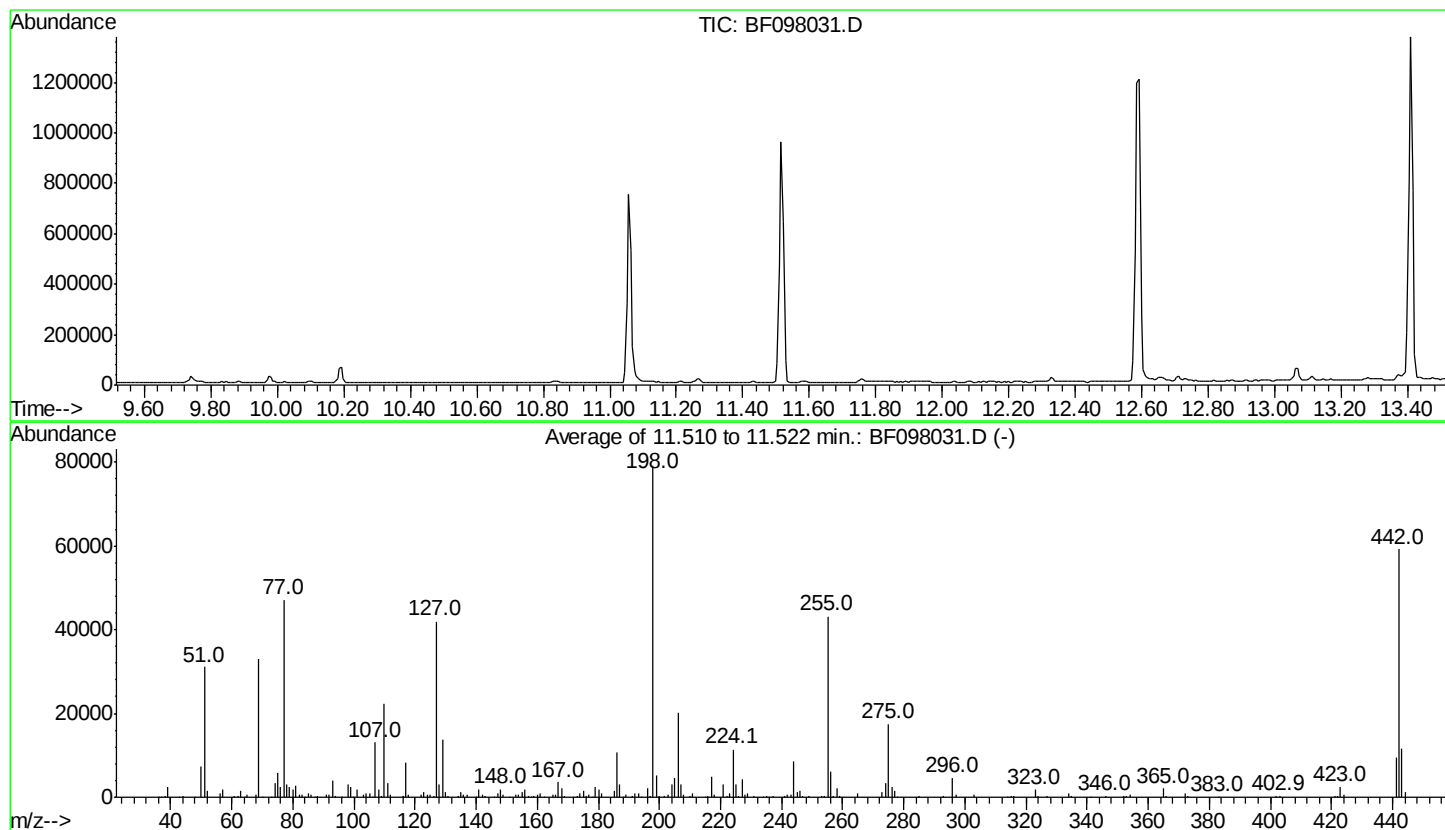

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1597

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 39.2         | 31033      | PASS                |
| 68             | 69              | 0.00            | 2               | 2.0          | 650        | PASS                |
| 69             | 198             | 0.00            | 100             | 41.7         | 32994      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.3          | 108        | PASS                |
| 127            | 198             | 10              | 80              | 52.9         | 41869      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.5          | 385        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 79144      | PASS                |
| 199            | 198             | 5               | 9               | 6.6          | 5259       | PASS                |
| 275            | 198             | 10              | 60              | 22.1         | 17457      | PASS                |
| 365            | 198             | 1               | 100             | 2.6          | 2078       | PASS                |
| 441            | 442             | 0.01            | 24              | 16.1         | 9538       | PASS                |
| 442            | 198             | 50              | 100             | 74.7         | 59144      | PASS                |
| 443            | 442             | 15              | 24              | 19.9         | 11756      | PASS                |