

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082521\
 Data File : BF125201.D
 Acq On : 25 Aug 2021 10:20
 Operator : JU/CG
 Sample : PB138680BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB138680BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125201.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.257	23	29	35	rVB	88464	125161	2.81%	0.444%
2	5.540	582	587	590	rBV	4178472	4102962	92.20%	14.543%
3	6.540	751	757	760	rBV	3796219	3964167	89.08%	14.051%
4	6.916	817	821	824	rBV	1054175	855439	19.22%	3.032%
5	7.475	911	916	919	rBV	2740327	2634455	59.20%	9.338%
6	8.198	1035	1039	1042	rBV	1240022	1081558	24.30%	3.834%
7	9.269	1216	1221	1225	rBV	4584834	4449970	100.00%	15.773%
8	9.951	1333	1337	1345	rBV	1397579	1164918	26.18%	4.129%
9	10.739	1467	1471	1474	rBV	3244678	2817761	63.32%	9.987%
10	11.439	1586	1590	1597	rBV	1246928	1107390	24.89%	3.925%
11	13.027	1855	1860	1863	rBV	4570754	4192875	94.22%	14.862%
12	14.080	2035	2039	2043	rBV	997325	871353	19.58%	3.088%
13	15.574	2288	2293	2301	rVB2	654275	844917	18.99%	2.995%




Sum of corrected areas: 28212926

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082521\
Data File : BF125201.D
Acq On : 25 Aug 2021 10:20
Operator : JU/CG
Sample : PB138680BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138680BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

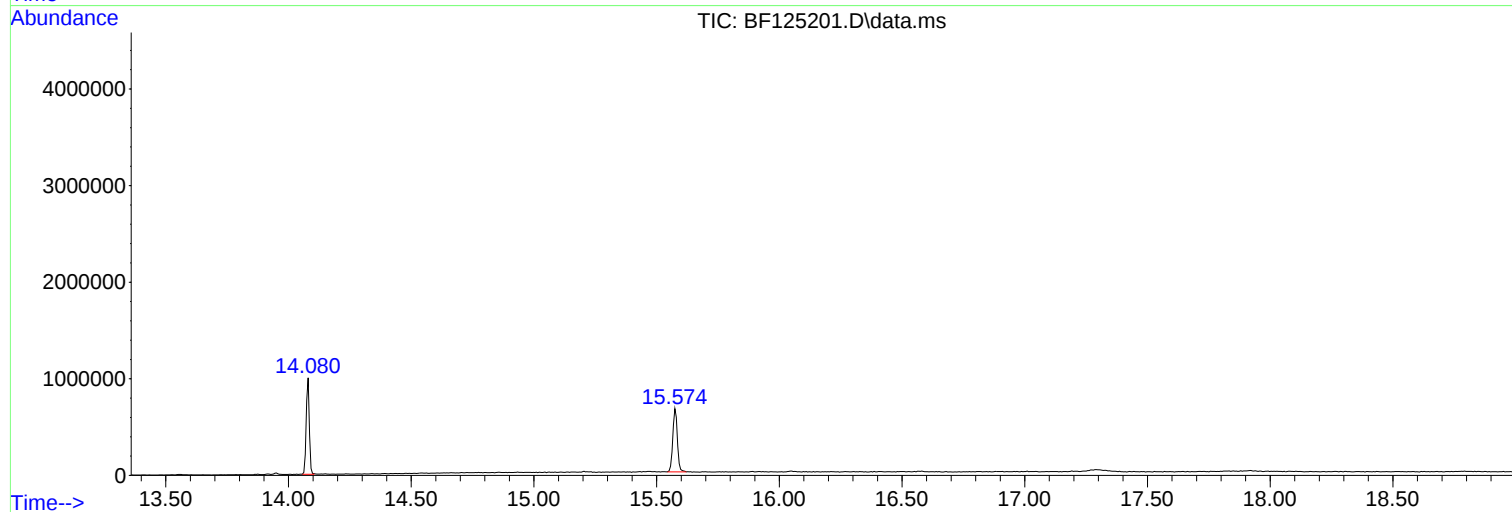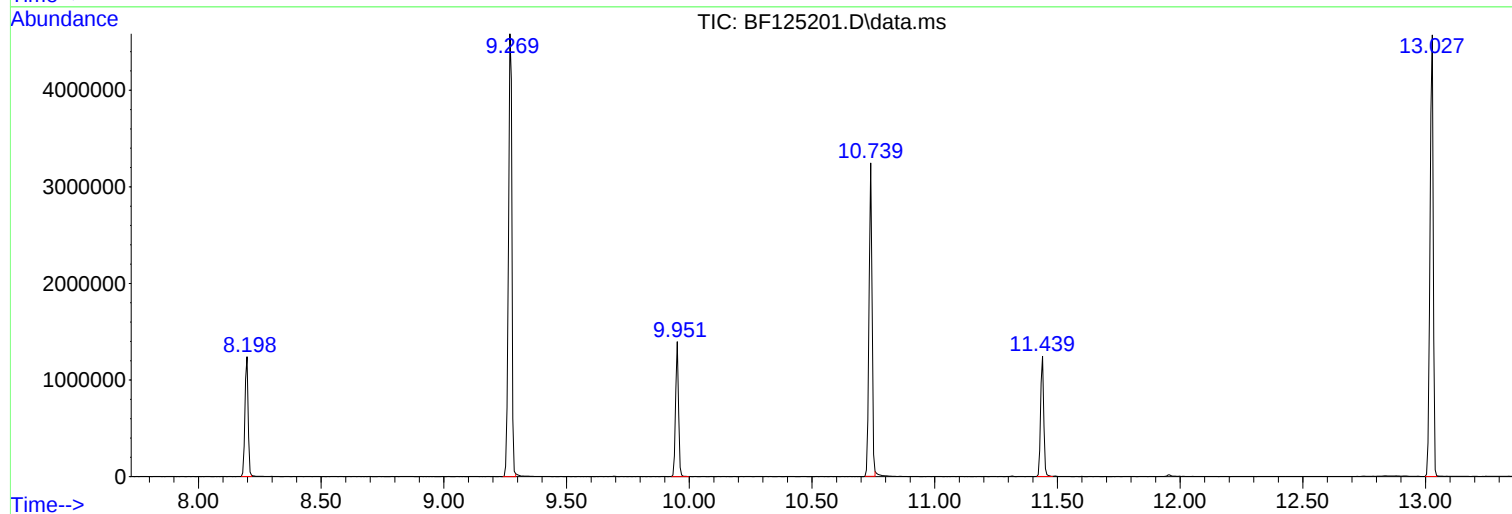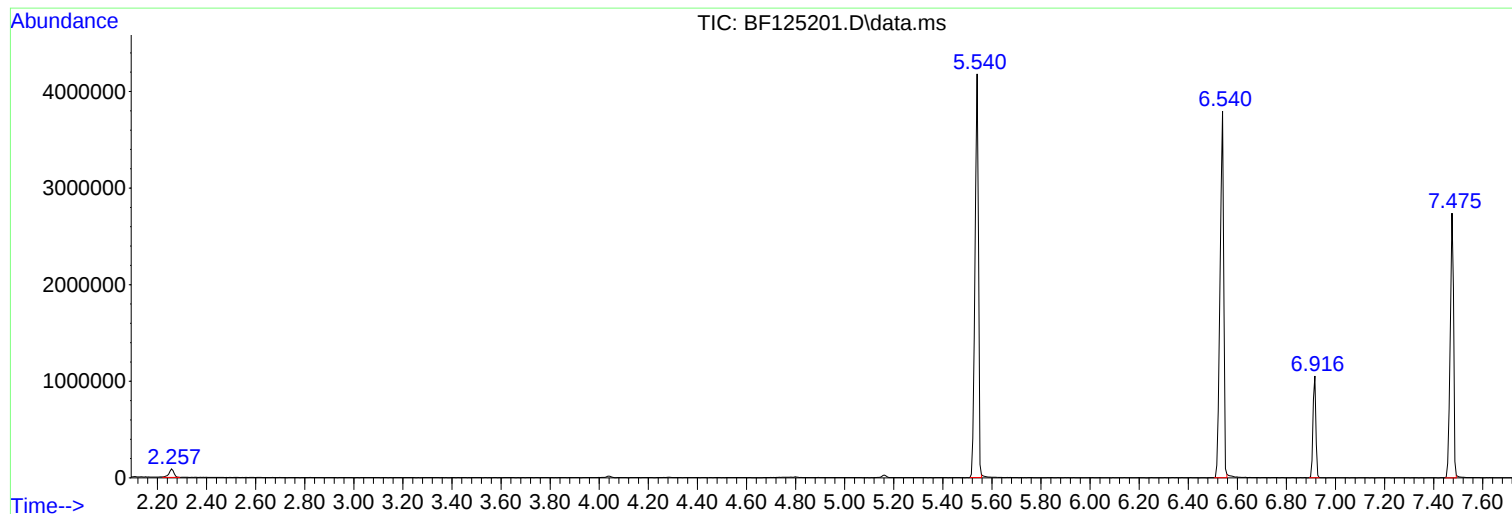

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082521\
Data File : BF125201.D
Acq On : 25 Aug 2021 10:20
Operator : JU/CG
Sample : PB138680BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138680BL









Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.257	2.93 ng	125161	1,4-Dichlorobenzene-d4	6.916

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	43
3			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	43
4			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	38
5			3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	17

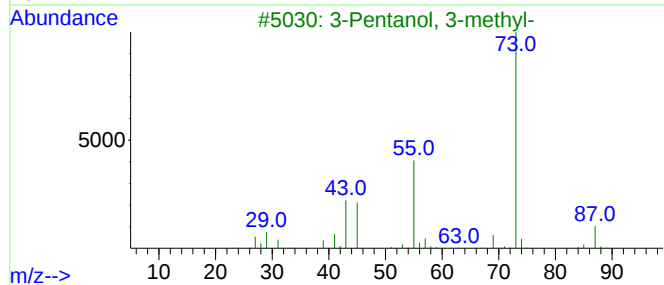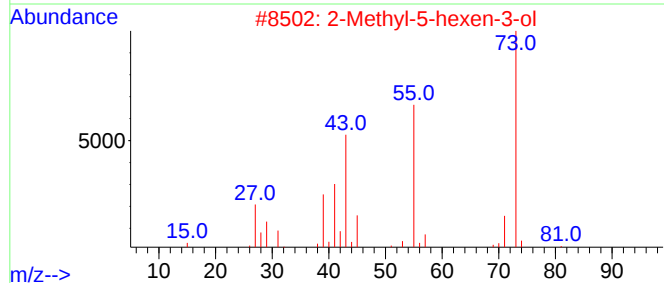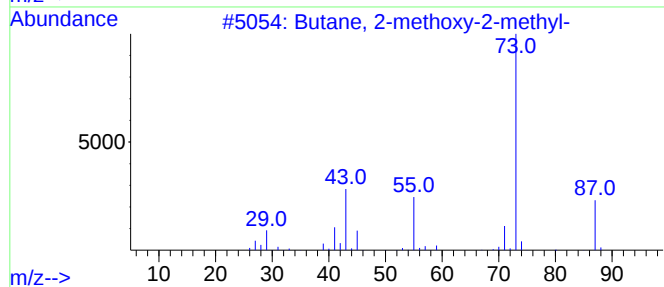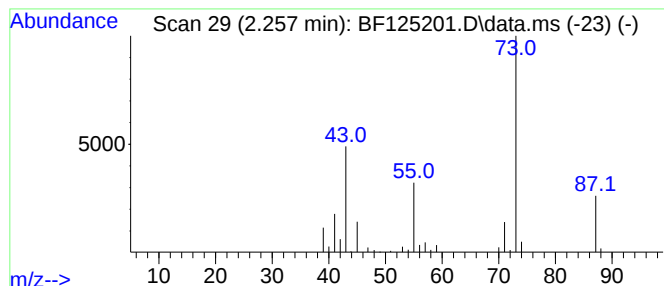

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082521\
Data File : BF125201.D
Acq On : 25 Aug 2021 10:20
Operator : JU/CG
Sample : PB138680BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138680BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.257	2.9	ng	125161	1	6.916	855439	20.0