
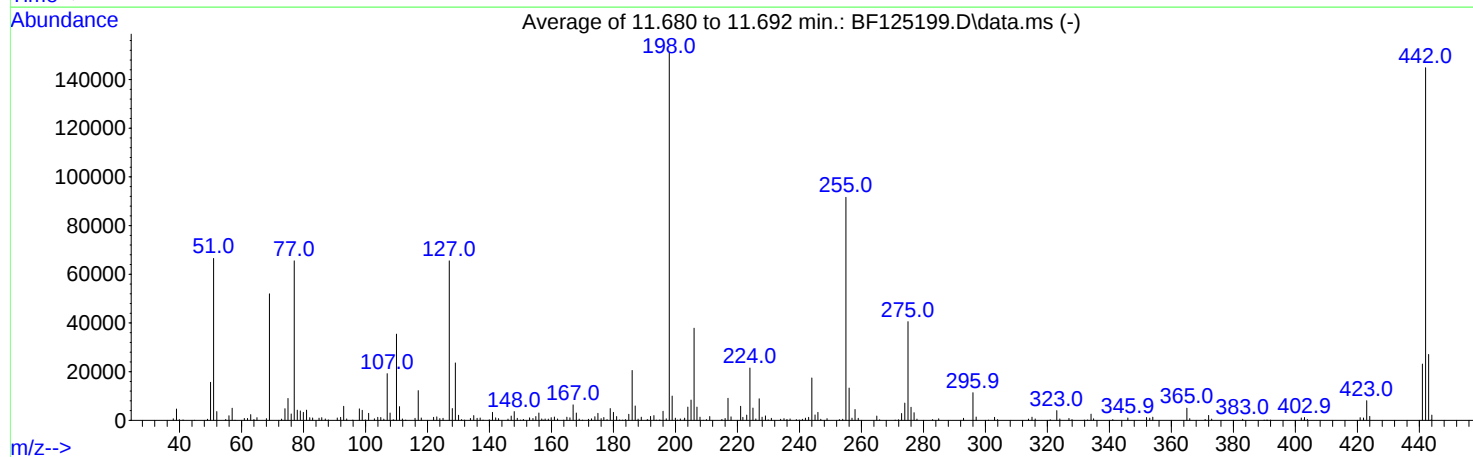


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082521\
 Data File : BF125199.D
 Acq On : 25 Aug 2021 9:17
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 24 12:39:21 2021

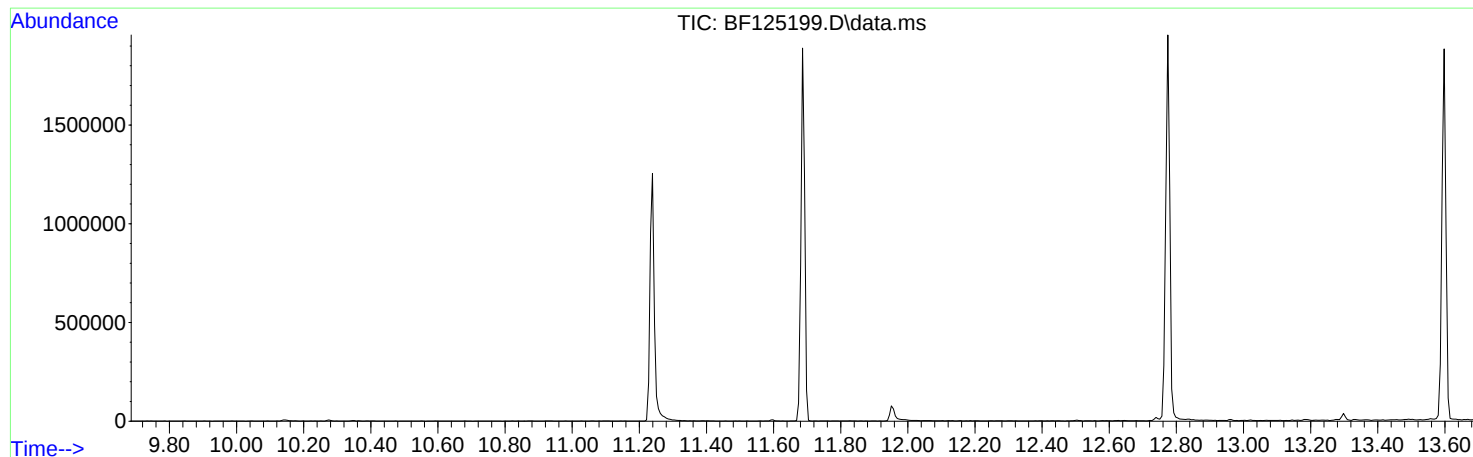




AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.0	66520	PASS
68	69	0.00	2	1.4	749	PASS
69	198	0.00	100	34.4	52005	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.4	65557	PASS
197	198	0.00	2	0.4	654	PASS
198	198	100	100	100.0	151099	PASS
199	198	5	9	6.6	10002	PASS
275	198	10	60	26.8	40536	PASS
365	198	1	100	3.3	5017	PASS
441	198	0.01	100	15.3	23130	PASS
442	442	50	100	100.0	144885	PASS
443	442	15	24	18.7	27102	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082521\
 Data File : BF125199.D
 Acq On : 25 Aug 2021 9:17
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 25 10:56:40 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 12:39:21 2021
 Response via : Initial Calibration

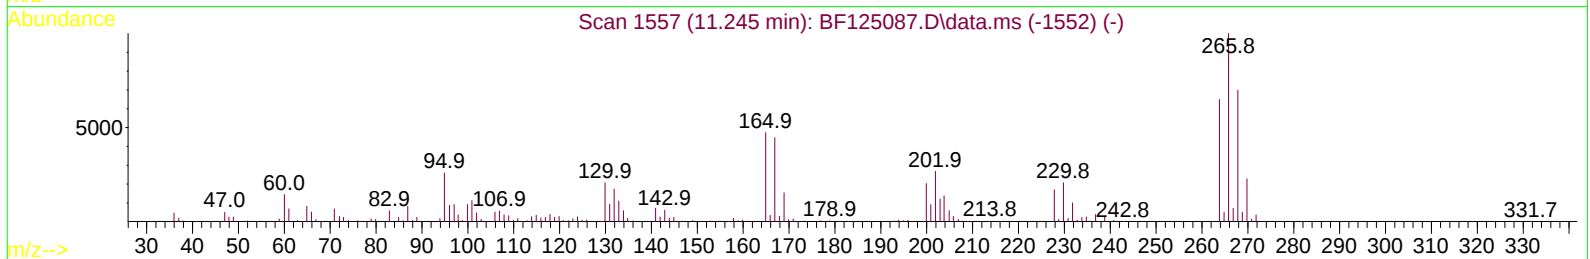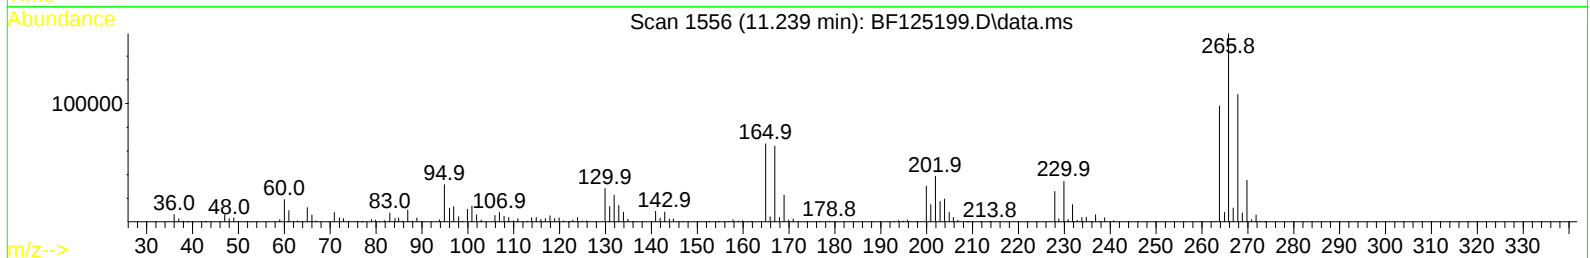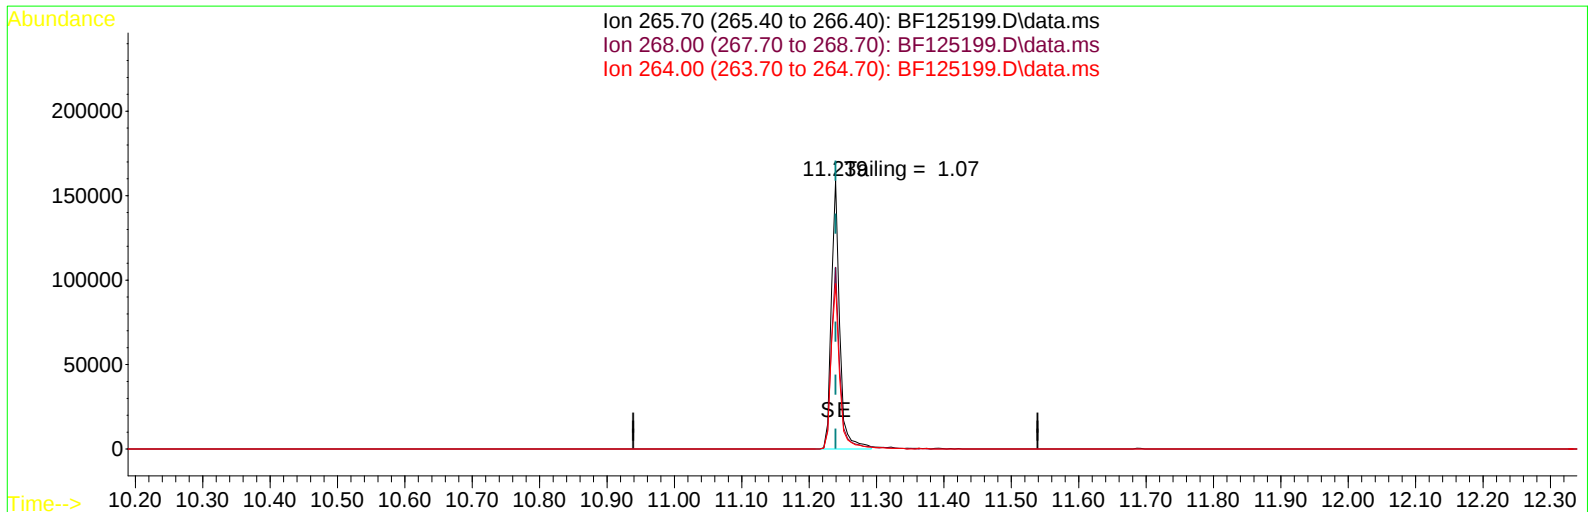

TIC: BF125199.D\data.ms

(70) Pentachlorophenol (C)

11.239min (+ 0.000) 37021.81 ng




response 140196

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	67.73
264.00	69.90	61.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082521\
Data File : BF125199.D
Acq On : 25 Aug 2021 9:17
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 25 10:56:40 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 12:39:21 2021
Response via : Initial Calibration

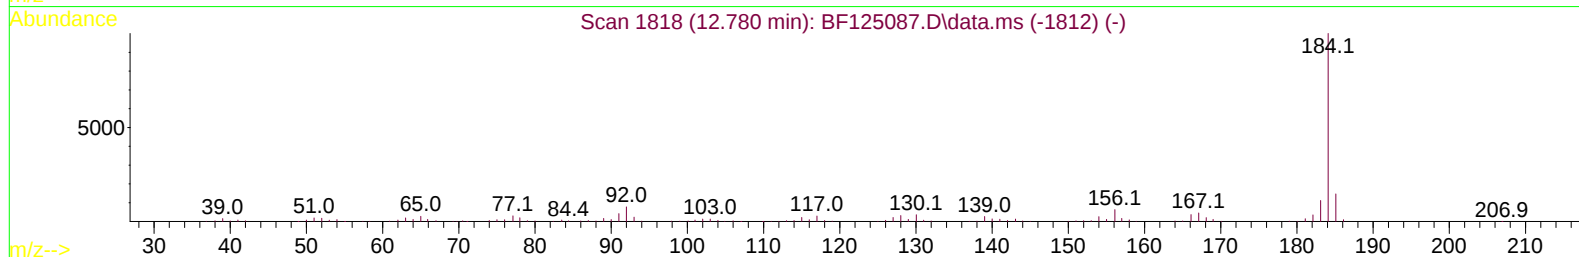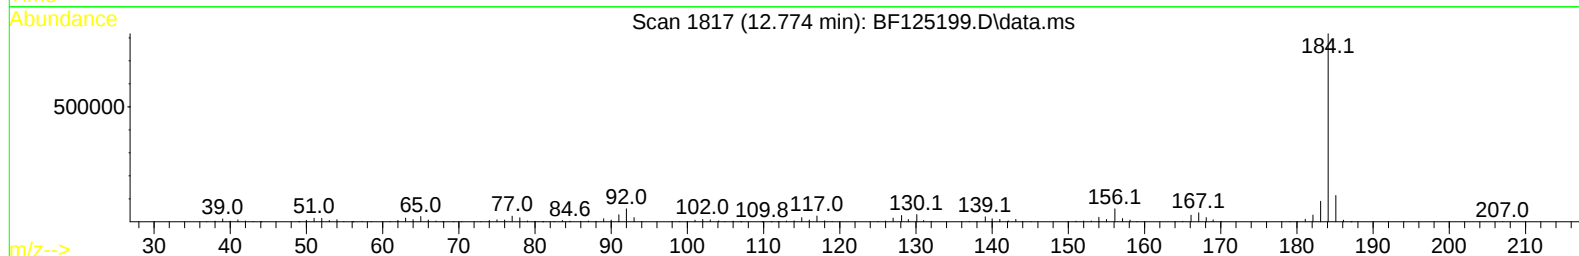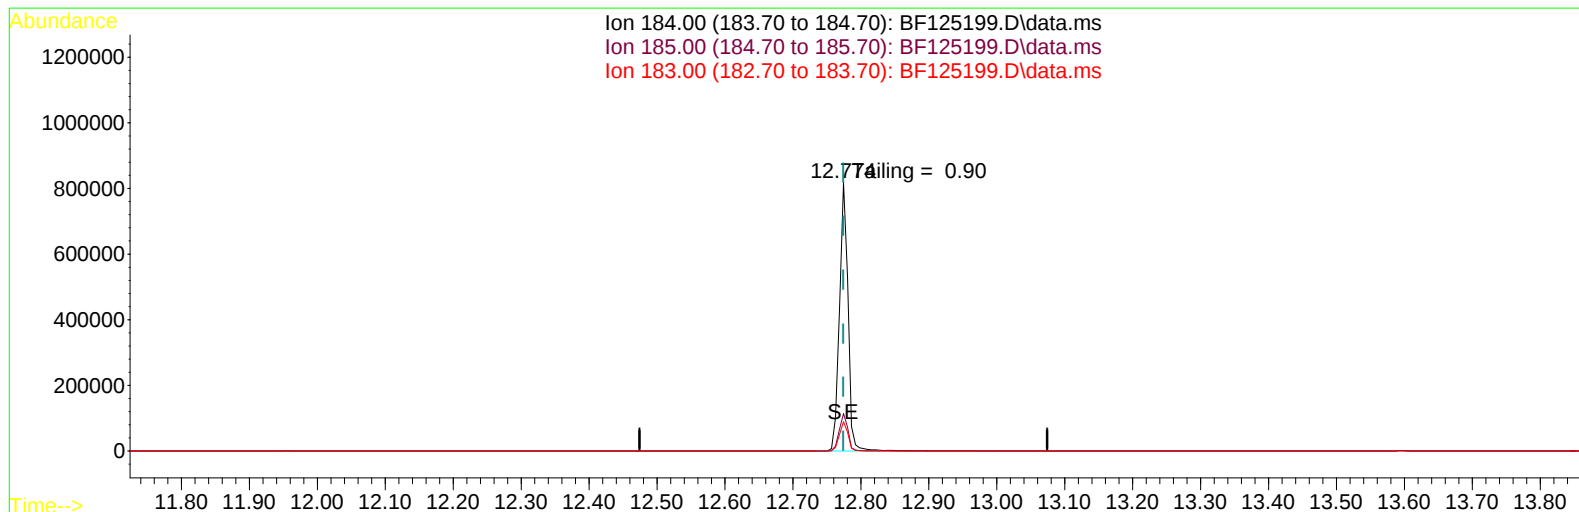

TIC: BF125199.D\data.ms

(77) Benzidine

12.774min (+ 0.000) 0.00 ng

response 714403

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.96
183.00	10.10	10.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/25/2021	BNA_F	<u>BF125199.D</u>
Compound Name	Response	Retention Time
DDT	321389	13.59
DDD	7599	13.29
DDE	826	12.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8425	329814	2.55

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP