

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082615\
 Data File : BF081217.D
 Acq On : 26 Aug 2015 17:41
 Operator : UM/IZ
 Sample : PB85190BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB85190BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.851	183	185	190	rBB	14141	24146	1.55%	0.183%
2	4.628	249	253	263	rBV	582827	1040464	66.91%	7.879%
3	5.086	290	293	295	rBV	1344248	1377108	88.56%	10.428%
4	5.509	328	330	332	rBV	28287	26731	1.72%	0.202%
5	6.171	385	388	390	rBV	1430551	1554916	100.00%	11.774%
6	6.286	395	398	400	rBV	1160591	1435682	92.33%	10.871%
7	6.514	416	418	420	rBV	366298	299537	19.26%	2.268%
8	6.674	429	432	434	rBV	955762	1068867	68.74%	8.094%
9	7.086	465	468	470	rBV	930395	885512	56.95%	6.705%
10	7.806	528	531	533	rBV	264892	364292	23.43%	2.759%
11	8.880	622	625	627	rBV	1526821	1431802	92.08%	10.842%
12	9.543	680	683	685	rBV	462515	406866	26.17%	3.081%
13	10.320	749	751	754	rBV2	587356	836645	53.81%	6.335%
14	11.006	809	811	814	rBV	334001	396210	25.48%	3.000%
15	12.595	947	950	953	rBV	1300831	1366024	87.85%	10.344%
16	13.624	1037	1040	1042	rBV	445667	397791	25.58%	3.012%
17	14.949	1154	1156	1159	rBV	286120	293441	18.87%	2.222%




Sum of corrected areas: 13206034

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082615\
Data File : BF081217.D
Acq On : 26 Aug 2015 17:41
Operator : UM/IZ
Sample : PB85190BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB85190BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

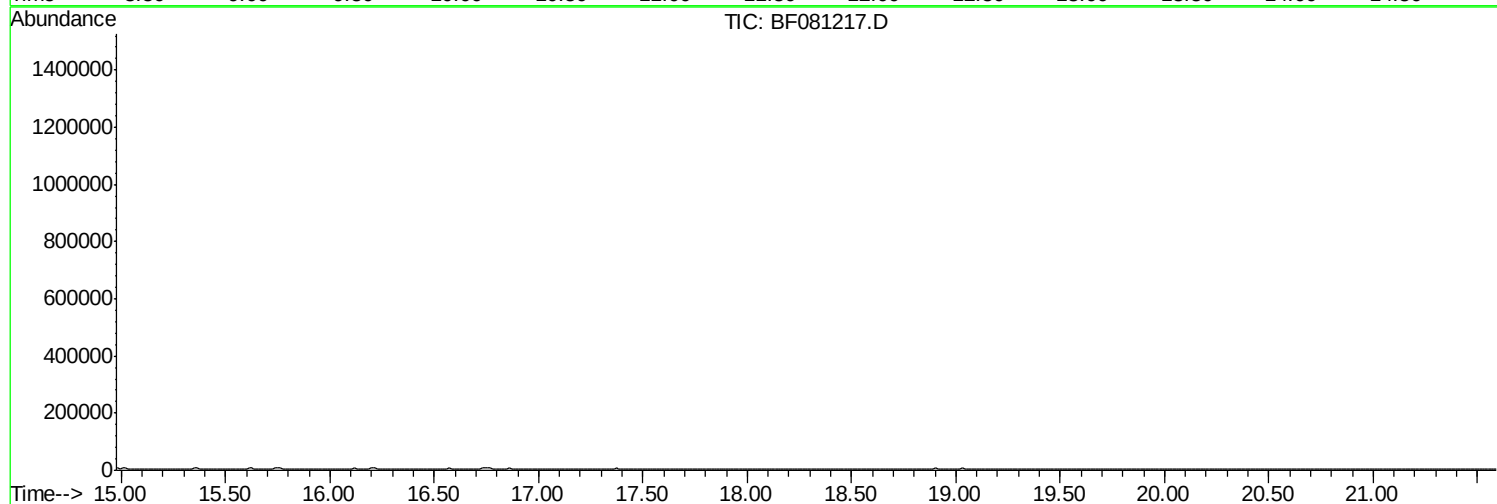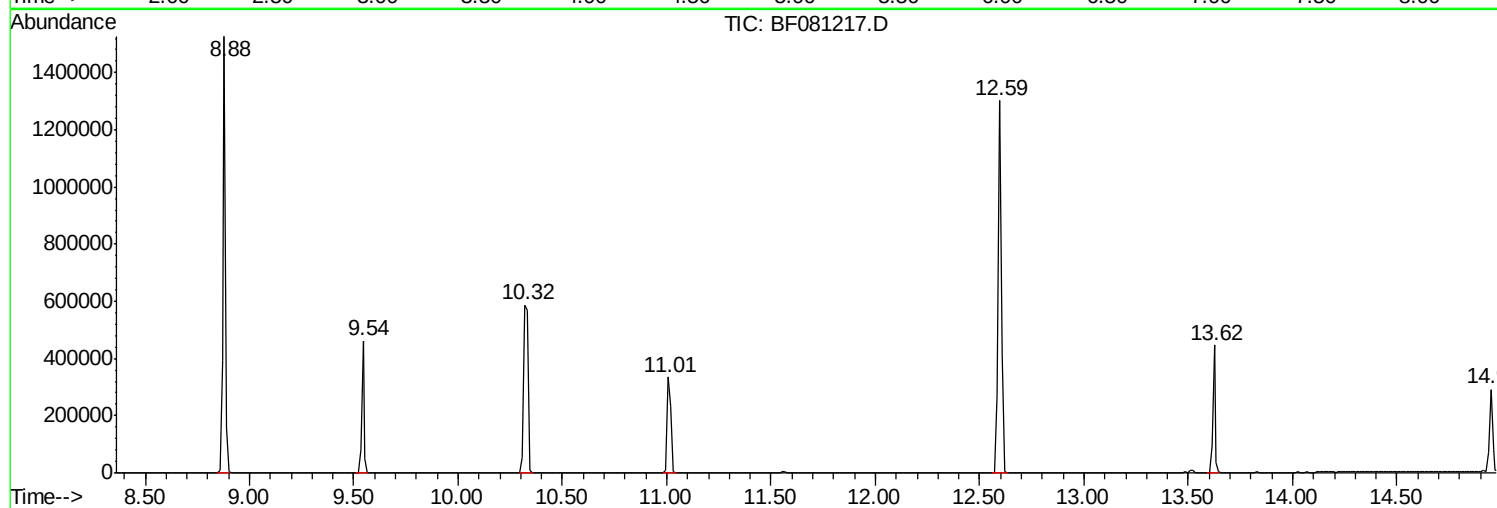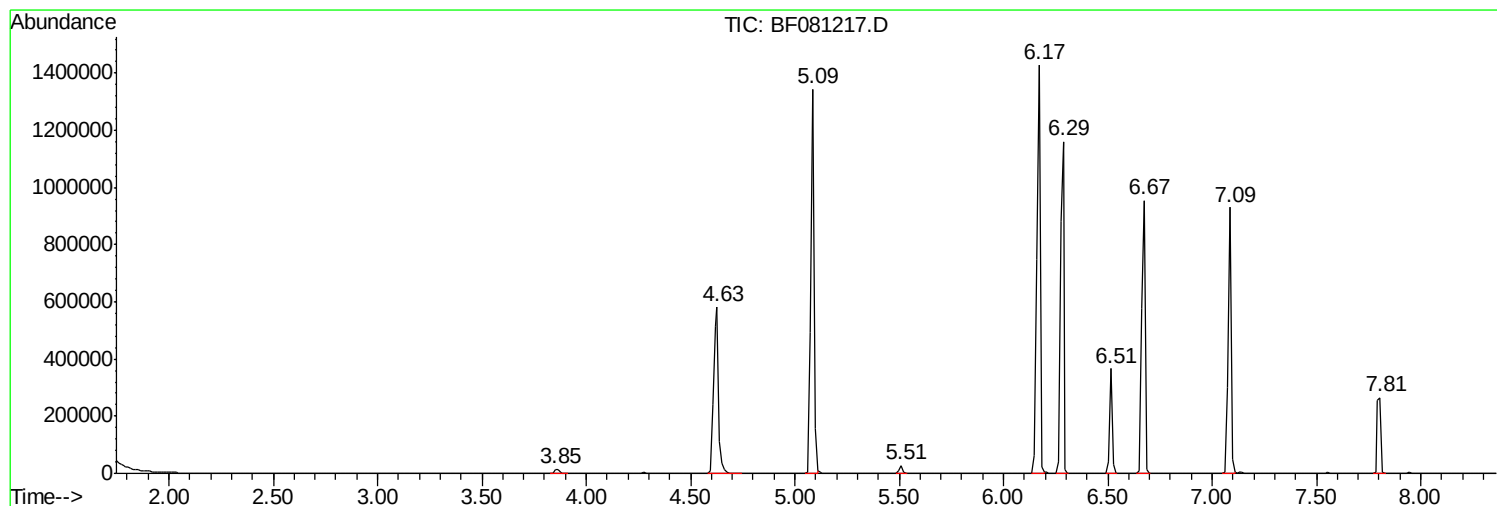

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082615\
Data File : BF081217.D
Acq On : 26 Aug 2015 17:41
Operator : UM/IZ
Sample : PB85190BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB85190BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.63	69.47 ng	1040460	1,4-Dichlorobenzene-d4	6.51

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50	
2	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	33	
3	3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33	
4	2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	33	
5	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23	

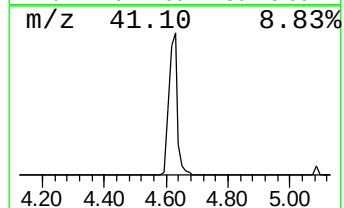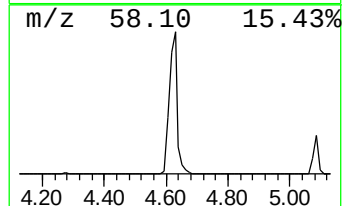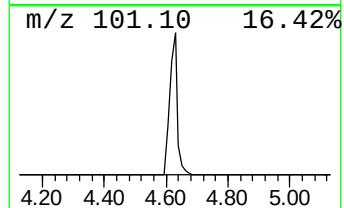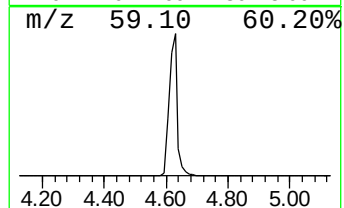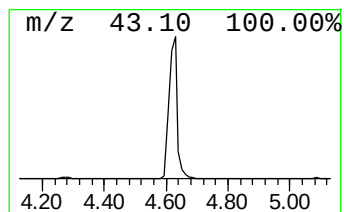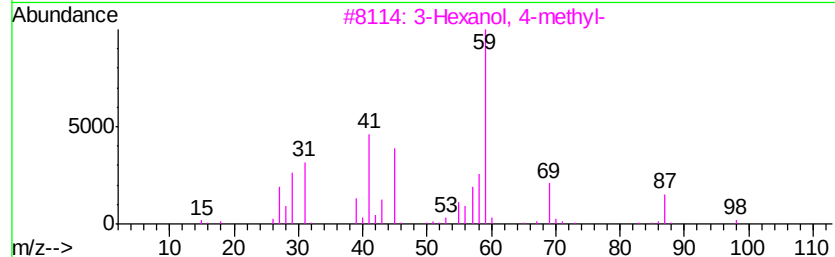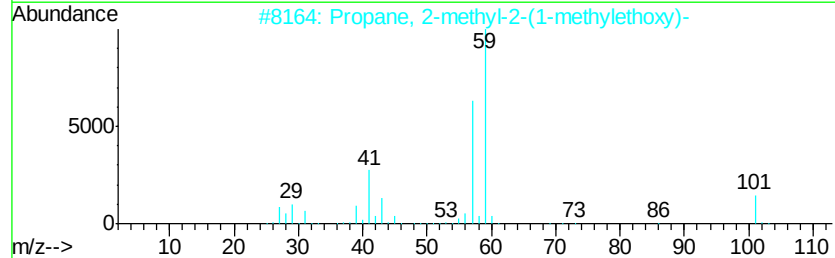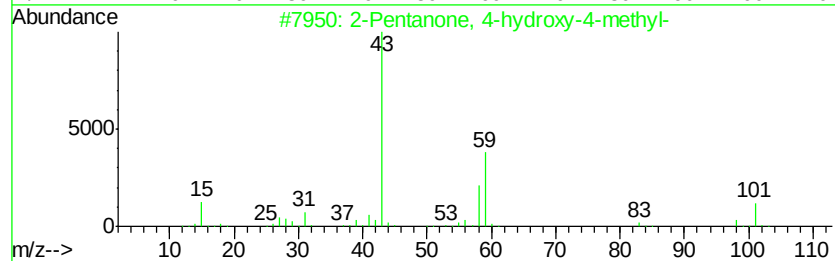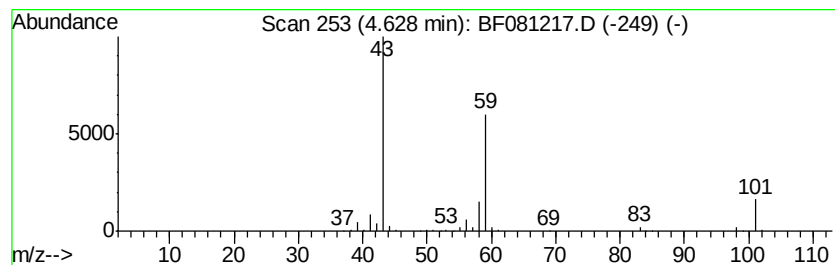

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082615\
Data File : BF081217.D
Acq On : 26 Aug 2015 17:41
Operator : UM/IZ
Sample : PB85190BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB85190BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.29 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.29	95.86 ng	1435680	1,4-Dichlorobenzene-d4	6.51

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Tranlycypromine-propionyl	189	C12H15NO	1000123-86-3	10
4		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

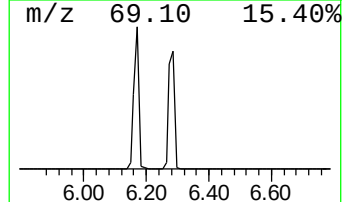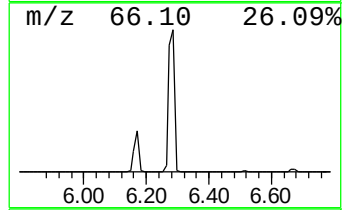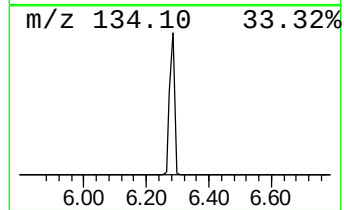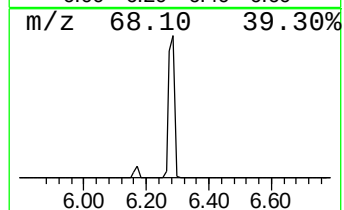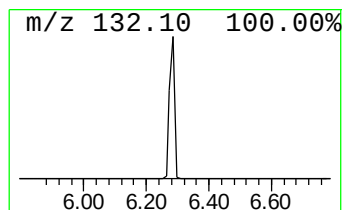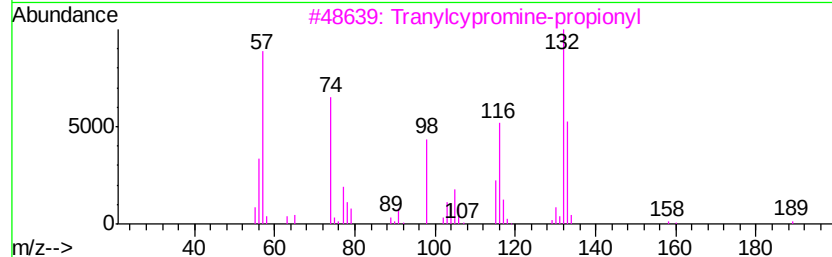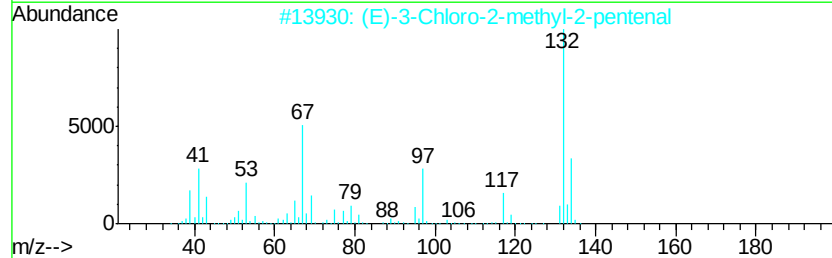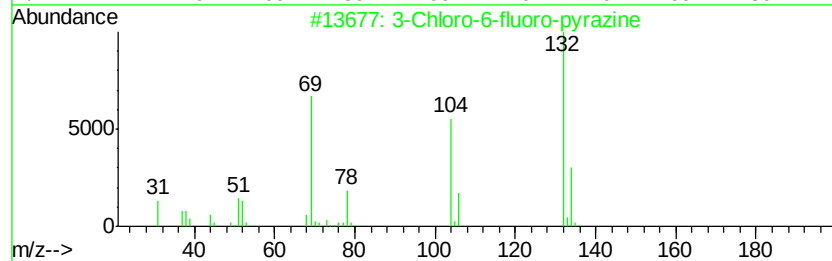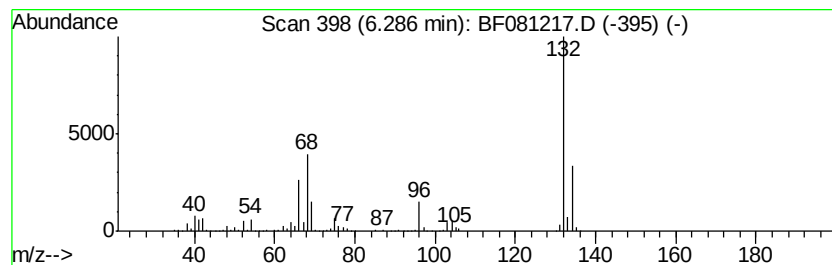

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082615\
Data File : BF081217.D
Acq On : 26 Aug 2015 17:41
Operator : UM/IZ
Sample : PB85190BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB85190BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.63	69.5	ng	1040460	1	6.51	299537	20.0
unknown6.29	6.29	95.9	ng	1435680	1	6.51	299537	20.0