


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082615\
 Data File : BF081215.D
 Acq On : 26 Aug 2015 16:16
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 24 13:58:19 2015

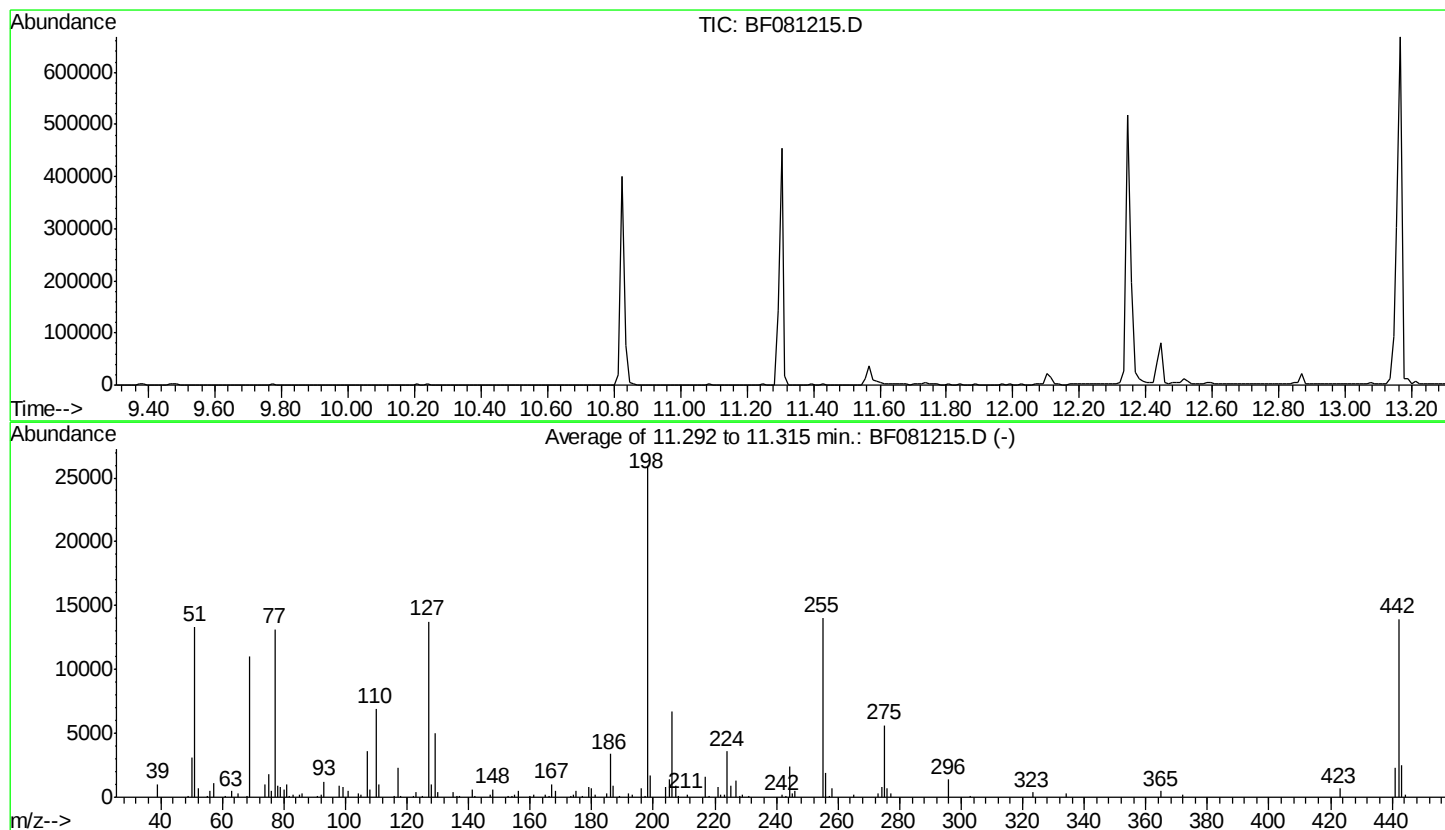

AutoFind: Scans 836, 837, 838; Background Corrected with Scan 833

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.4	13333	PASS
68	69	0.00	2	1.0	107	PASS
69	198	0.00	100	42.6	11060	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.0	13759	PASS
197	198	0.00	2	0.4	109	PASS
198	198	100	100	100.0	25954	PASS
199	198	5	9	6.5	1680	PASS
275	198	10	60	21.6	5619	PASS
365	198	1	100	1.9	487	PASS
441	442	0.01	24	16.2	2264	PASS
442	198	50	100	53.8	13954	PASS
443	442	15	24	17.8	2479	PASS