

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082616\
 Data File : BF089918.D
 Acq On : 26 Aug 2016 20:08
 Operator : UM/SJ
 Sample : PB93109BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB93109BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.644	3	5	13	rBV	1081878	2671848	36.10%	4.078%
2	1.758	13	15	22	rBV	3549472	7400502	100.00%	11.295%
3	4.787	277	280	286	rBV	708520	1182635	15.98%	1.805%
4	5.233	316	319	321	rBV	4631739	4903526	66.26%	7.484%
5	6.284	408	411	414	rBV	3548508	5433624	73.42%	8.293%
6	6.410	419	422	425	rBV	4500028	5378232	72.67%	8.209%
7	6.650	440	443	445	rBV	1842372	1713763	23.16%	2.616%
8	6.799	454	456	459	rBV	3365416	4570154	61.75%	6.975%
9	7.210	489	492	495	rBV	2796301	3131796	42.32%	4.780%
10	7.930	552	555	558	rBV	2577545	2266913	30.63%	3.460%
11	9.016	646	650	652	rBV	6329930	6982352	94.35%	10.657%
12	9.679	705	708	710	rBV	3022283	2683206	36.26%	4.095%
13	10.456	774	776	779	rBV2	2589913	3783246	51.12%	5.774%
14	11.154	834	837	839	rBV	2893205	2806660	37.93%	4.284%
15	12.742	973	976	978	rBV	5483416	6341894	85.70%	9.679%
16	13.771	1063	1066	1068	rBV	2502679	2451458	33.13%	3.742%
17	15.120	1181	1184	1187	rBV	1679590	1817870	24.56%	2.775%


Sum of corrected areas: 65519679

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082616\
Data File : BF089918.D
Acq On : 26 Aug 2016 20:08
Operator : UM/SJ
Sample : PB93109BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB93109BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

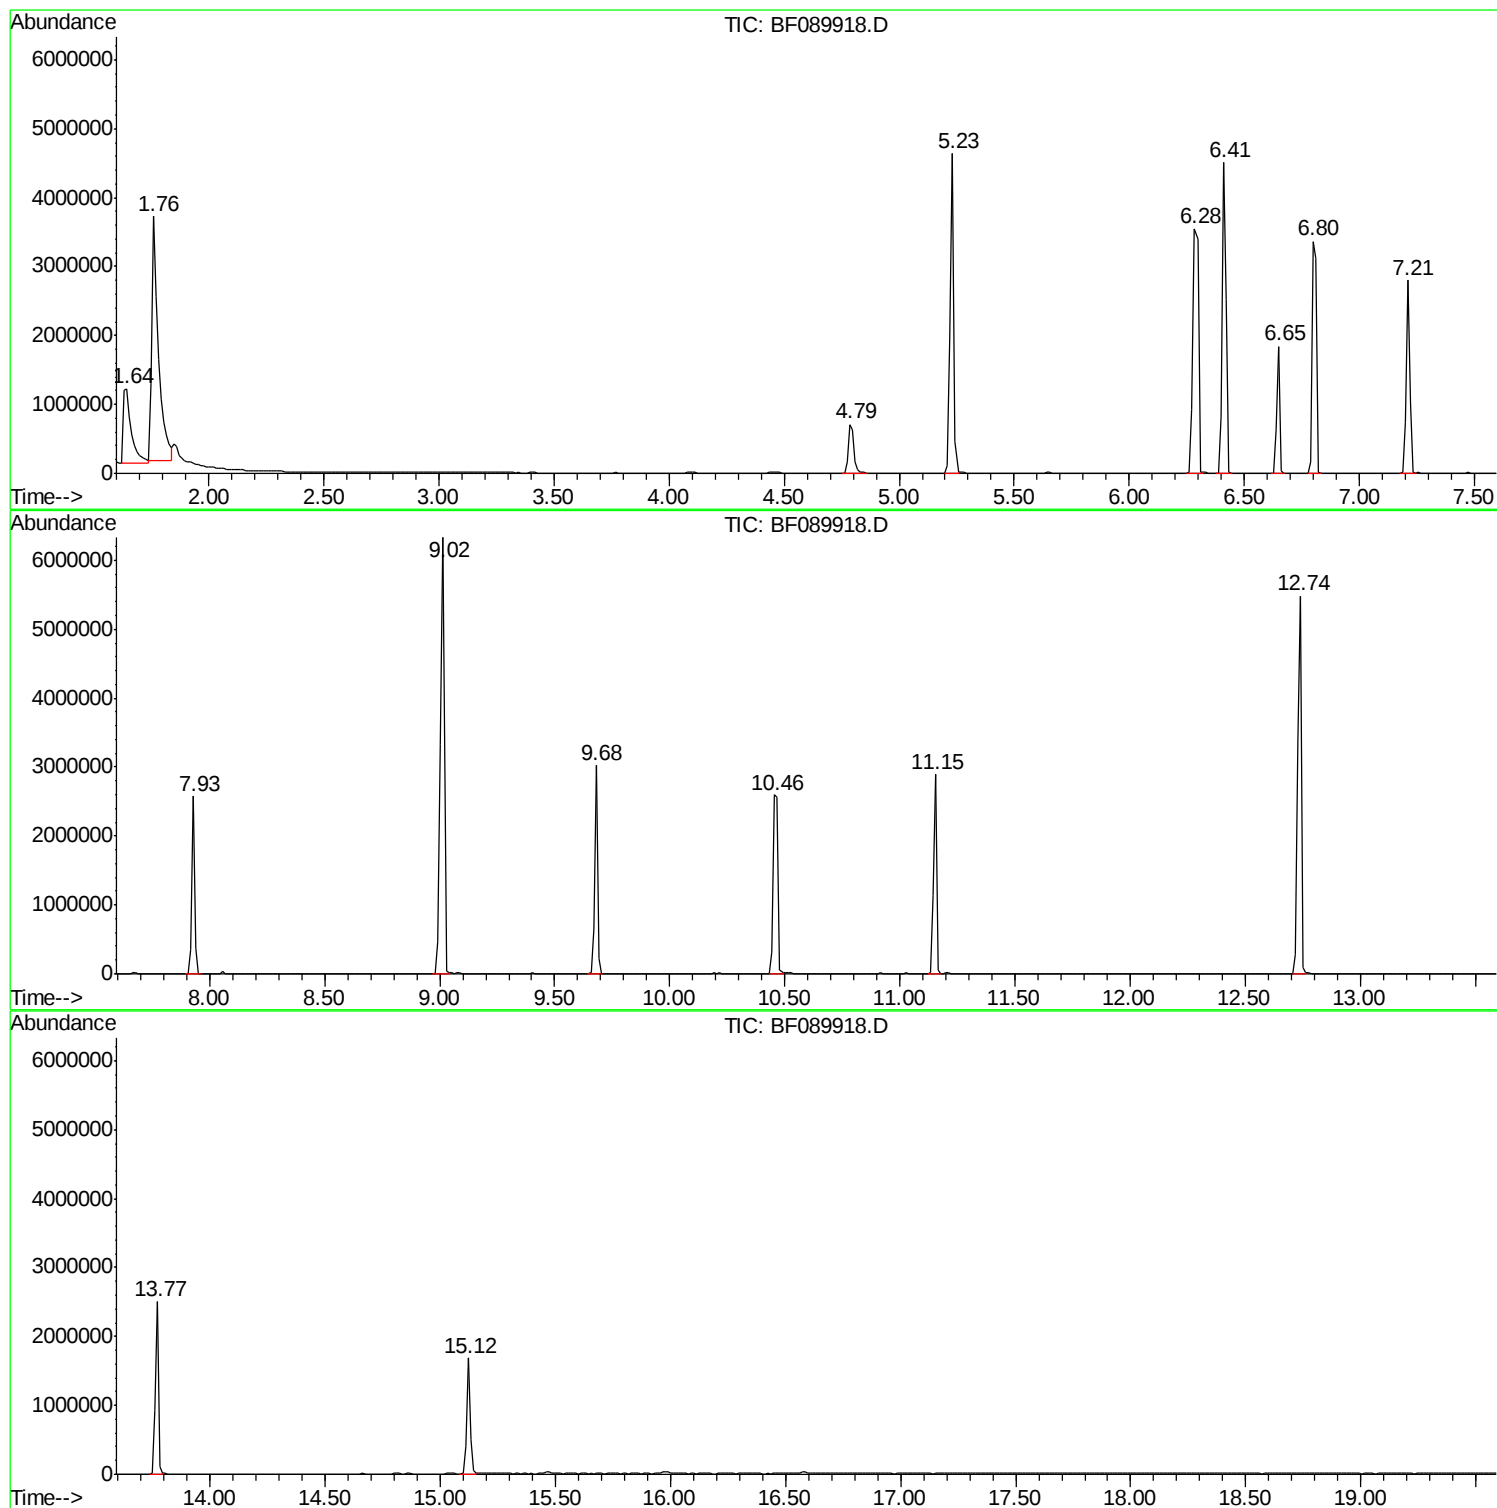

Data Path : Z:\HPCHEM1\BNA F\DATA\BF082616\
Data File : BF089918.D
Acq On : 26 Aug 2016 20:08
Operator : UM/SJ
Sample : PB93109BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB93109BL










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.79	13.80 ng	1182640	1,4-Dichlorobenzene-d4	6.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2		Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	25
3		5-Hexen-2-one	98	C6H10O	000109-49-9	9
4		Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9
5		(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9

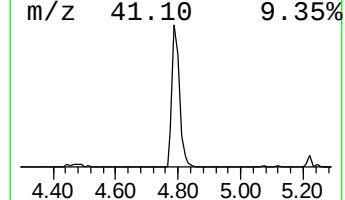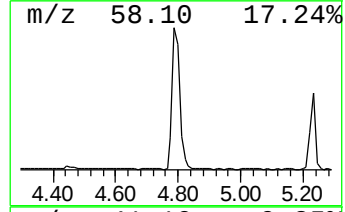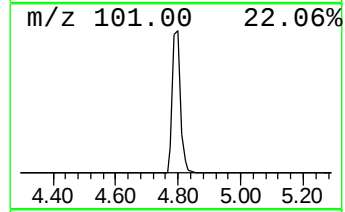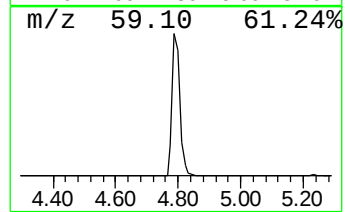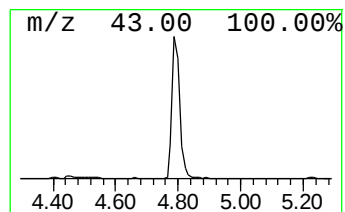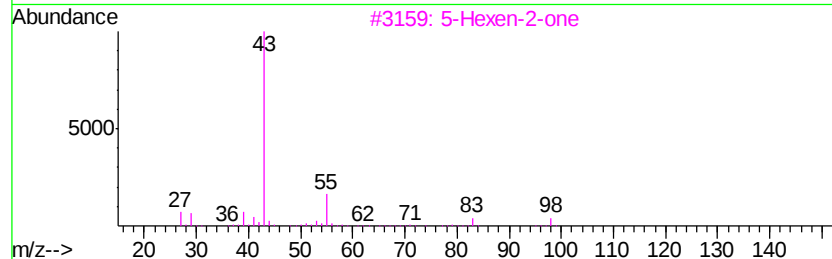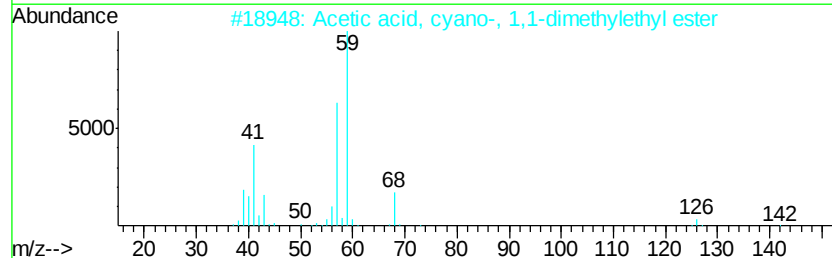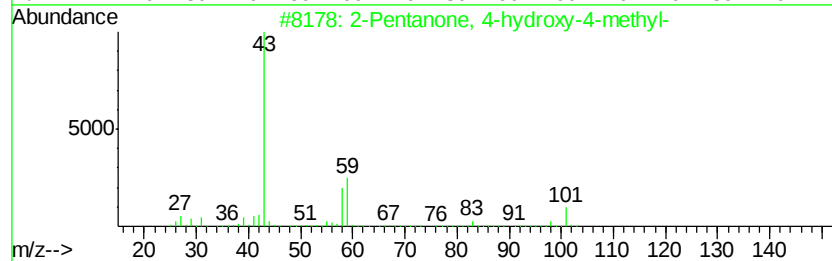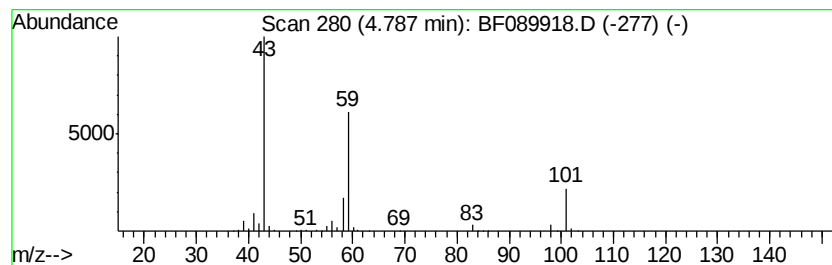

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082616\
Data File : BF089918.D
Acq On : 26 Aug 2016 20:08
Operator : UM/SJ
Sample : PB93109BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB93109BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown6.41 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.41	62.77 ng	5378230	1,4-Dichlorobenzene-d4	6.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

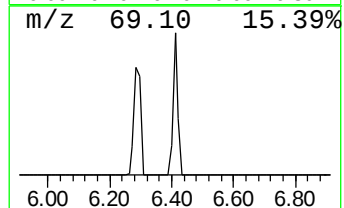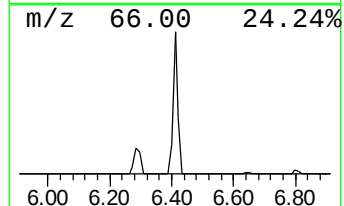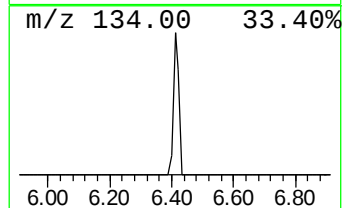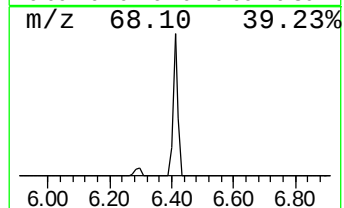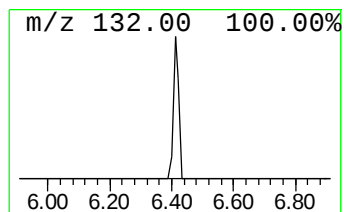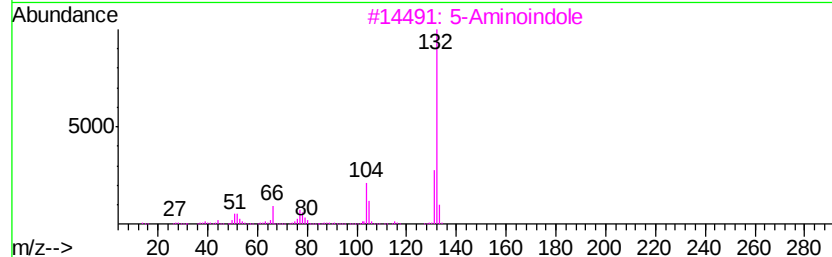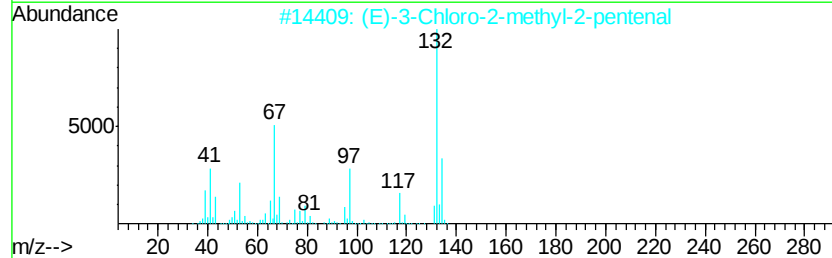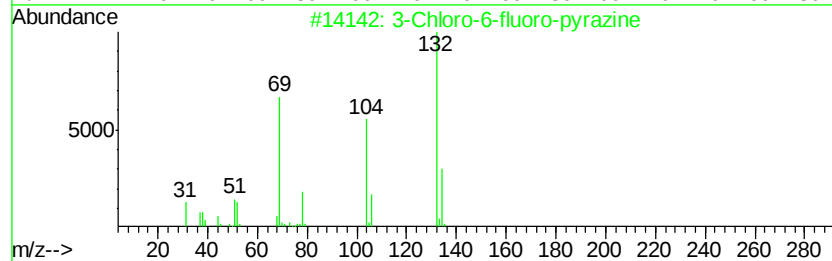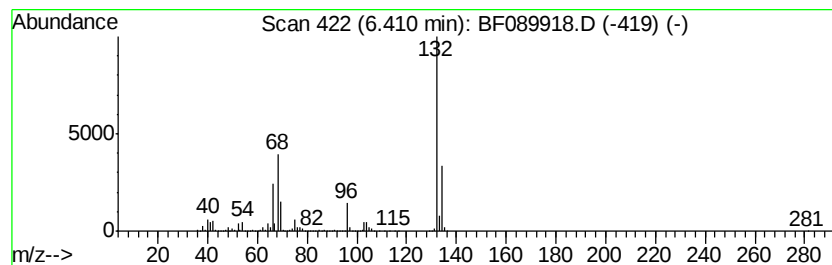

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF082616\
Data File : BF089918.D
Acq On : 26 Aug 2016 20:08
Operator : UM/SJ
Sample : PB93109BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB93109BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.79	13.8	ng	1182640	1	6.65	1713760	20.0
unknown6.41	6.41	62.8	ng	5378230	1	6.65	1713760	20.0