


Data Path : Z:\HPCHEM1\BNA F\DATA\BF082616\
 Data File : BF089912.D
 Acq On : 26 Aug 2016 16:38
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081916.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 26 18:51:25 2016

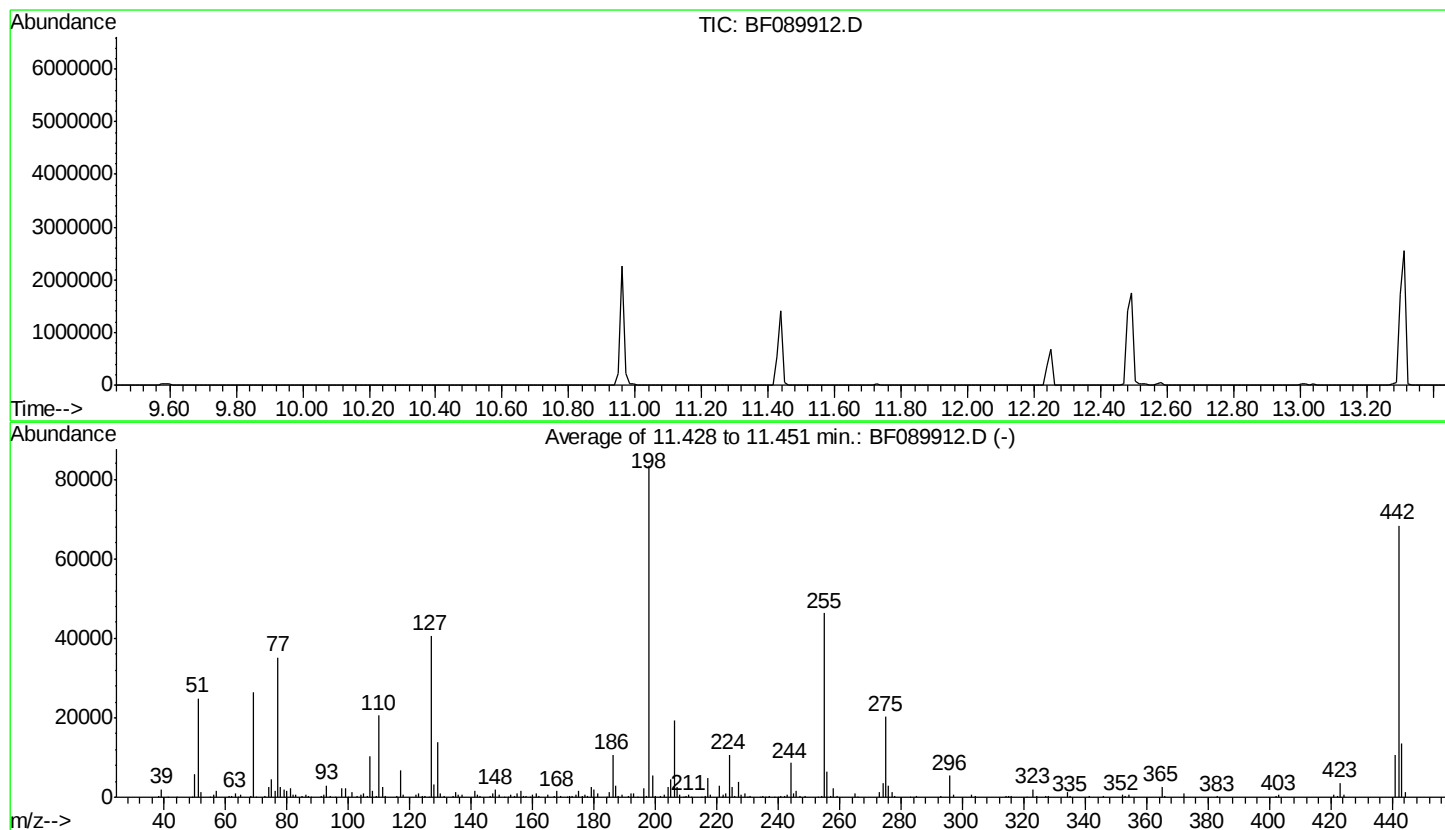

AutoFind: Scans 861, 862, 863; Background Corrected with Scan 857

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	24933	PASS
68	69	0.00	2	1.7	447	PASS
69	198	0.00	100	31.6	26370	PASS
70	69	0.00	2	0.4	115	PASS
127	198	10	80	48.7	40657	PASS
197	198	0.00	2	0.3	290	PASS
198	198	100	100	100.0	83418	PASS
199	198	5	9	6.5	5451	PASS
275	198	10	60	24.3	20269	PASS
365	198	1	100	3.1	2590	PASS
441	442	0.01	24	15.7	10717	PASS
442	198	50	100	81.9	68281	PASS
443	442	15	24	19.8	13493	PASS