

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082619\
 Data File : BF116576.D
 Acq On : 26 Aug 2019 15:57
 Operator : HP/JU
 Sample : K4392-01DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 GW-1DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.040	147	162	170	rVV	1551505	3327052	20.13%	0.619%
2	3.951	309	317	324	rBV2	1681398	3585459	21.70%	0.667%
3	4.093	333	341	346	rBV	1673512	3091488	18.71%	0.575%
4	4.240	356	366	369	rBV	4202092	6719770	40.66%	1.249%
5	4.281	369	373	377	rVB	2505053	2851678	17.26%	0.530%
6	4.557	414	420	427	rVB4	3395164	6419544	38.84%	1.194%
7	4.663	430	438	442	rBV	2508621	3051602	18.46%	0.567%
8	4.863	467	472	475	rBV	1991804	2286194	13.83%	0.425%
9	4.981	481	492	495	rBV	3371165	5693193	34.45%	1.059%
10	5.069	501	507	514	rVV3	6738075	12894325	78.02%	2.398%
11	5.134	514	518	521	rVV	5602100	6325934	38.28%	1.176%
12	5.175	521	525	530	rVV3	1525432	3013958	18.24%	0.560%
13	5.328	546	551	554	rBV	6798566	8747692	52.93%	1.627%
14	5.363	554	557	560	rVB2	1935385	2431316	14.71%	0.452%
15	5.416	560	566	568	rBV	3457889	4877879	29.52%	0.907%
16	5.440	568	570	573	rVB	4017443	3629181	21.96%	0.675%
17	5.492	575	579	580	rBV2	2864321	3691609	22.34%	0.686%
18	5.522	580	584	589	rVB	5724523	7934300	48.01%	1.475%
19	5.604	595	598	601	rBV	2363827	2153167	13.03%	0.400%
20	5.687	608	612	615	rBV2	3457177	4638612	28.07%	0.862%
21	5.734	615	620	622	rVB	5746062	6404851	38.75%	1.191%
22	5.775	622	627	629	rBV	4005669	4725032	28.59%	0.879%
23	5.822	632	635	641	rVB2	1761968	3189378	19.30%	0.593%
24	5.934	647	654	658	rBV4	5075009	9399862	56.88%	1.748%
25	5.992	658	664	671	rBV3	3652683	9138838	55.30%	1.699%
26	6.069	671	677	681	rVB2	7292964	11280983	68.26%	2.098%
27	6.122	681	686	690	rBV2	3649187	5925304	35.85%	1.102%
28	6.175	690	695	700	rBV3	8584162	13805364	83.53%	2.567%
29	6.228	700	704	706	rBV2	3734112	4132811	25.01%	0.768%
30	6.357	720	726	730	rBV3	6902740	11505910	69.62%	2.139%
31	6.428	730	738	740	rBV2	6131156	12037187	72.83%	2.238%
32	6.457	740	743	745	rVV2	4927510	6063023	36.69%	1.127%
33	6.516	749	753	756	rVB2	7354006	7937998	48.03%	1.476%
34	6.592	764	766	769	rVB3	2045338	1928374	11.67%	0.359%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082619\
 Data File : BF116576.D
 Acq On : 26 Aug 2019 15:57
 Operator : HP/JU
 Sample : K4392-01DL 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 GW-1DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	6.663	773	778	782	rBV3	4366501	7800462	47.20%	1.450%
36	6.739	787	791	795	rBV2	5744102	5994409	36.27%	1.115%
37	6.839	803	808	809	rBV3	1703337	2103794	12.73%	0.391%
38	6.898	813	818	820	rBV2	2070046	2659862	16.09%	0.495%
39	6.934	820	824	826	rVB	5926351	6147449	37.20%	1.143%
40	6.963	826	829	834	rVB3	4525795	5909025	35.75%	1.099%
41	7.063	842	846	849	rVB2	4699250	5255882	31.80%	0.977%
42	7.139	856	859	863	rBV4	1879686	2670903	16.16%	0.497%
43	7.186	863	867	870	rVB2	4297817	5396415	32.65%	1.003%
44	7.222	870	873	875	rBV2	5219993	5081568	30.75%	0.945%
45	7.251	875	878	882	rVB2	4400637	4894466	29.62%	0.910%
46	7.298	882	886	890	rBV2	5800797	6812297	41.22%	1.267%
47	7.439	905	910	913	rBV2	5162139	7400551	44.78%	1.376%
48	7.504	919	921	924	rVB2	2973034	2569368	15.55%	0.478%
49	7.551	924	929	932	rVB4	3048144	4833574	29.25%	0.899%
50	7.616	936	940	943	rVB3	2284128	2904414	17.57%	0.540%
51	7.675	943	950	951	rBV2	1845628	3071469	18.58%	0.571%
52	7.698	951	954	960	rVB3	3457843	6119305	37.03%	1.138%
53	7.786	965	969	971	rBV4	1714375	2214039	13.40%	0.412%
54	7.875	979	984	986	rVB3	2717824	3929736	23.78%	0.731%
55	7.904	986	989	991	rBV2	2919194	3384784	20.48%	0.629%
56	7.986	999	1003	1004	rBV2	2219431	2206371	13.35%	0.410%
57	8.145	1024	1030	1031	rVV5	2180208	3438439	20.81%	0.639%
58	8.175	1031	1035	1037	rVV3	5632841	7199582	43.56%	1.339%
59	8.204	1037	1040	1043	rVV2	4073440	5358474	32.42%	0.996%
60	8.233	1043	1045	1046	rVV	2659687	2593945	15.70%	0.482%
61	8.251	1046	1048	1050	rVV	4468245	4176051	25.27%	0.776%
62	8.480	1081	1087	1090	rBV5	3692494	5837646	35.32%	1.085%
63	8.569	1099	1102	1105	rBV2	3813364	3968865	24.01%	0.738%
64	8.622	1106	1111	1114	rVV2	5072290	6353493	38.44%	1.181%
65	8.651	1114	1116	1119	rVB	2268302	2279314	13.79%	0.424%
66	8.692	1120	1123	1126	rBV2	2363597	2732161	16.53%	0.508%
67	8.792	1135	1140	1144	rBV3	3628994	5137514	31.09%	0.955%
68	8.916	1152	1161	1163	rVB3	6600929	15605539	94.43%	2.902%
69	9.016	1172	1178	1180	rVV	5187035	7578624	45.86%	1.409%
70	9.222	1209	1213	1215	rVB	4991237	5714341	34.58%	1.063%
71	9.357	1231	1236	1240	rBV4	3972939	7163115	43.34%	1.332%

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082619\
Data File : BF116576.D
Acq On : 26 Aug 2019 15:57
Operator : HP/JU
Sample : K4392-01DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GW-1DL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082319.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	9.469	1252	1255	1260	rVB	3910630	5454726	33.01%	1.014%
73	9.551	1261	1269	1271	rBV	6159948	13148283	79.56%	2.445%
74	9.627	1271	1282	1284	rBV4	6324705	16526660	100.00%	3.073%
75	9.680	1288	1291	1293	rVV2	6178718	6974175	42.20%	1.297%
76	9.733	1296	1300	1305	rBV	4359015	6857823	41.50%	1.275%
77	9.816	1310	1314	1318	rVB2	3277371	3906410	23.64%	0.726%
78	9.886	1324	1326	1330	rVB2	2881751	2298705	13.91%	0.427%
79	9.927	1330	1333	1334	rBV	3038234	3166433	19.16%	0.589%
80	9.969	1338	1340	1342	rBV2	1674042	1861284	11.26%	0.346%
81	10.057	1351	1355	1359	rVB2	4454934	7245233	43.84%	1.347%
82	10.098	1359	1362	1366	rBV5	2223786	3331531	20.16%	0.619%
83	10.157	1367	1372	1375	rVV2	4754073	8219790	49.74%	1.528%
84	10.204	1376	1380	1387	rVB4	5789365	9734979	58.90%	1.810%
85	10.275	1387	1392	1394	rBV	4080904	5081500	30.75%	0.945%
86	10.304	1394	1397	1399	rVB	3700141	3098232	18.75%	0.576%
87	10.363	1403	1407	1408	rBV	2781893	3357987	20.32%	0.624%
88	10.380	1408	1410	1413	rVB	4351871	3528395	21.35%	0.656%
89	10.445	1418	1421	1424	rVB2	2052970	2186342	13.23%	0.407%
90	10.492	1426	1429	1431	rBV2	2022583	1924314	11.64%	0.358%
91	10.604	1446	1448	1451	rVB2	4961507	4810077	29.10%	0.894%
92	10.880	1488	1495	1500	rVB2	6208138	11882535	71.90%	2.209%
93	10.933	1501	1504	1506	rBV2	1783687	1983589	12.00%	0.369%
94	11.039	1518	1522	1524	rVV4	2072893	2633005	15.93%	0.490%
95	11.074	1524	1528	1531	rVV3	3400411	3899348	23.59%	0.725%
96	11.327	1567	1571	1576	rVB2	4975035	6793259	41.10%	1.263%
97	11.451	1589	1592	1595	rVV	2145050	2155932	13.05%	0.401%
98	11.751	1639	1643	1645	rBV3	1503367	2029063	12.28%	0.377%
99	11.951	1675	1677	1681	rVB	2308324	2176775	13.17%	0.405%
100	12.468	1761	1765	1768	rBV2	2029830	2214264	13.40%	0.412%


Sum of corrected areas: 537816763

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF082619\
Data File : BF116576.D
Acq On : 26 Aug 2019 15:57
Operator : HP/JU
Sample : K4392-01DL 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
GW-1DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

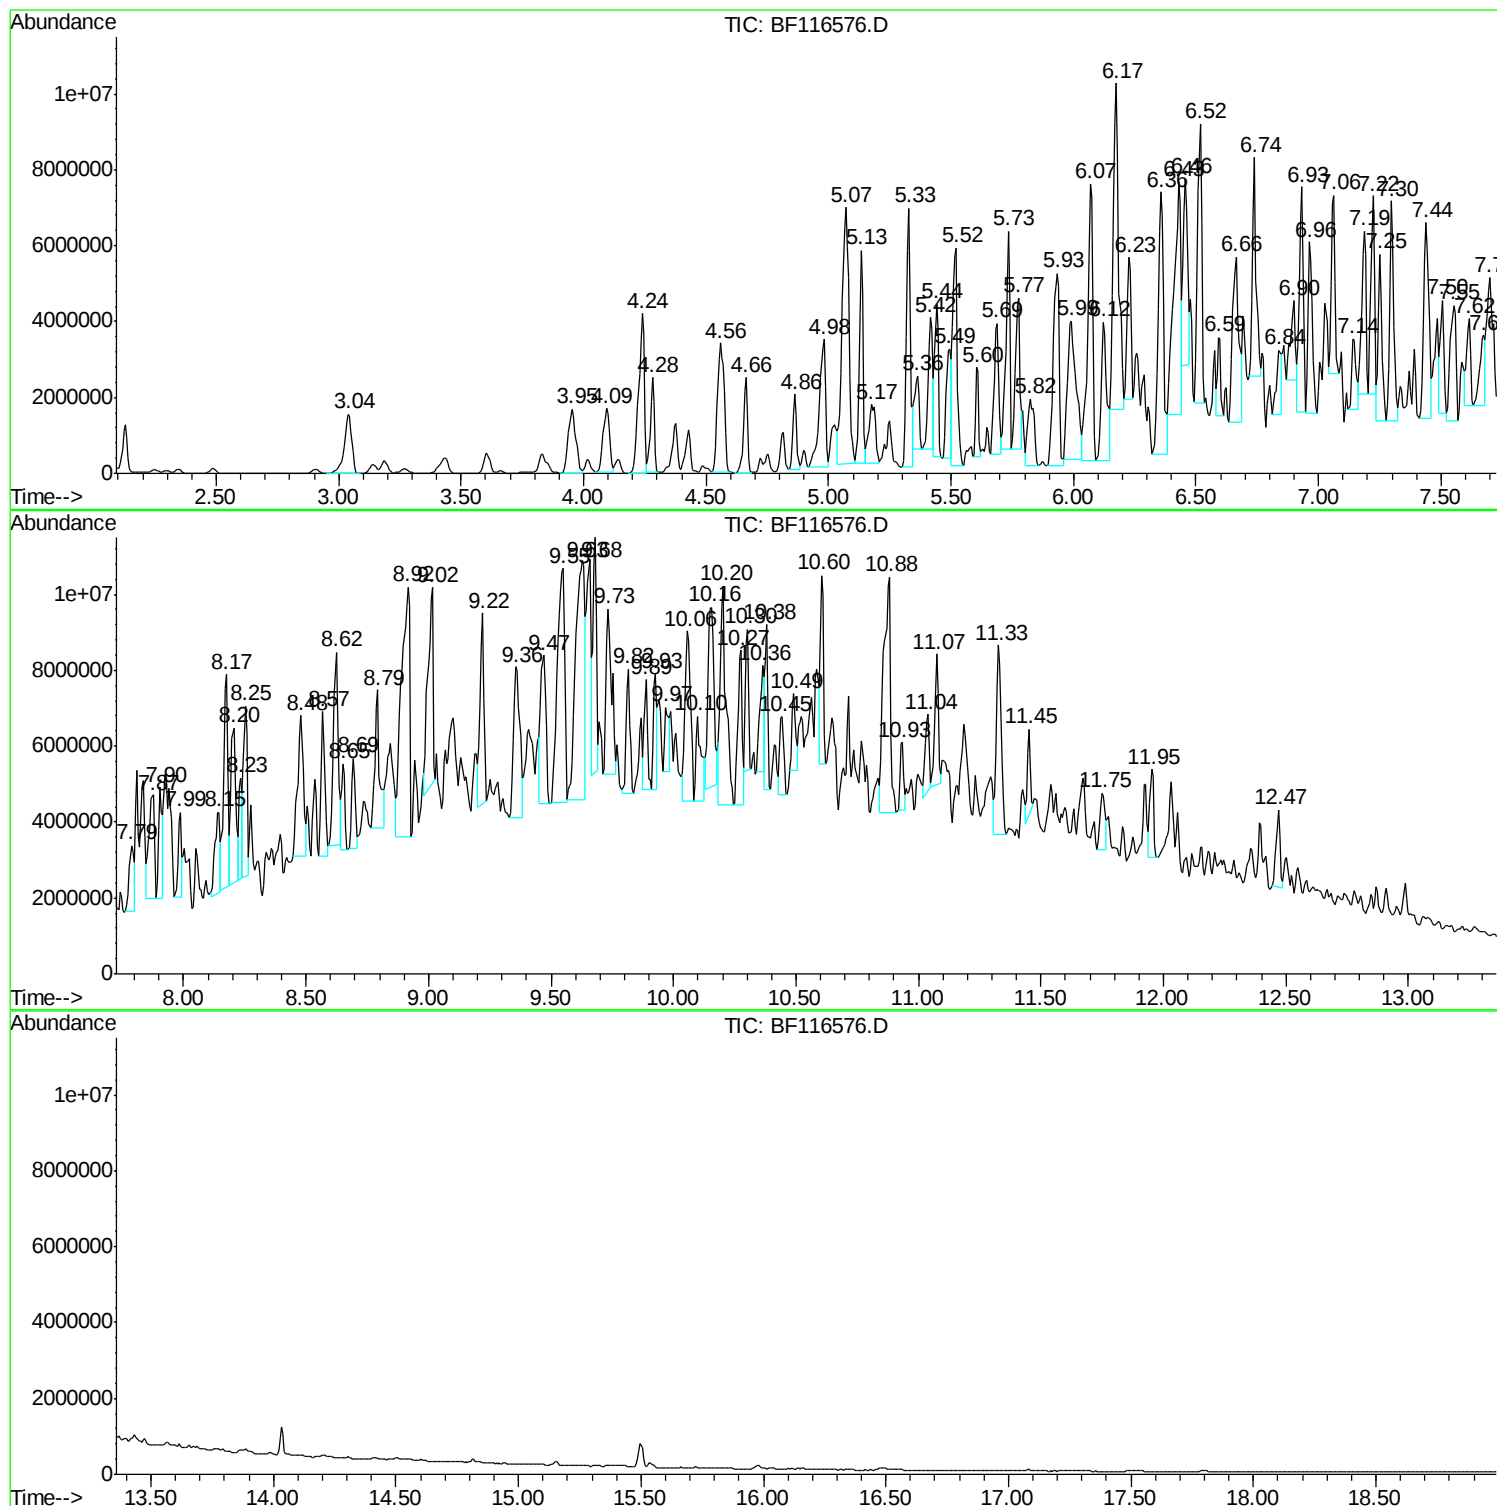

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082619\
Data_File : BF116576.D
Acq_On : 26_Aug_2019_ 15:577
Operator : HP/JUU
Sample : K4392-01DL_5XX
Misc :
ALS_Vial : 13 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
GW-1DL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082319.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
