


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF082619\
 Data File : BF116564.D
 Acq On : 26 Aug 2019 10:28
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF082319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 23 13:38:31 2019

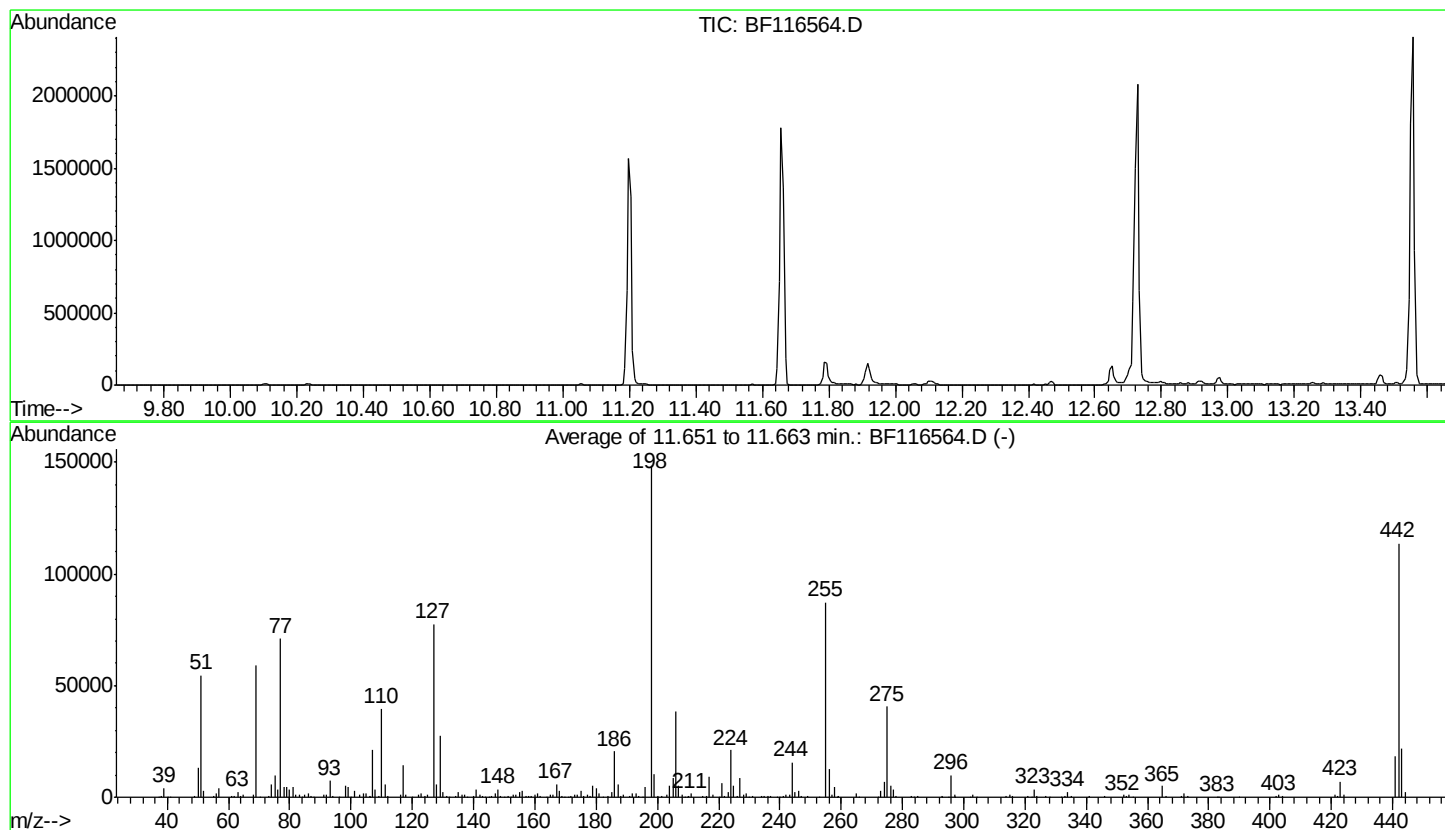

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	54624	PASS
68	69	0.00	2	1.9	1116	PASS
69	198	0.00	100	40.0	59359	PASS
70	69	0.00	2	0.3	193	PASS
127	198	10	80	52.1	77437	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	148557	PASS
199	198	5	9	6.8	10168	PASS
275	198	10	60	27.4	40688	PASS
365	198	1	100	3.3	4952	PASS
441	198	0.01	100	12.5	18555	PASS
442	198	50	100	76.6	113768	PASS
443	442	15	24	19.2	21896	PASS