
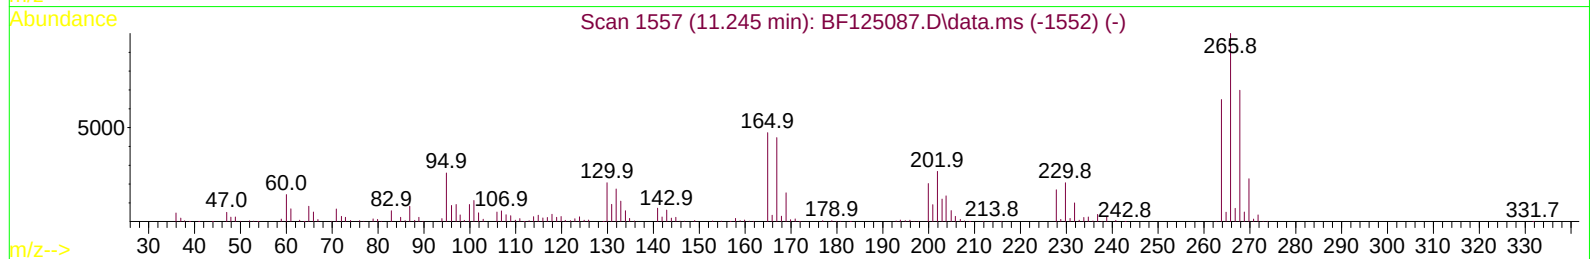
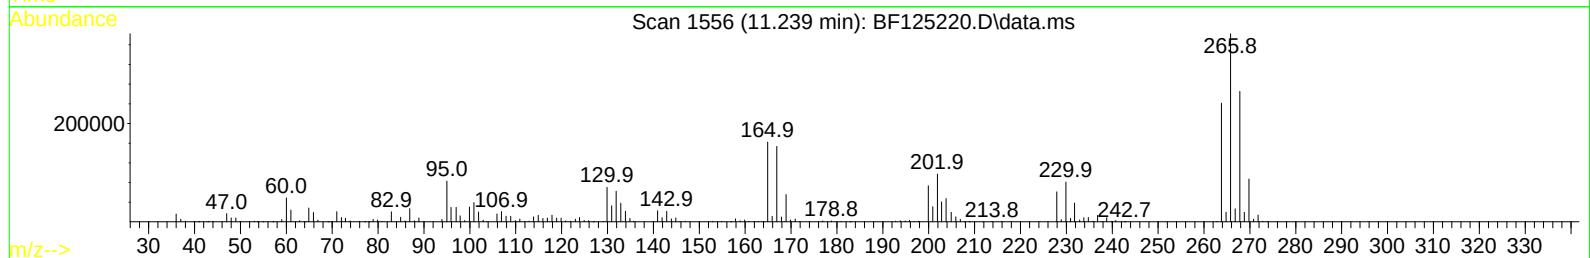


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF082621\  
Data File : BF125220.D  
Acq On : 26 Aug 2021 11:11  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 12:56:40 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF081821.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Aug 24 12:39:21 2021  
Response via : Initial Calibration

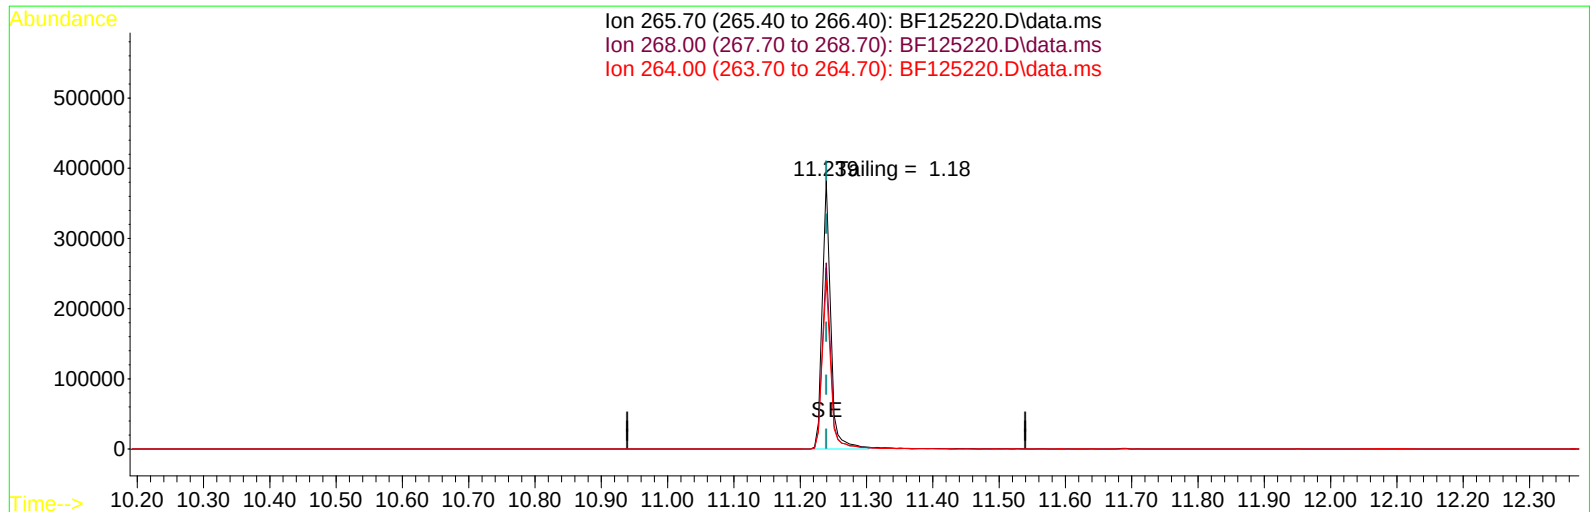

TIC: BF125220.D\data.ms

**(70) Pentachlorophenol (C)**




**11.239min ( 0.000) 40577.08 ng**

**response 347709**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.10  | 69.35  |
| 264.00 | 69.90  | 63.06  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF082621\  
 Data File : BF125220.D  
 Acq On : 26 Aug 2021 11:11  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 12:56:40 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF081821.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Aug 24 12:39:21 2021  
 Response via : Initial Calibration

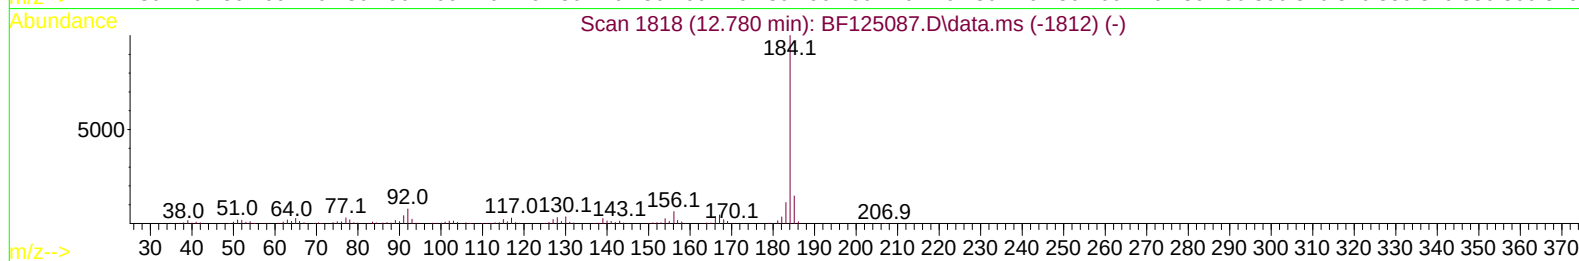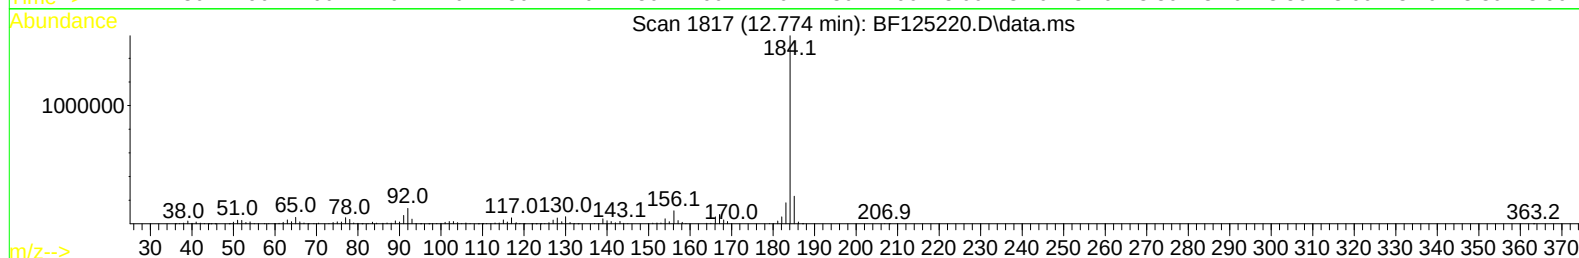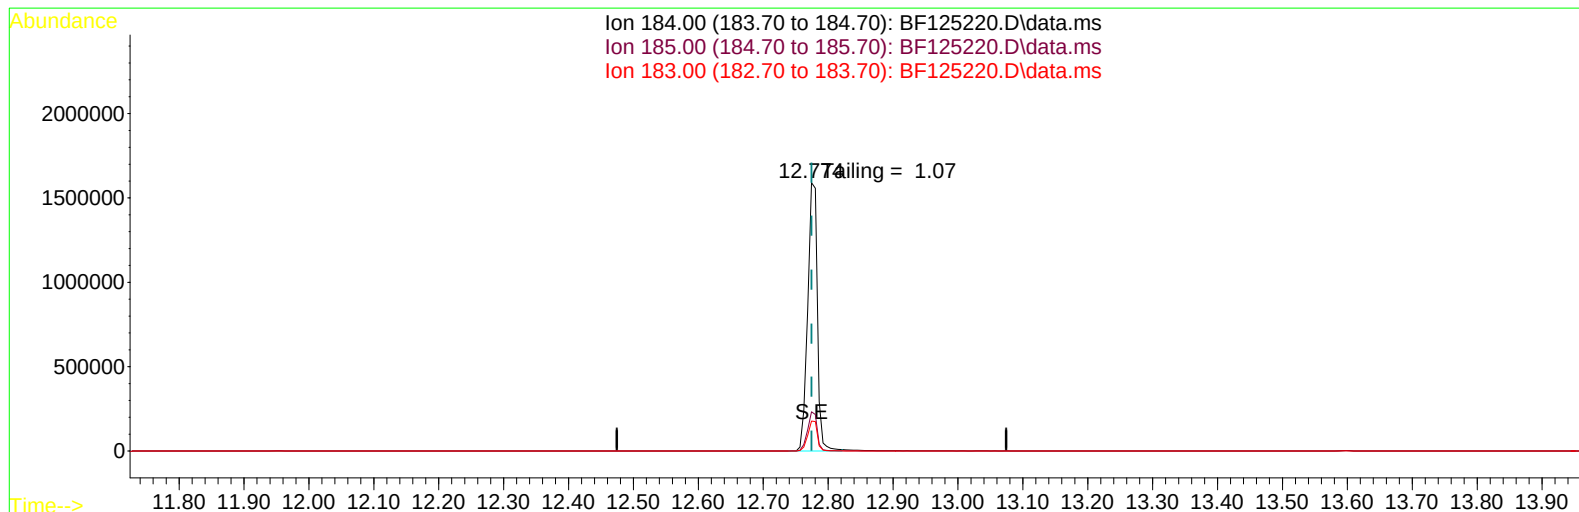

TIC: BF125220.D\data.ms

**(77) Benzidine**

12.774min (+ 0.000) 0.00 ng

response 1669055

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.50  | 14.64  |
| 183.00 | 10.10  | 11.14  |
| 0.00   | 0.00   | 0.00   |