
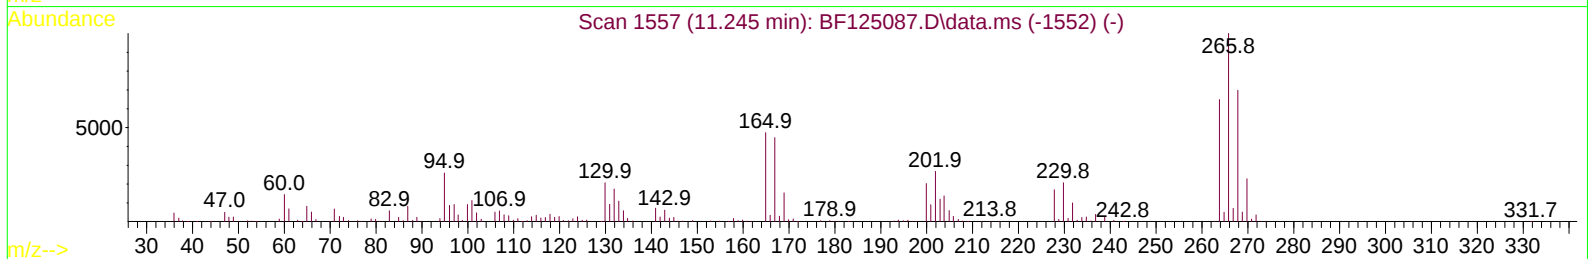
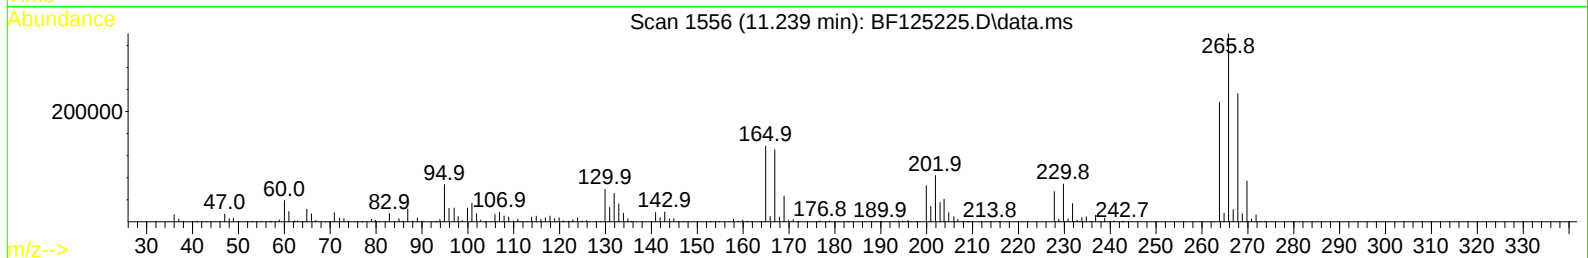


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082621\
 Data File : BF125225.D
 Acq On : 26 Aug 2021 14:13
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 14:56:44 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 12:39:21 2021
 Response via : Initial Calibration

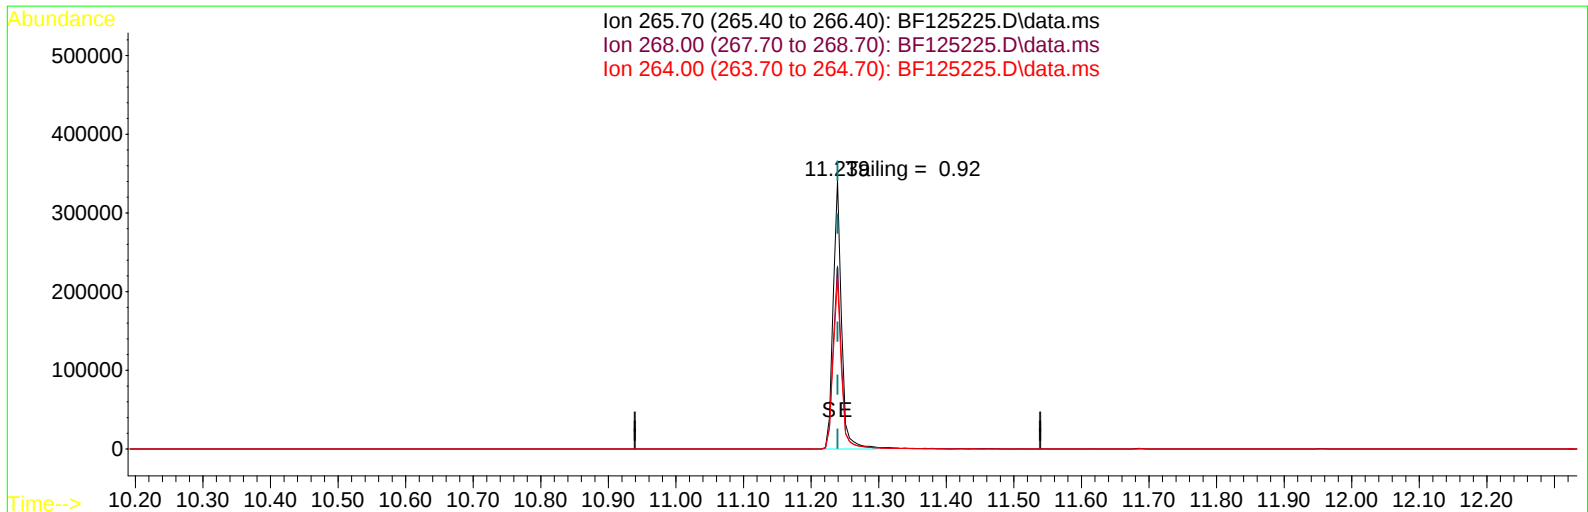

TIC: BF125225.D\data.ms

(70) Pentachlorophenol (C)




11.239min (-0.000) 300359.57 ng

response 294645

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	68.16
264.00	69.90	63.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082621\
Data File : BF125225.D
Acq On : 26 Aug 2021 14:13
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 26 14:56:44 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 12:39:21 2021
Response via : Initial Calibration

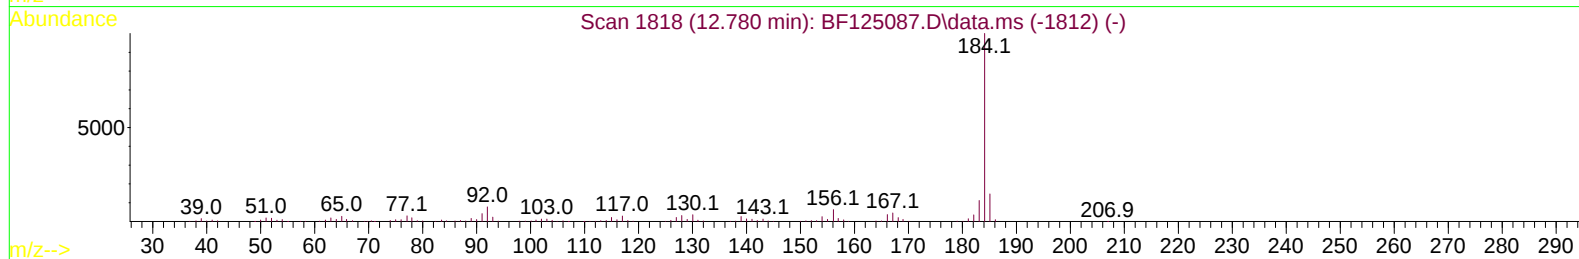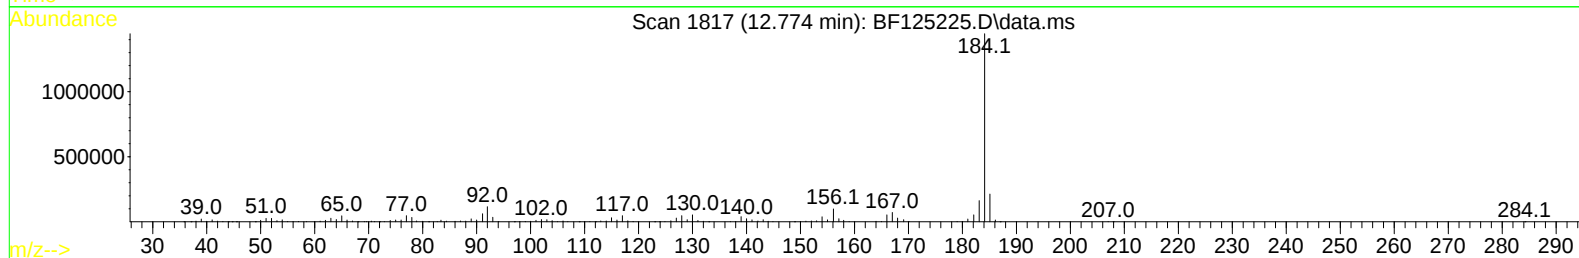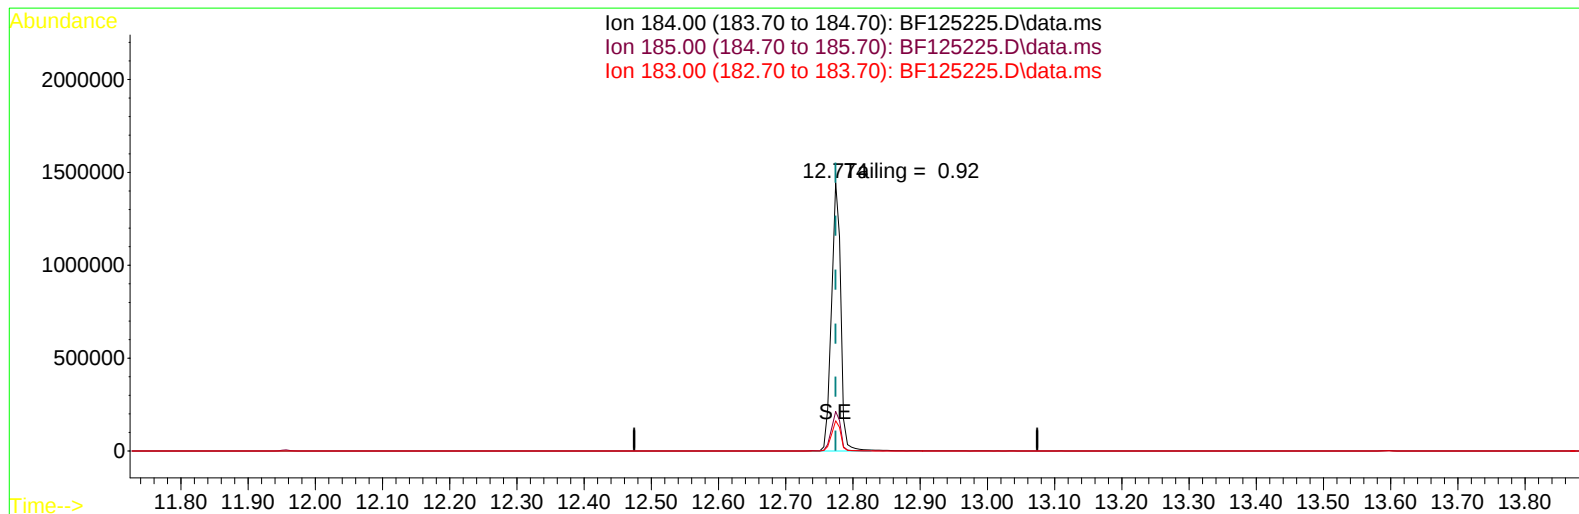

TIC: BF125225.D\data.ms

(77) Benzidine

12.774min (-0.000) 43272.50 ng

response 1393403

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.73
183.00	10.10	11.26
0.00	0.00	0.00