

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082621\
 Data File : BF125232.D
 Acq On : 26 Aug 2021 19:01
 Operator : JU/CG
 Sample : M3528-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PT-3-082421

Quant Time: Aug 27 05:02:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 12:39:21 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.916	152	197581	20.000	ng	0.00
21) Naphthalene-d8	8.192	136	752175	20.000	ng	# 0.00
39) Acenaphthene-d10	9.951	164	398894	20.000	ng	0.00
64) Phenanthrene-d10	11.433	188	687235	20.000	ng	0.00
76) Chrysene-d12	14.074	240	423134	20.000	ng	0.00
86) Perylene-d12	15.568	264	418696	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.546	112	1297988	99.434	ng	0.02
7) Phenol-d6	6.540	99	1485339	87.980	ng	0.00
23) Nitrobenzene-d5	7.475	82	1208472	80.885	ng	0.00
42) 2,4,6-Tribromophenol	10.739	330	528653	132.766	ng	0.00
45) 2-Fluorobiphenyl	9.269	172	2126002	74.282	ng	0.00
79) Terphenyl-d14	13.022	244	2178148	82.007	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082621\
Data File : BF125232.D
Acq On : 26 Aug 2021 19:01
Operator : JU/CG
Sample : M3528-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PT-3-082421

Quant Time: Aug 27 05:02:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 24 12:39:21 2021
Response via : Initial Calibration




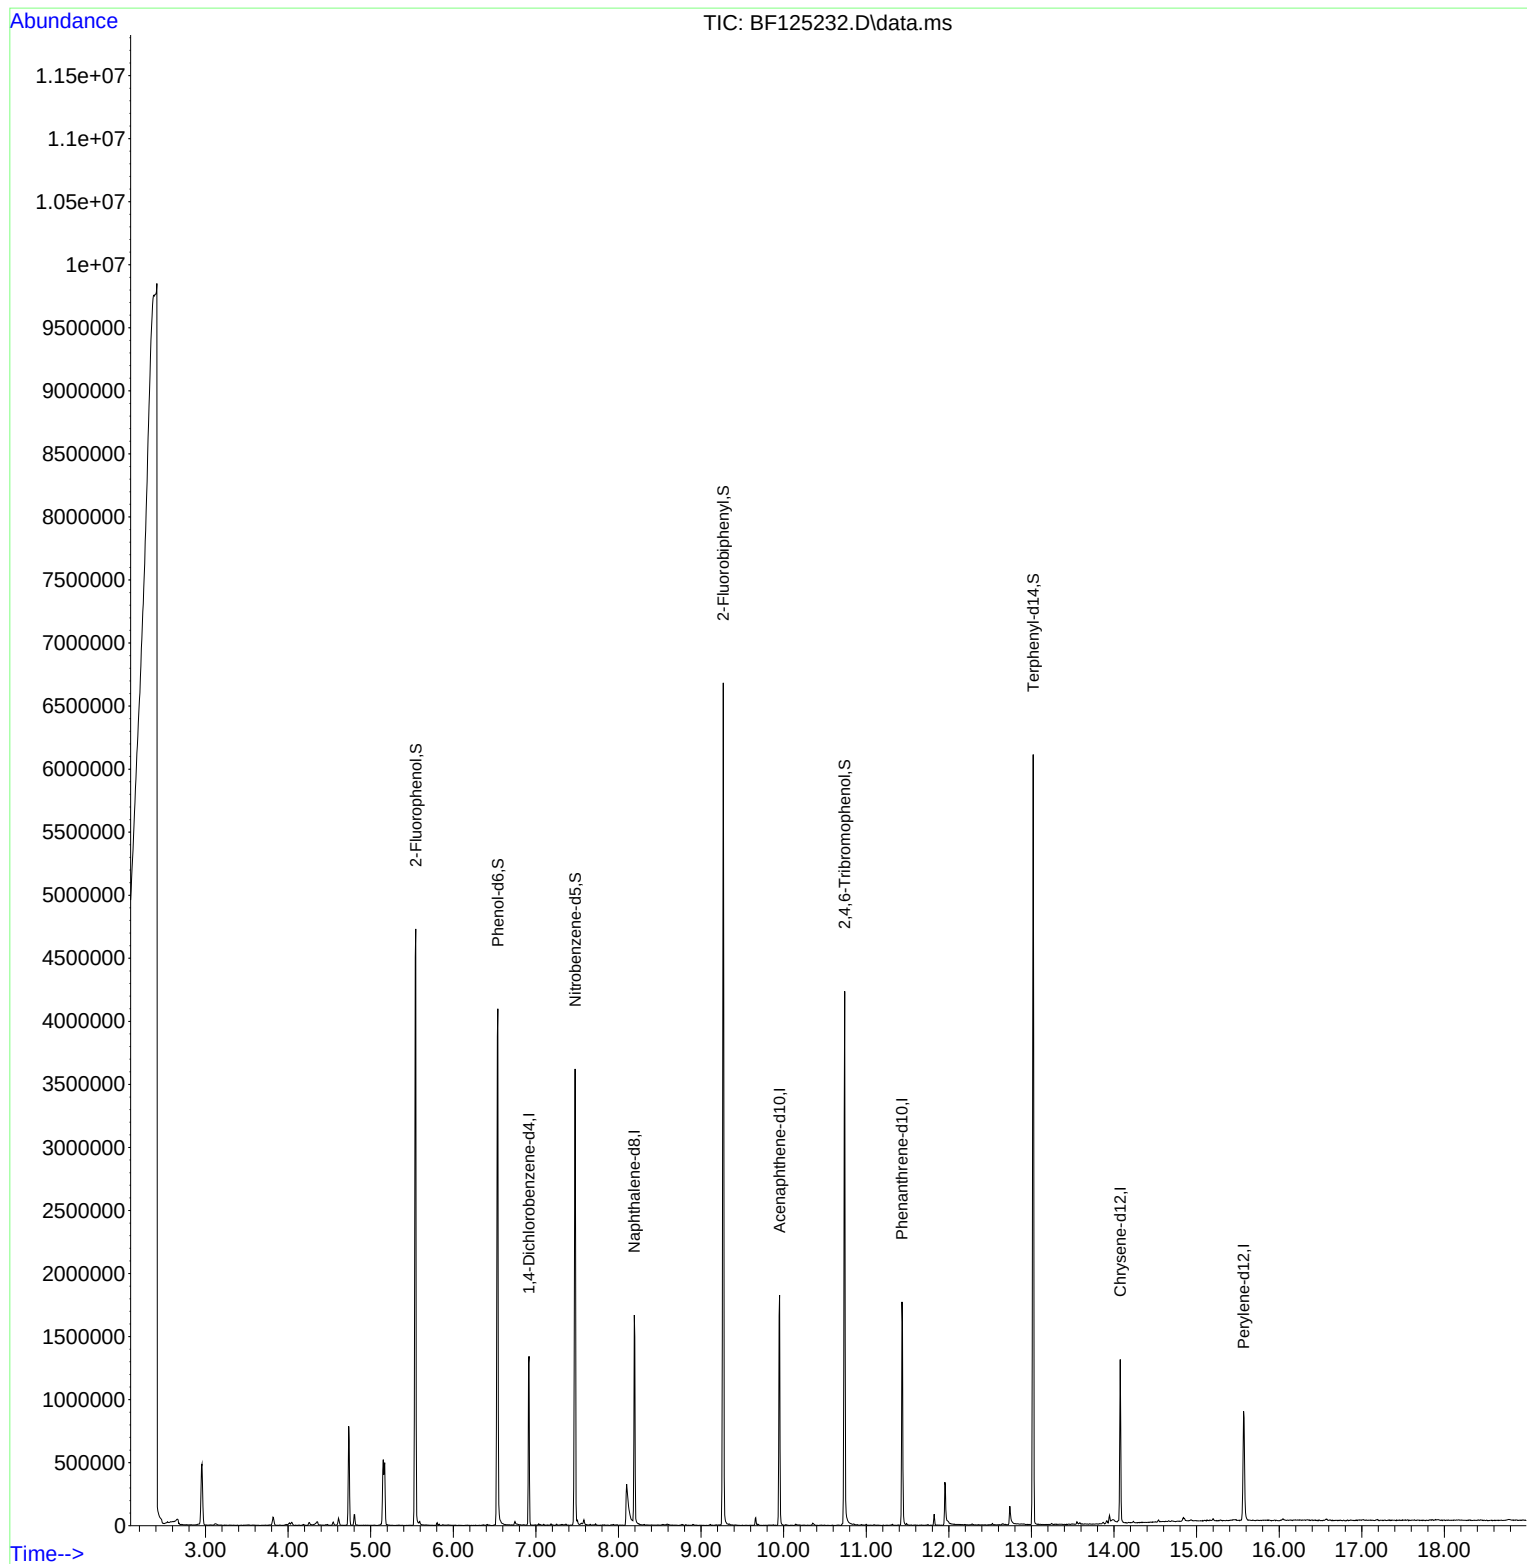


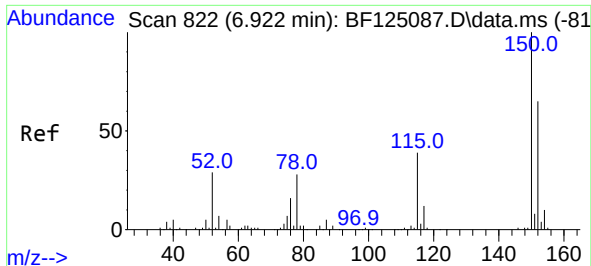

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.916 min Scan# 821
Delta R.T. 0.000 min
Lab File: BF125232.D
Acq: 26 Aug 2021 19:01




Instrument :
BNA_F
ClientSampleId :
PT-3-082421


Tgt Ion:152 Resp: 197581
Ion Ratio Lower Upper
152 100
150 151.7 117.6 176.4
115 57.5 47.1 70.7

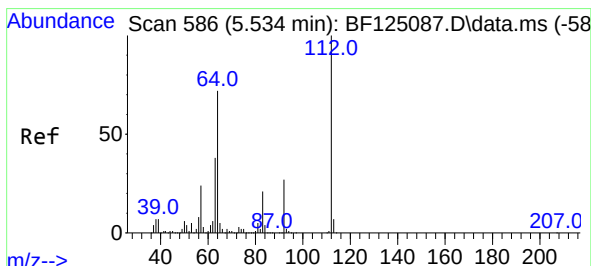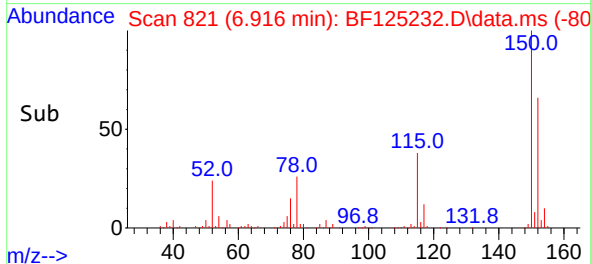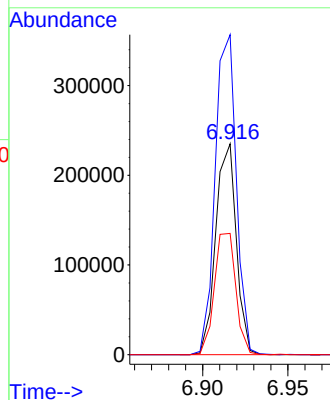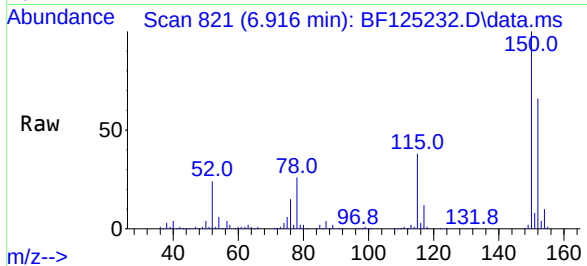

#5
2-Fluorophenol
Concen: 99.434 ng
RT: 5.546 min Scan# 588
Delta R.T. 0.018 min
Lab File: BF125232.D
Acq: 26 Aug 2021 19:01

Tgt Ion:112 Resp: 1297988
Ion Ratio Lower Upper
112 100
64 67.1 44.2 66.2#
63 34.8 26.2 39.2


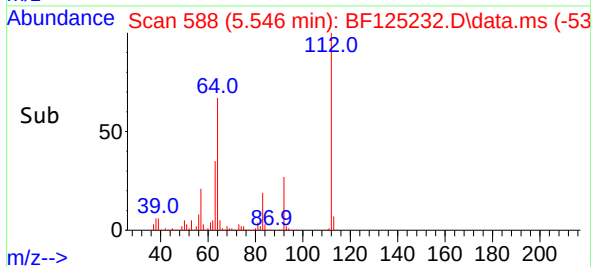
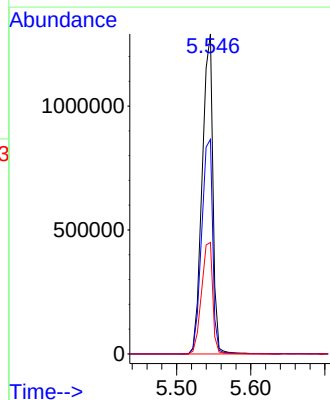
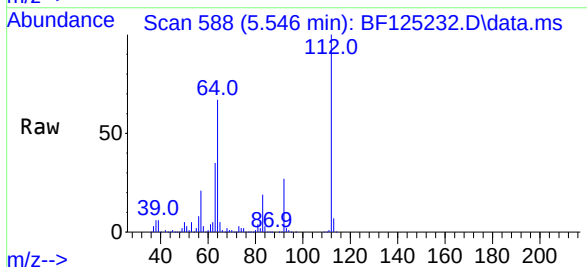


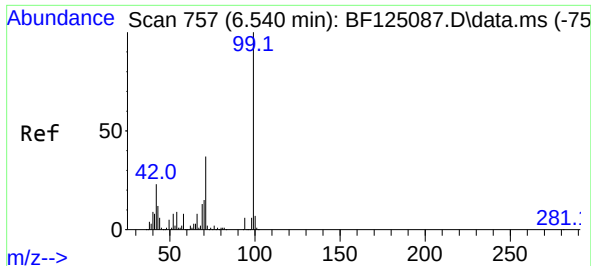

#7
Phenol-d6
Concen: 87.980 ng
RT: 6.540 min Scan# 757
Delta R.T. 0.000 min
Lab File: BF125232.D
Acq: 26 Aug 2021 19:01




Instrument :
BNA_F
ClientSampleId :
PT-3-082421


Tgt Ion: 99 Resp: 1485339
Ion Ratio Lower Upper
99 100
42 19.2 23.5 35.3#
71 33.5 25.6 38.4

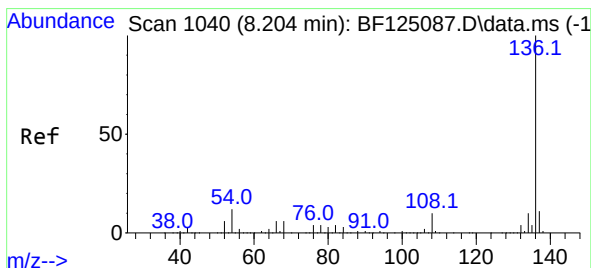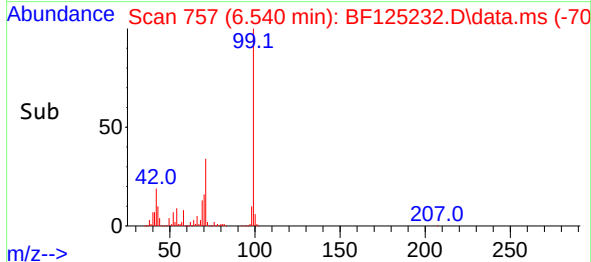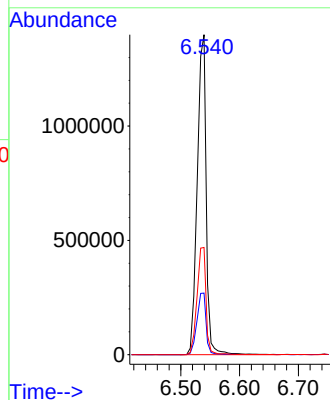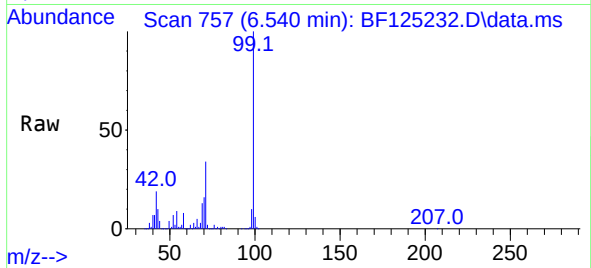

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.192 min Scan# 1038
Delta R.T. -0.006 min
Lab File: BF125232.D
Acq: 26 Aug 2021 19:01

Tgt Ion: 136 Resp: 752175
Ion Ratio Lower Upper
136 100
137 11.6 9.8 14.6
54 10.6 6.4 9.6#
68 6.8 3.3 4.9#


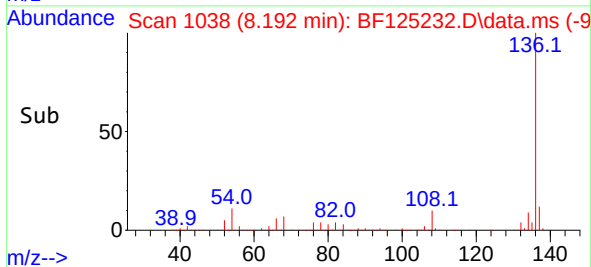
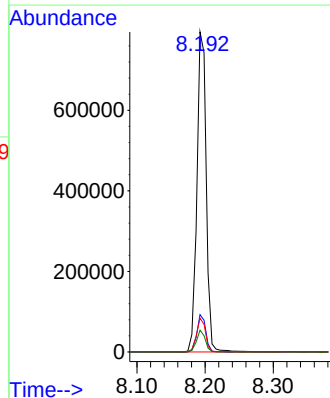
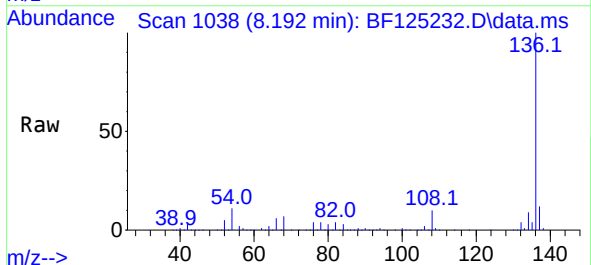


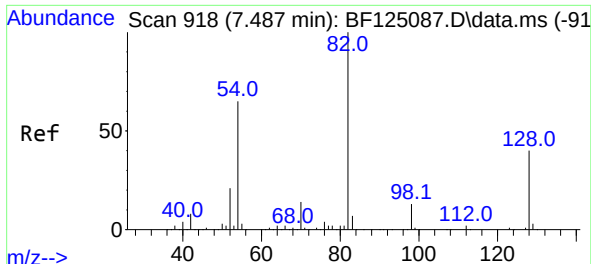

#23
Nitrobenzene-d5
Concen: 80.885 ng
RT: 7.475 min Scan# 916
Delta R.T. -0.006 min
Lab File: BF125232.D
Acq: 26 Aug 2021 19:01




Instrument :
BNA_F
ClientSampleId :
PT-3-082421


Tgt Ion: 82 Resp: 1208472
Ion Ratio Lower Upper
82 100
128 41.1 40.6 60.8
54 61.3 49.6 74.4

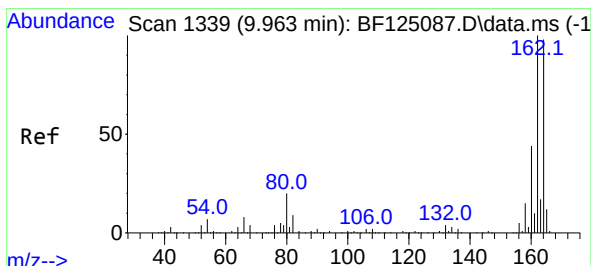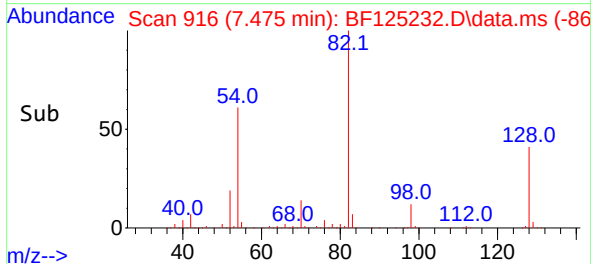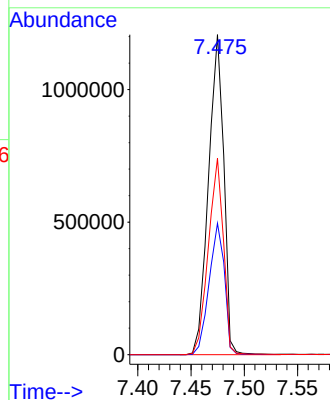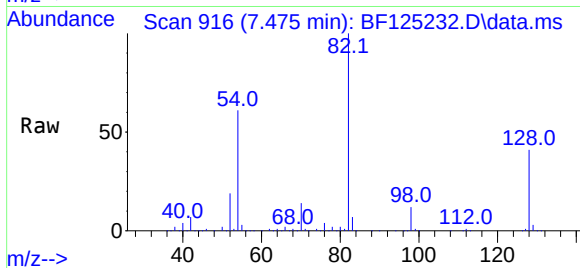

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.951 min Scan# 1337
Delta R.T. 0.000 min
Lab File: BF125232.D
Acq: 26 Aug 2021 19:01

Tgt Ion: 164 Resp: 398894
Ion Ratio Lower Upper
164 100
162 101.4 81.3 121.9
160 45.5 38.0 57.0


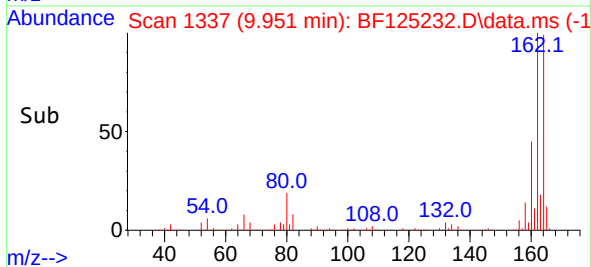
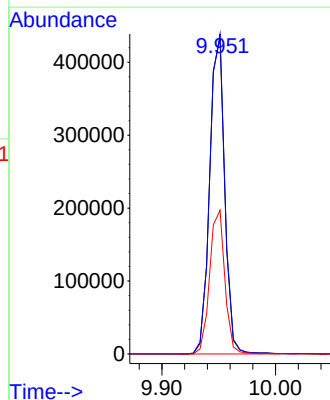
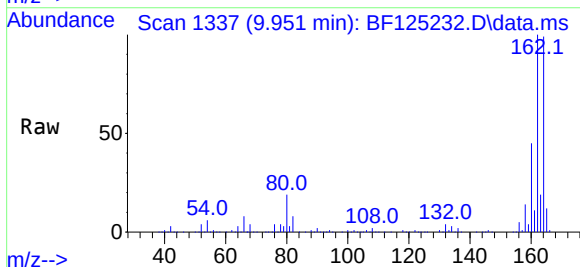


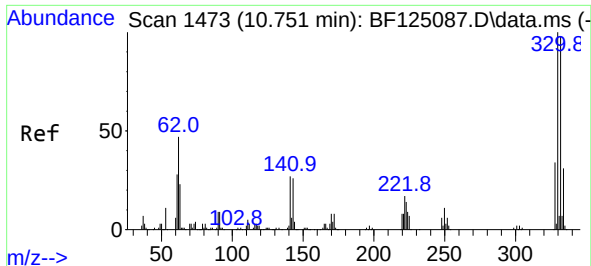

#42
2,4,6-Tribromophenol
Concen: 132.766 ng
RT: 10.739 min Scan# 1471
Delta R.T. 0.000 min
Lab File: BF125232.D
Acq: 26 Aug 2021 19:01




Instrument :
BNA_F
ClientSampleId :
PT-3-082421


Tgt Ion:330 Resp: 528653
Ion Ratio Lower Upper
330 100
332 95.8 76.2 114.4
141 29.3 44.6 66.8#

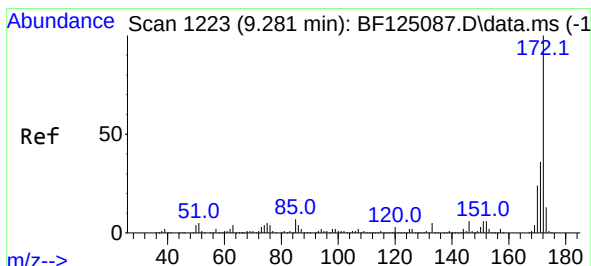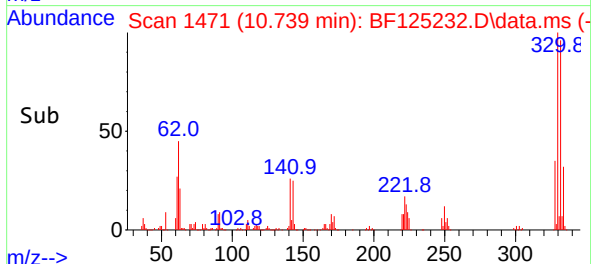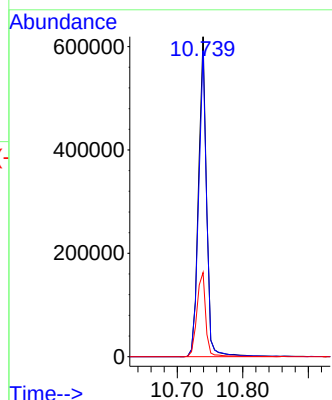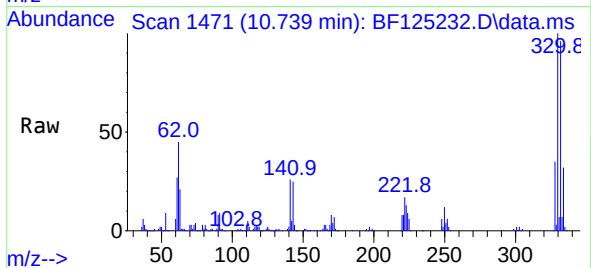

#45
2-Fluorobiphenyl
Concen: 74.282 ng
RT: 9.269 min Scan# 1221
Delta R.T. -0.006 min
Lab File: BF125232.D
Acq: 26 Aug 2021 19:01

Tgt Ion:172 Resp: 2126002
Ion Ratio Lower Upper
172 100
171 35.9 26.5 39.7
170 25.0 18.8 28.2


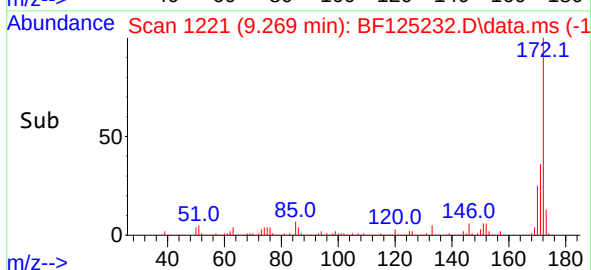
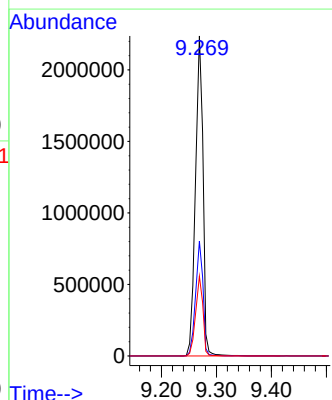
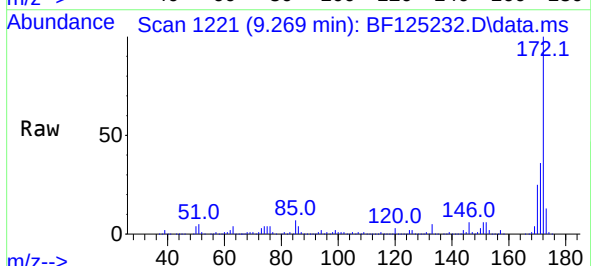


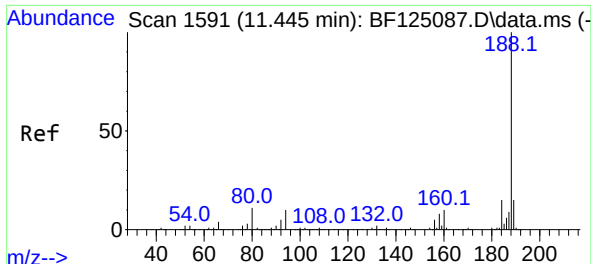

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.433 min Scan# 1589
Delta R.T. -0.006 min
Lab File: BF125232.D
Acq: 26 Aug 2021 19:01




Instrument :
BNA_F
ClientSampleId :
PT-3-082421


Tgt Ion:188 Resp: 687235
Ion Ratio Lower Upper
188 100
94 10.0 6.7 10.1
80 11.2 7.5 11.3

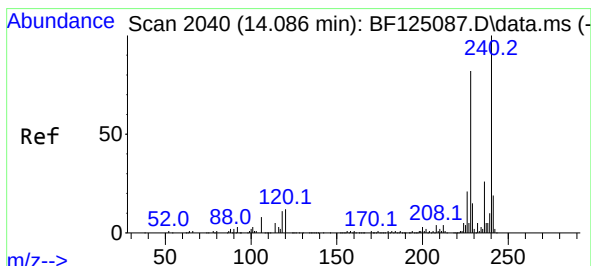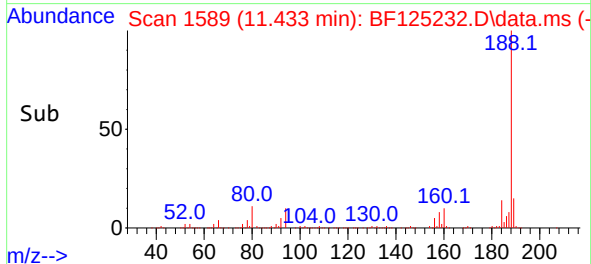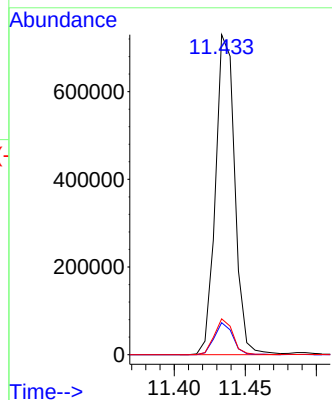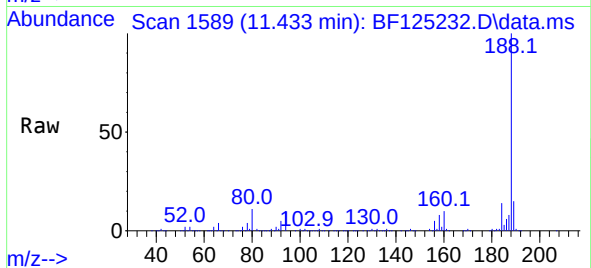

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.074 min Scan# 2038
Delta R.T. -0.006 min
Lab File: BF125232.D
Acq: 26 Aug 2021 19:01

Tgt Ion:240 Resp: 423134
Ion Ratio Lower Upper
240 100
120 11.3 10.8 16.2
236 26.8 21.6 32.4


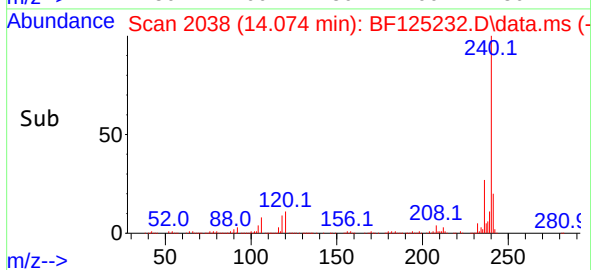
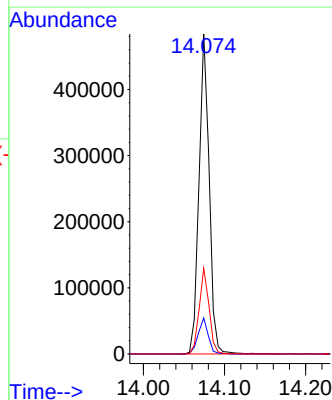
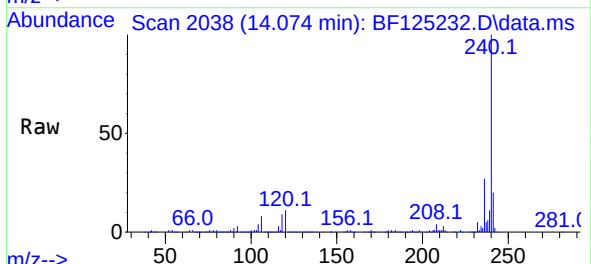


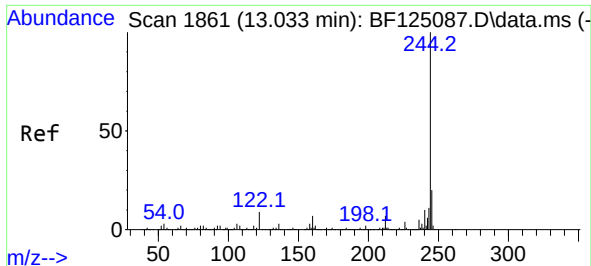

#79
 Terphenyl-d14
 Concen: 82.007 ng
 RT: 13.022 min Scan# 1859
 Delta R.T. 0.000 min
 Lab File: BF125232.D
 Acq: 26 Aug 2021 19:01

Instrument :
 BNA_F
 ClientSampleId :
 PT-3-082421

Tgt Ion:244 Resp: 2178148
 Ion Ratio Lower Upper
 244 100
 212 6.7 5.9 8.9
 122 9.2 9.0 13.4

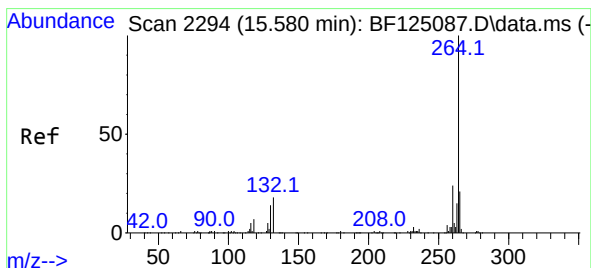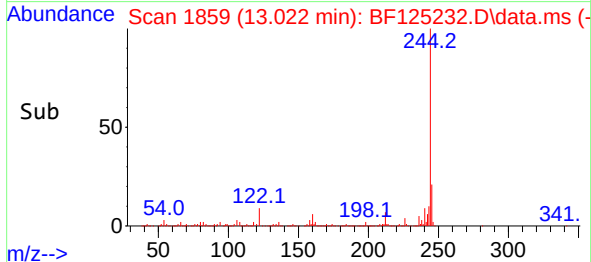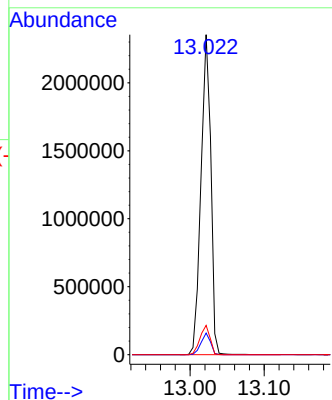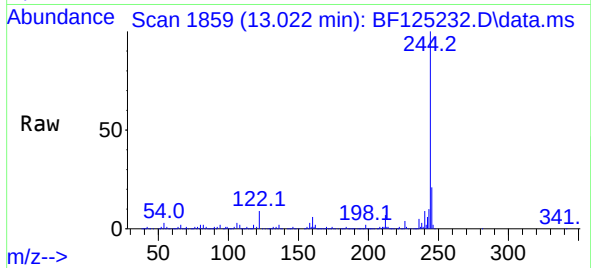

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.568 min Scan# 2292
 Delta R.T. -0.006 min
 Lab File: BF125232.D
 Acq: 26 Aug 2021 19:01

Tgt Ion:264 Resp: 418696
 Ion Ratio Lower Upper
 264 100
 260 25.2 19.6 29.4
 265 22.2 17.2 25.8

