

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082621\
 Data File : BF125222.D
 Acq On : 26 Aug 2021 12:15
 Operator : JU/CG
 Sample : PB138680BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB138680BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125222.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.263	21	30	37	rVB	141490	202985	3.09%	0.476%
2	5.540	582	587	590	rBV	5941047	6399056	97.51%	14.991%
3	6.539	751	757	760	rBV	5391610	6175423	94.10%	14.467%
4	6.916	817	821	824	rBV	1541880	1345186	20.50%	3.151%
5	7.475	911	916	919	rBV	3917375	4087297	62.28%	9.575%
6	8.198	1034	1039	1042	rBV	1866015	1752332	26.70%	4.105%
7	9.269	1216	1221	1225	rBV	6685370	6562483	100.00%	15.373%
8	9.951	1333	1337	1347	rVB	2144649	1872242	28.53%	4.386%
9	10.739	1466	1471	1474	rBV	4444263	3936693	59.99%	9.222%
10	11.439	1586	1590	1597	rBV	1871685	1762031	26.85%	4.128%
11	13.027	1855	1860	1863	rBV	5966614	5968778	90.95%	13.983%
12	14.074	2034	2038	2048	rVB	1378028	1320348	20.12%	3.093%
13	15.574	2287	2293	2306	rVB2	930516	1302390	19.85%	3.051%




Sum of corrected areas: 42687244

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082621\
Data File : BF125222.D
Acq On : 26 Aug 2021 12:15
Operator : JU/CG
Sample : PB138680BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138680BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

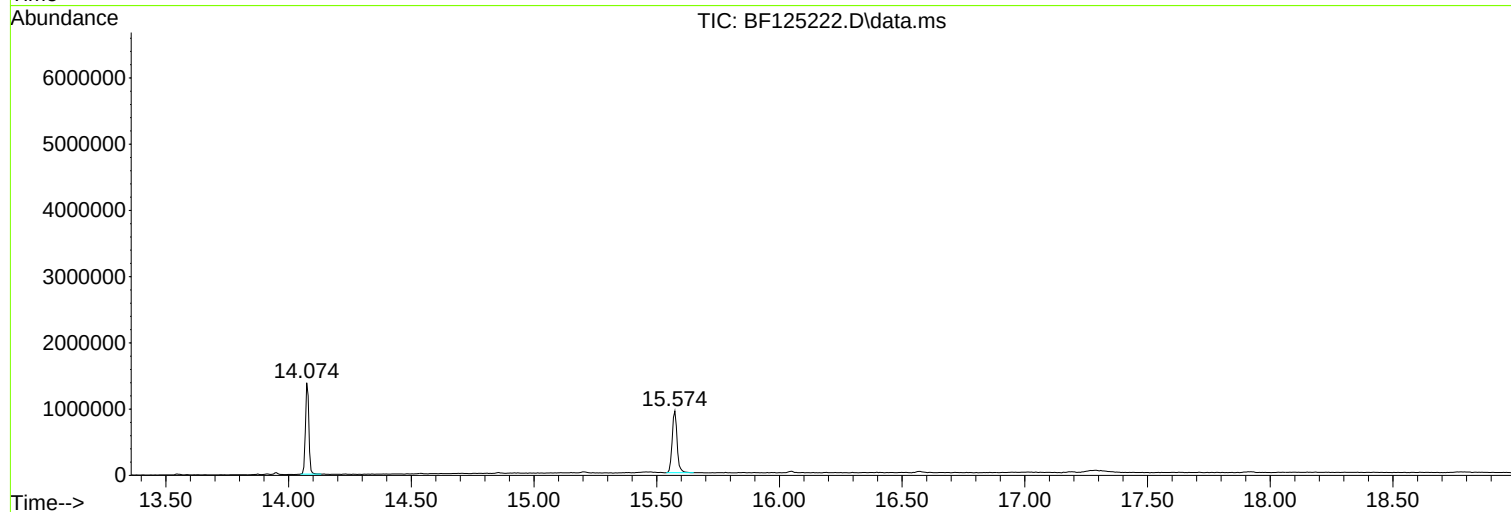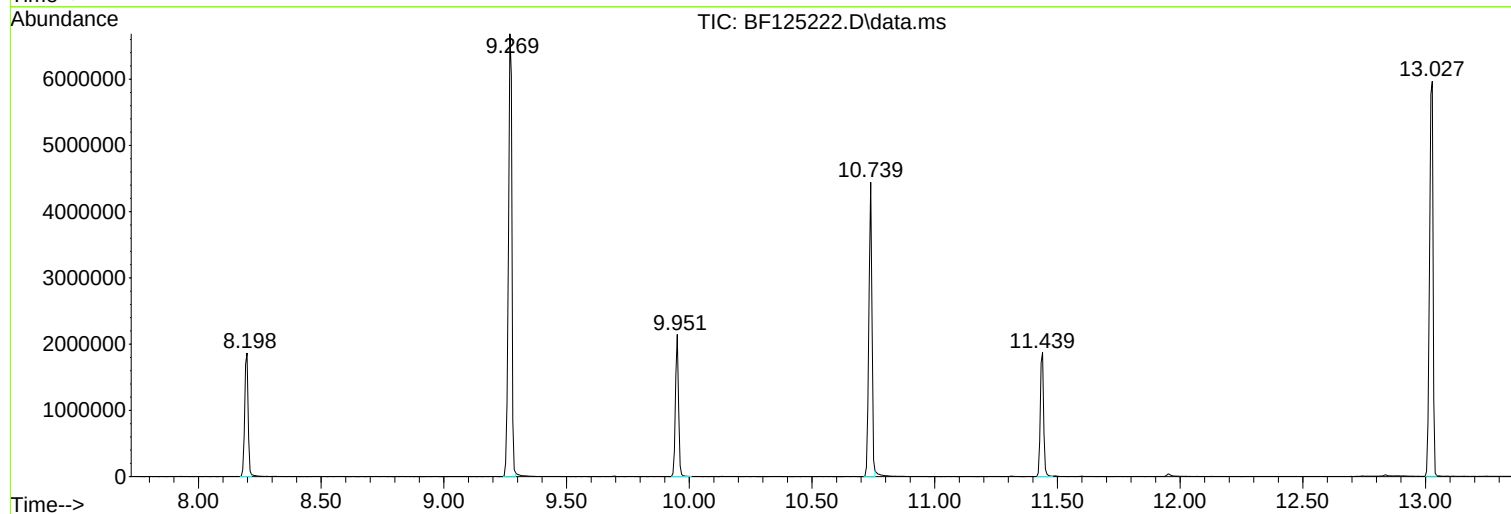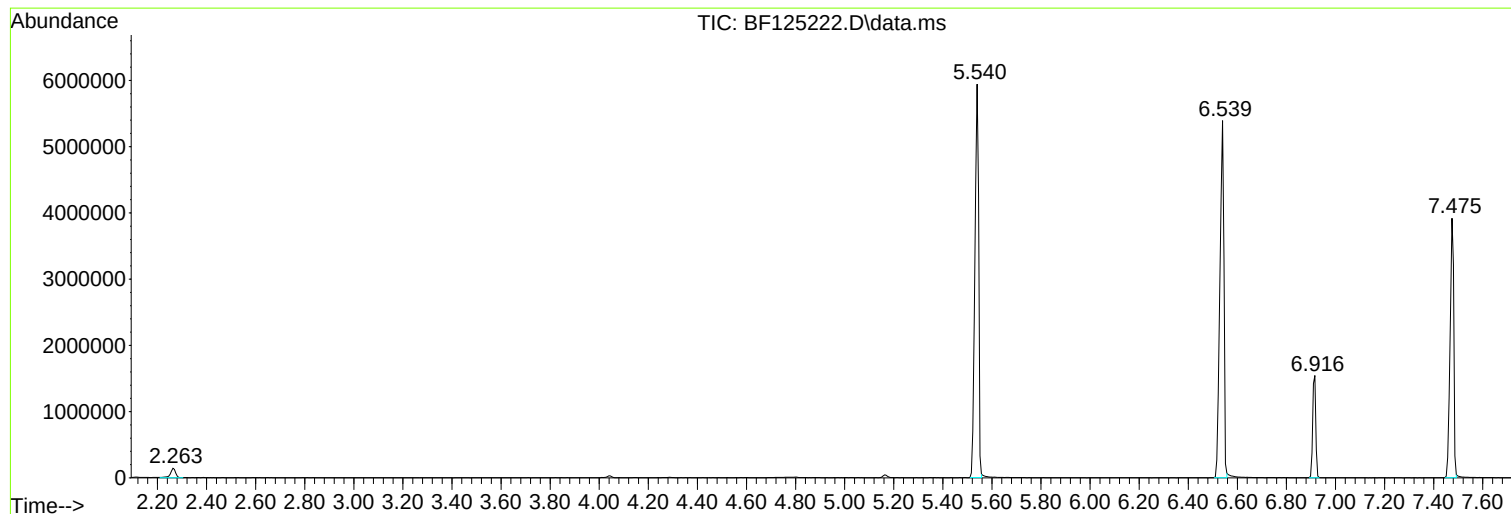

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082621\
Data File : BF125222.D
Acq On : 26 Aug 2021 12:15
Operator : JU/CG
Sample : PB138680BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138680BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.263	3.02 ng	202985	1,4-Dichlorobenzene-d4	6.916

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2		2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3		1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	37
4		3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	25
5		3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	17

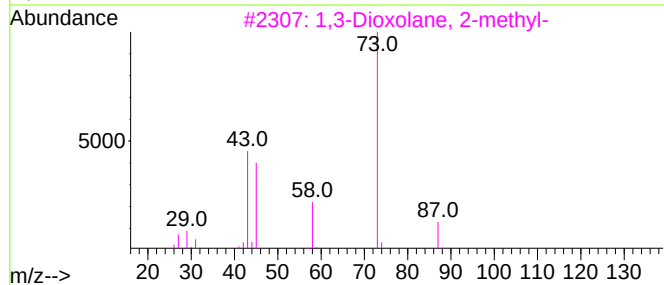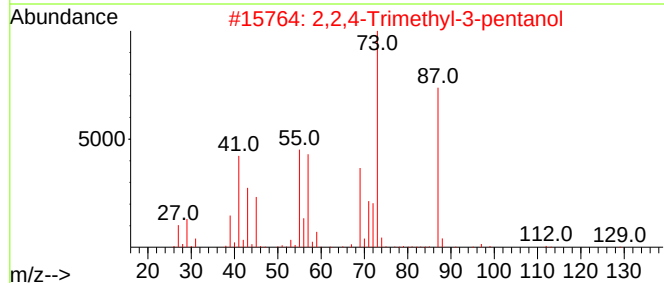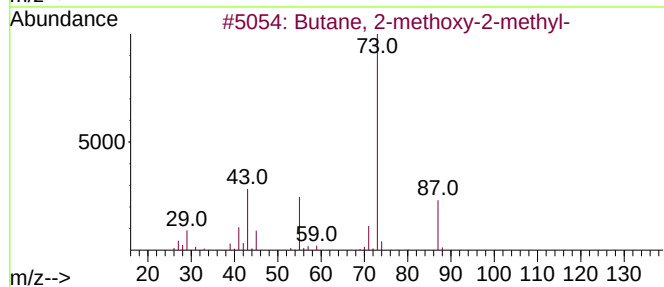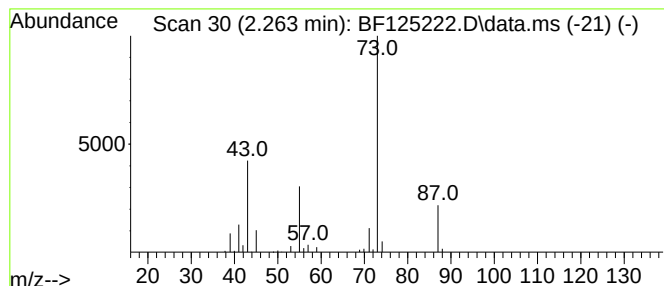

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082621\
Data File : BF125222.D
Acq On : 26 Aug 2021 12:15
Operator : JU/CG
Sample : PB138680BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138680BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.263	3.0	ng	202985	1	6.916	1345190	20.0