

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082621\
 Data File : BF125227.D
 Acq On : 26 Aug 2021 16:03
 Operator : JU/CG
 Sample : PB138720BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB138720BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125227.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.287	27	34	41	rVB	150564	220260	2.67%	0.430%
2	5.545	582	588	591	rBV	6283173	7023350	85.28%	13.726%
3	6.539	751	757	760	rBV	5644632	6941110	84.28%	13.565%
4	6.910	817	820	824	rBV	1764169	1501234	18.23%	2.934%
5	7.475	910	916	919	rBV	4256442	4589998	55.73%	8.970%
6	8.192	1034	1038	1042	rBV	2082779	2000300	24.29%	3.909%
7	9.269	1216	1221	1225	rBV	7390246	7692794	93.40%	15.034%
8	9.951	1332	1337	1340	rBV	2515468	2222936	26.99%	4.344%
9	10.739	1465	1471	1474	rBV	5363979	4996019	60.66%	9.764%
10	11.439	1585	1590	1597	rBV	2385880	2288209	27.78%	4.472%
11	13.027	1855	1860	1863	rBV	8235505	8236060	100.00%	16.096%
12	14.080	2034	2039	2048	rVB	1843624	1841862	22.36%	3.600%
13	15.574	2287	2293	2304	rBV2	1070382	1615314	19.61%	3.157%




Sum of corrected areas: 51169446

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082621\
Data File : BF125227.D
Acq On : 26 Aug 2021 16:03
Operator : JU/CG
Sample : PB138720BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138720BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

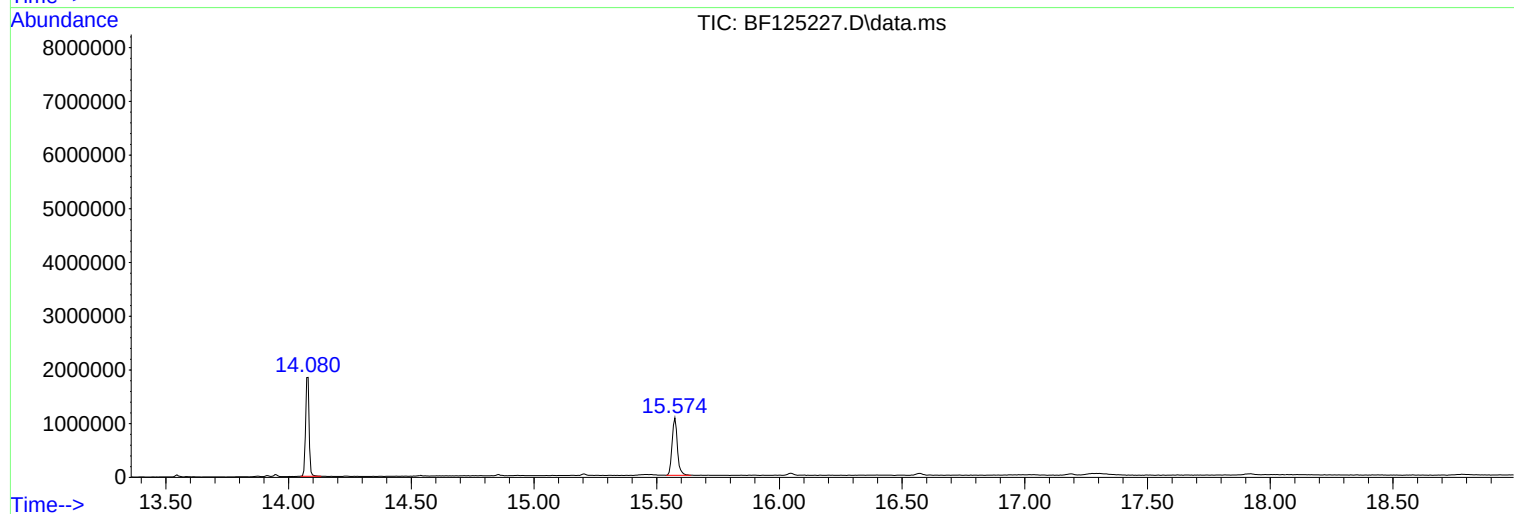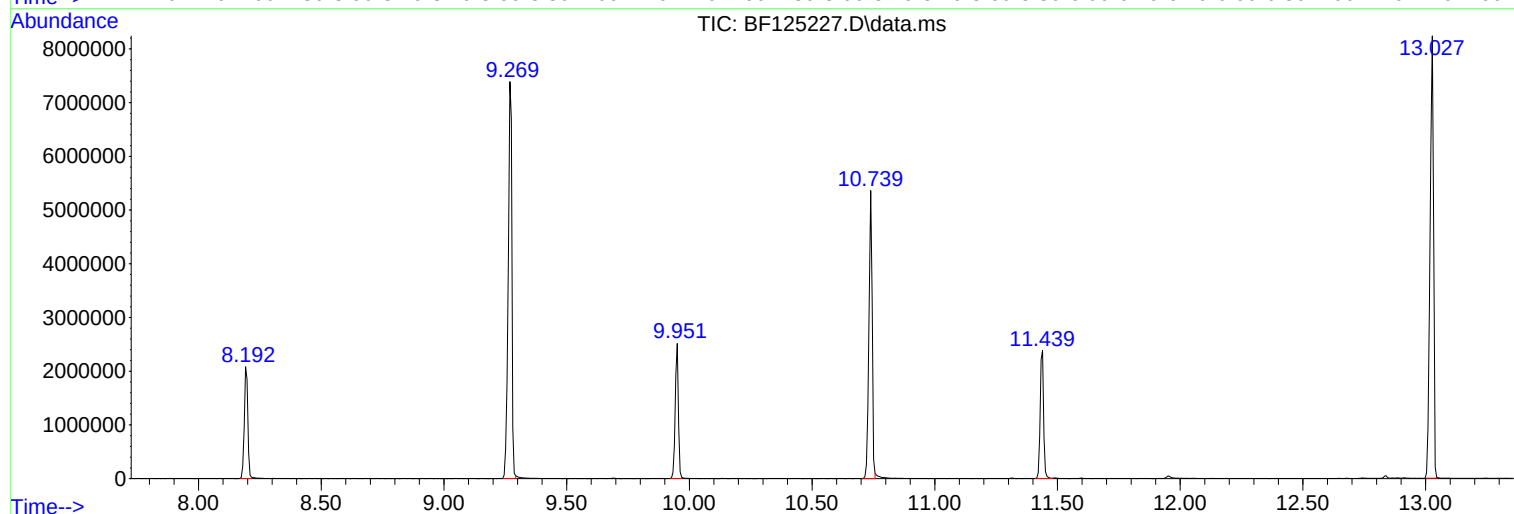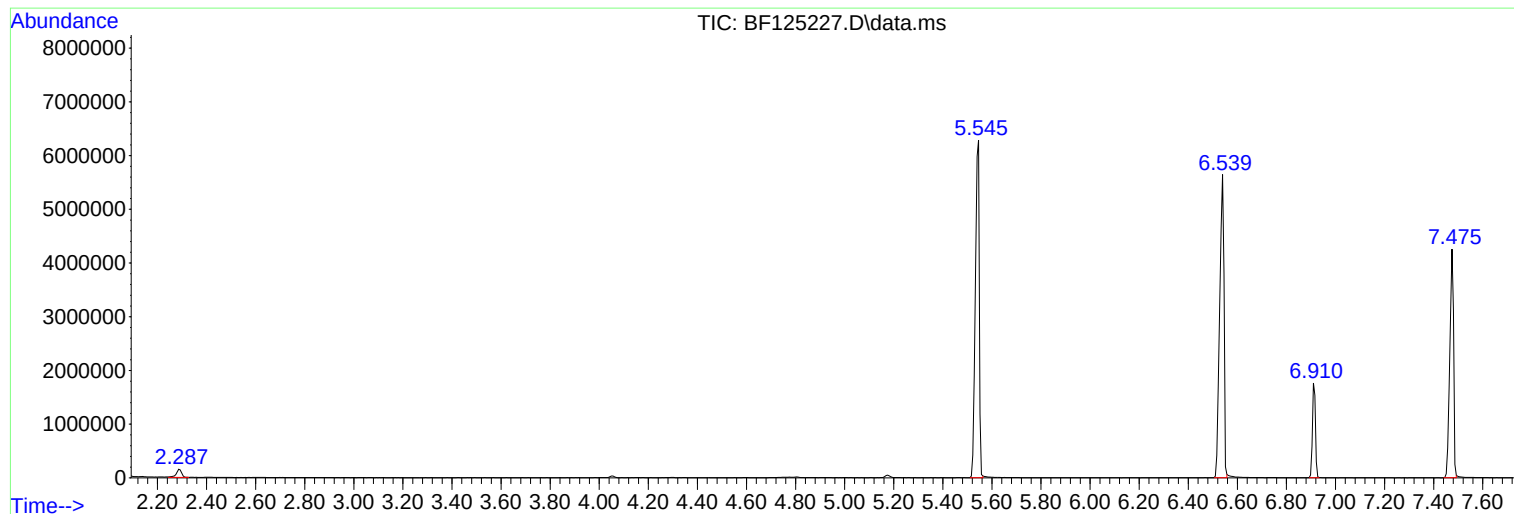

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082621\
Data File : BF125227.D
Acq On : 26 Aug 2021 16:03
Operator : JU/CG
Sample : PB138720BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138720BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.287	2.93 ng	220260	1,4-Dichlorobenzene-d4	6.910

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	72
2			3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	23
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	9
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
5			N-Ethylformamide	73	C3H7NO	000627-45-2	9

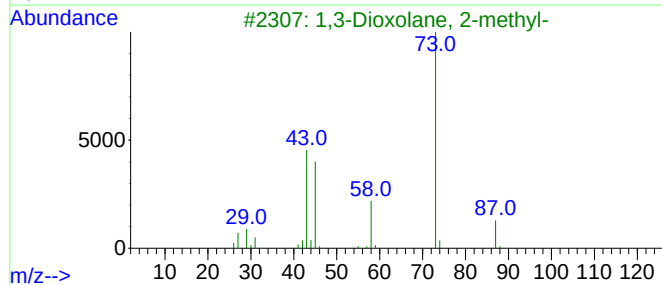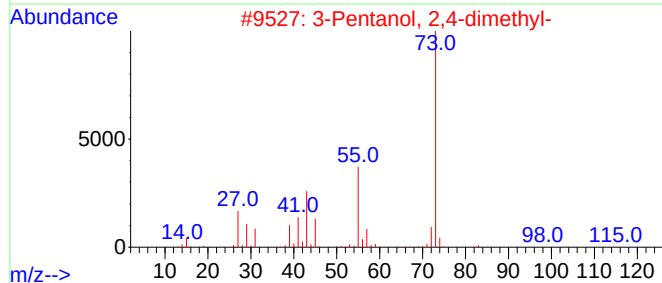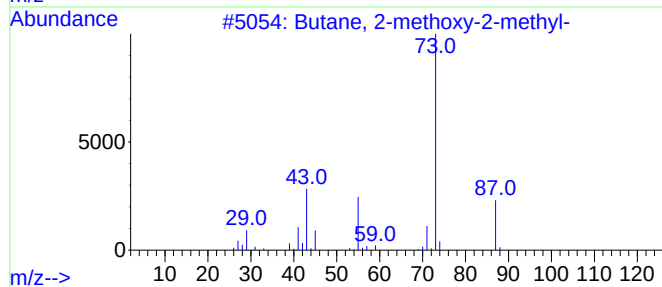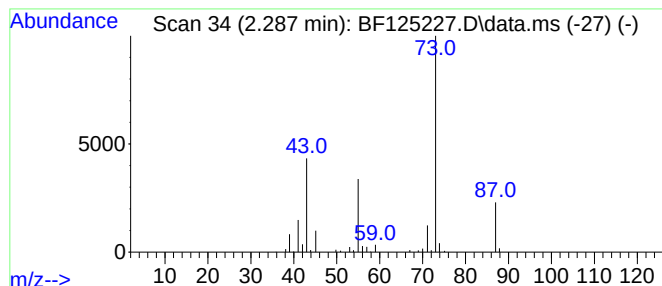

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082621\
Data File : BF125227.D
Acq On : 26 Aug 2021 16:03
Operator : JU/CG
Sample : PB138720BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138720BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.287	2.9	ng	220260	1	6.910	1501230	20.0