
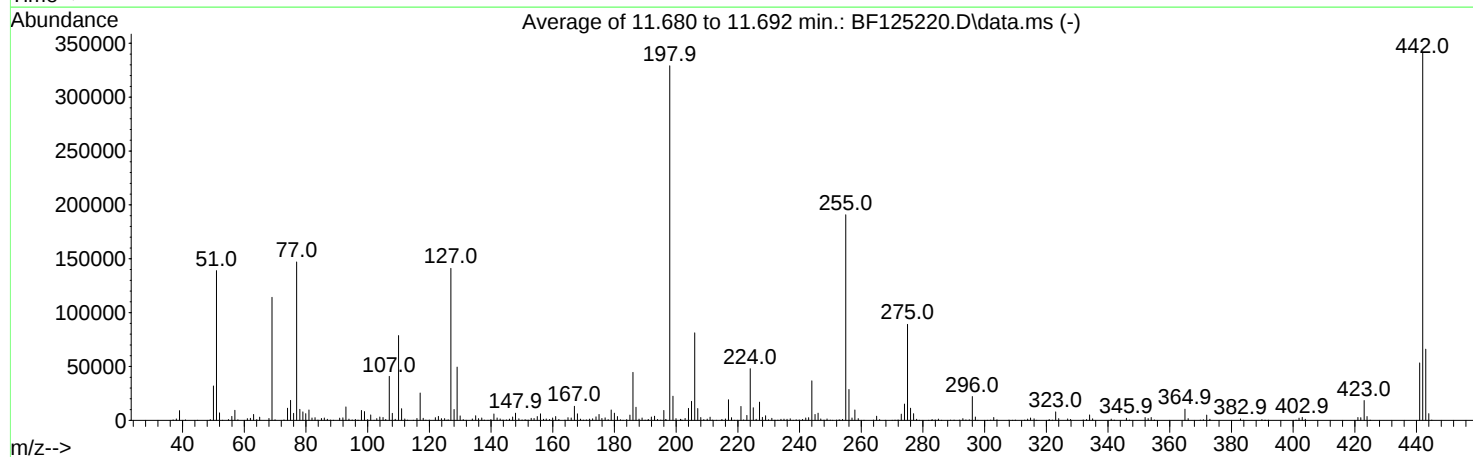


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082621\
 Data File : BF125220.D
 Acq On : 26 Aug 2021 11:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 24 12:39:21 2021

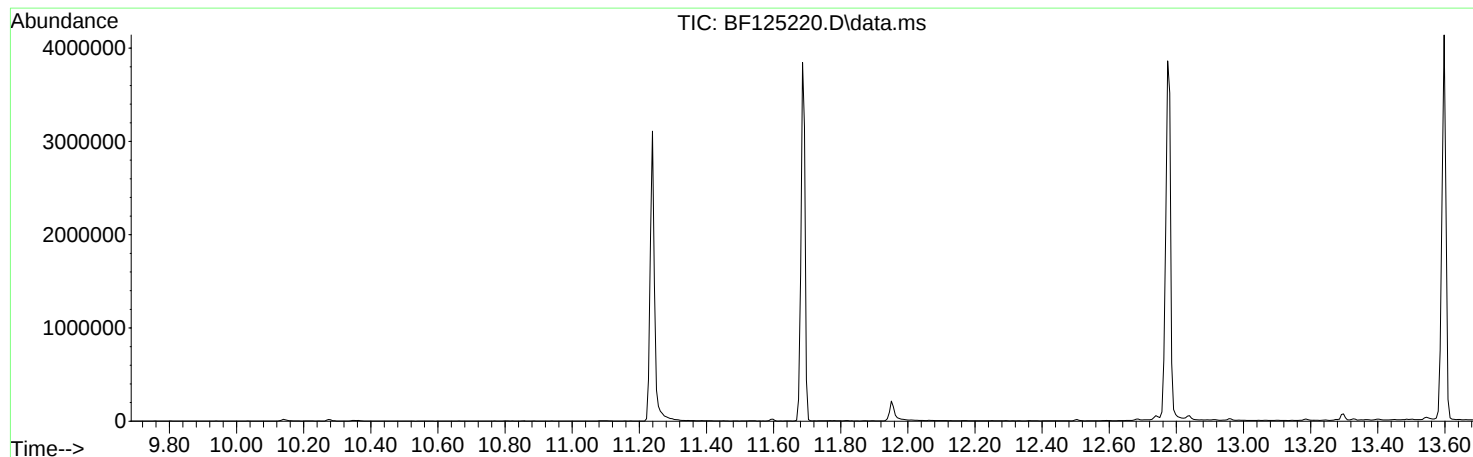

AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	138995	PASS
68	69	0.00	2	1.6	1794	PASS
69	198	0.00	100	34.7	114211	PASS
70	69	0.00	2	0.6	664	PASS
127	198	10	80	42.9	141120	PASS
197	198	0.00	2	0.1	253	PASS
198	198	100	100	100.0	329045	PASS
199	198	5	9	6.8	22499	PASS
275	198	10	60	27.1	89187	PASS
365	198	1	100	3.2	10449	PASS
441	198	0.01	100	16.2	53336	PASS
442	442	50	100	100.0	341440	PASS
443	442	15	24	19.4	66107	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/26/2021	BNA_F	<u>BF125220.D</u>
Compound Name	Response	Retention Time
DDT	726032	13.59
DDD	13330	13.29
DDE	2333	12.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15663	741695	2.11

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082621\
 Data File : BF125220.D
 Acq On : 26 Aug 2021 11:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 26 12:56:40 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 12:39:21 2021
 Response via : Initial Calibration

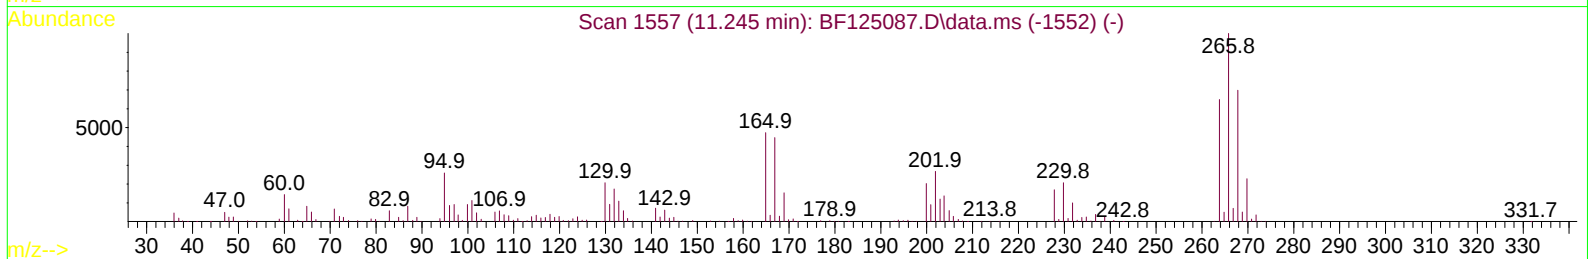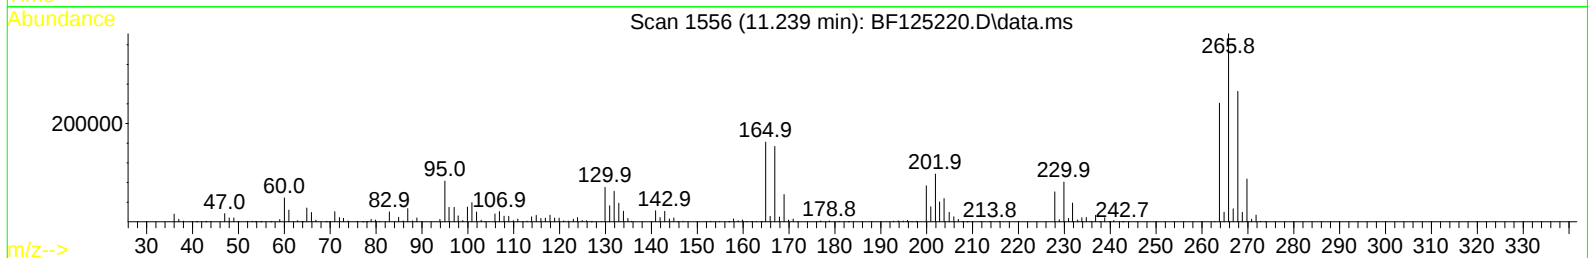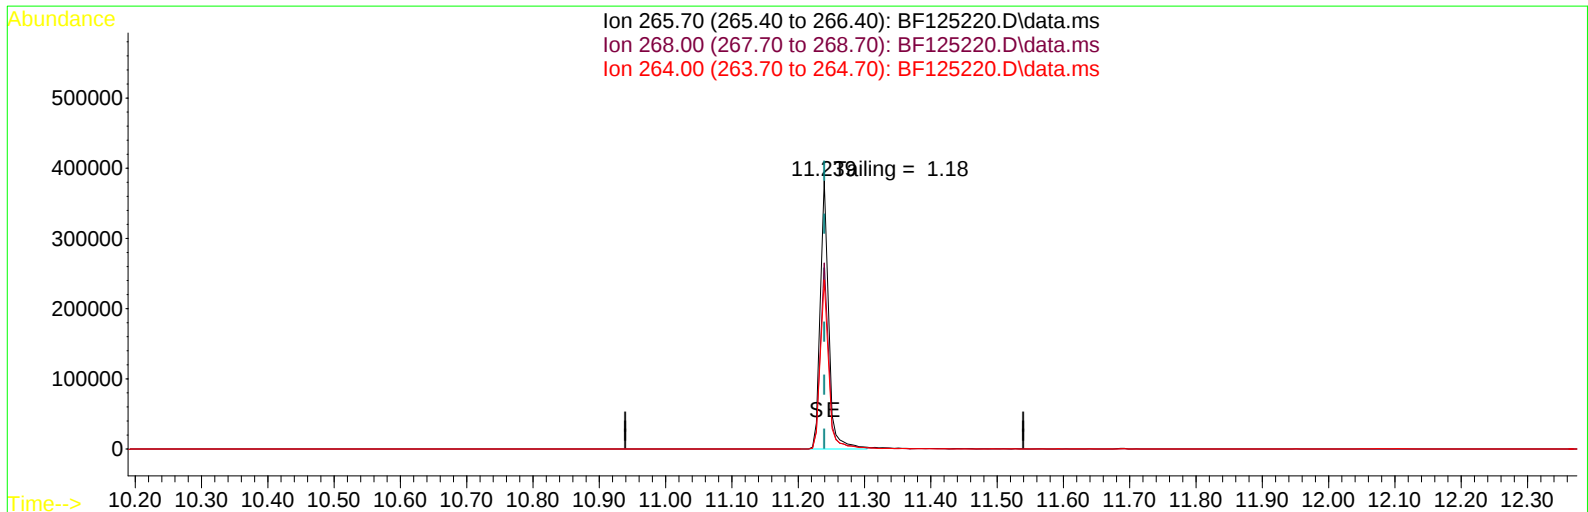

TIC: BF125220.D\data.ms

(70) Pentachlorophenol (C)

11.239min (0.000) 40577.08 ng




response 347709

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	69.35
264.00	69.90	63.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082621\
 Data File : BF125220.D
 Acq On : 26 Aug 2021 11:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 26 12:56:40 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 24 12:39:21 2021
 Response via : Initial Calibration

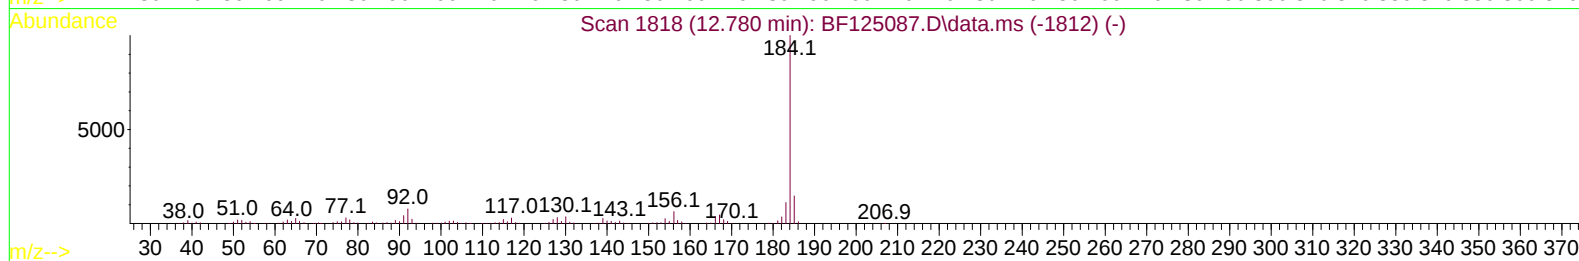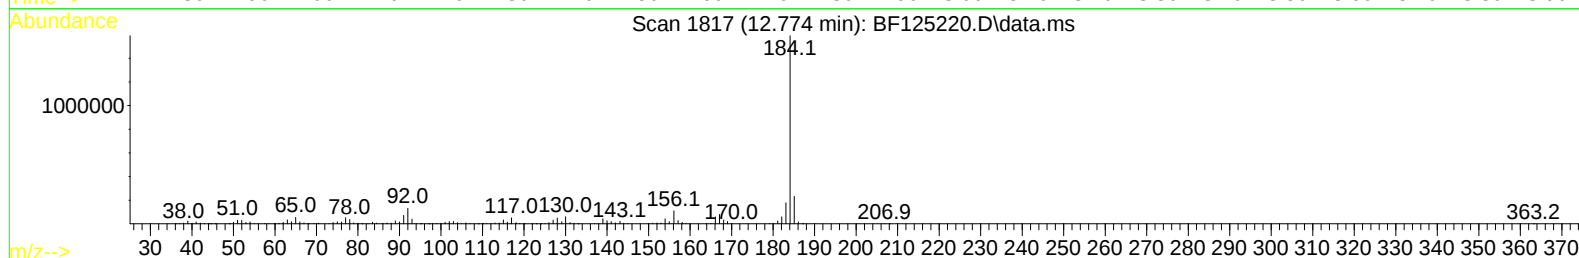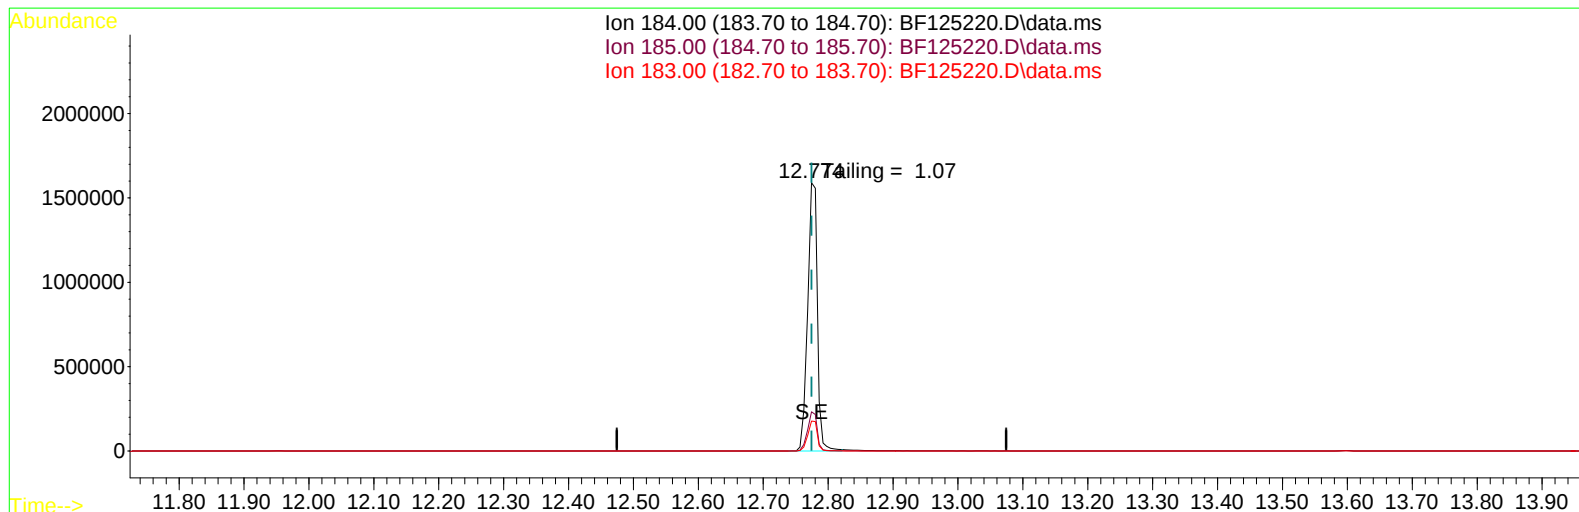

TIC: BF125220.D\data.ms

(77) Benzidine

12.774min (+ 0.000) 0.00 ng

response 1669055

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.64
183.00	10.10	11.14
0.00	0.00	0.00